Sri Venkateswara Institute of Medical Sciences (SVIMS), Tirupati

Quality & Patient Safety

It is envisaged to **transform SVIMS into a "High Reliability Organization"** and **an "Accountable Health System".** Towards that path of transformation & global repute, the Director / Vice Chancellor, on behalf of the institute, has laid out a road-map of value based health care. A major step towards this value proposition is emphasis on quality and patient safety as drivers of health system performance. To drive the performance, a programme of **SVIMS Quality Council (SQC)** is commissioned by the Director for iterative self improvement. Cataloguing, reporting, analyzing and learning from errors has become the lynchpin for quality improvement in health care.

The **SQC** planning process resulted in the formation of nine focus groups and four core groups of workforce consisting of Doctors, Nurses, Administrators, Allied health staff and various other types of employees representing all segments of health system. The focus groups were formed to address: Emergency services, Never events, Medication safety, workforce/workplace safety, fire safety / disaster management, Radiation safety, Hospital Acquired Infections, Blood / injection safety and operating room / interventional areas safety. The four core groups will find sustainable solutions through – Root cause analysis of sentinel events, check lists / communications, accreditations and hospitality services.

Domains of SVIMS Quality Council

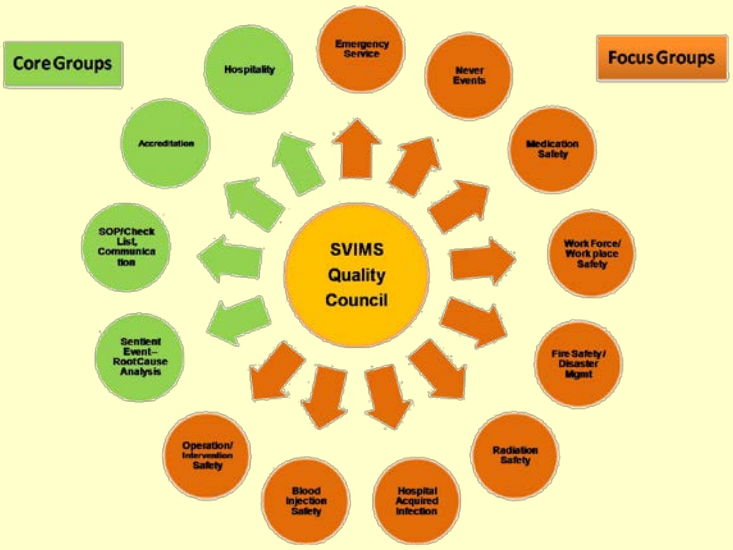

The groups work, on monthly deliverables and share barriers / successes, so as to find culturally competent and substantively sound sustainable solutions. The ultimate goal is to deliver **"Right Care,** to the **Right Patient** by the **Right Teams** in the **Right Place** at the **Right Time**…. ***Every Time***".

PDSA Cycle for Quality Improvement

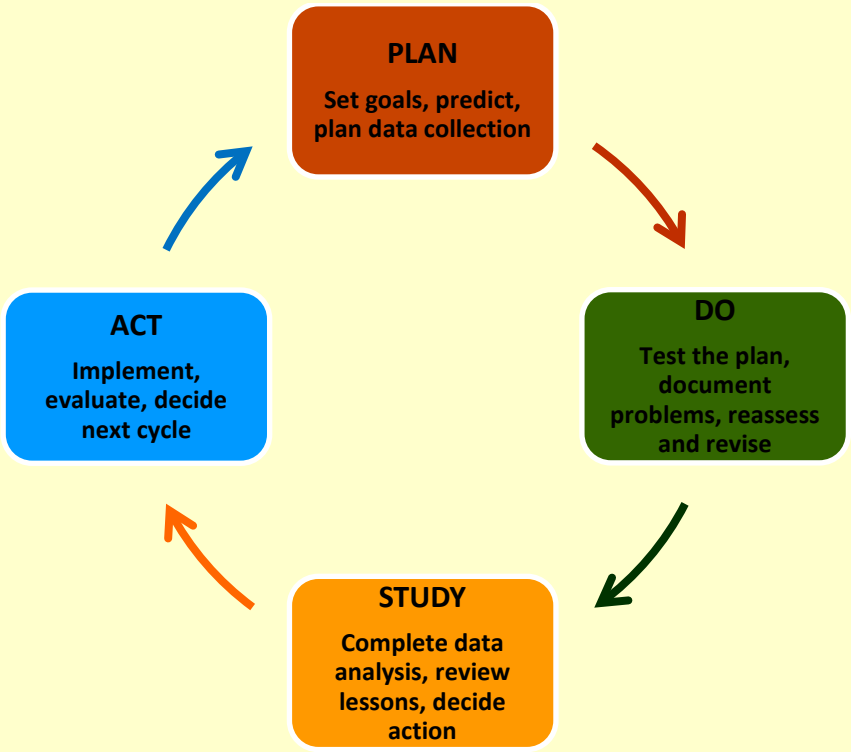

At SVIMS, a modified PDSA (Plan, Do, Study, Act) cycle is implemented and followed, during & between monthly SQC meetings. This is termed 'Rapid Cycle Bidirectional Learning' as shown below:

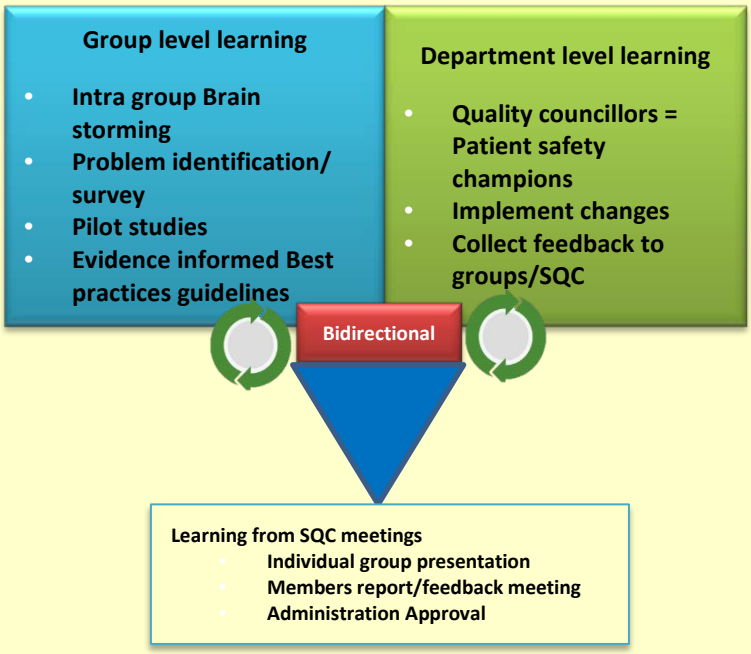

This is conceived as a two month cycle of Intra-group learning, Department level learning & monthly SQC meetings.

Tools of Trade

In order to empower ever healthcare worker and to measure performance against the set goals, SVIMS has developed several Tools of the Trade and analytics. One major tool & process is “Structured Mortality & Morbidity (M&M) Review”.

a) Structured M&M format

Structure for M&M

RCA	Categorization		QI Plan
	Preventive harm	Yes	with GANTT Chart
	Patient disease	yes	
	System issue	no	
	Human factor	no	
	Knowledge deficit	None	
	Cognitive dissonance	None	
	Delay in diagnosis	yes	
	Delay in treatment	No	
	Delay in escalation of treatment	Yes	
	Error in technique	No	
	Error in treatment	No	
	Communication gap	No	
	Policy issue	None	
	People issue	None	
	Team issue	None	

SVIMS Mortality & Morbidity (M&M) Review
"Safe Practices Save Lives"

- **Until 2015**
  - monthly/ Bimonthly hospital wide mortality meetings
    - 4 cases presented (2 medical/ 2 surgical)
- **December 2015**
  - SVIMS Quality Council (SQC) formed. RCA, patient safety education & categorization of root causes started in practice.
  - Order for weekly department-wide M&M; promulgated:
- **April 2016**
  - Structure for M&M defined: RCA → categorization of contributing factors → QI plan
- **July 2016:**
  - Voluntary public reporting of quality/patient safety metrics in website
- **June 2017:**
  - Daily mortality review with assignments to responsible departments for immediate review & remedial actions.
- **January 2018:**
  - Monthly analysis of death cohorts: Pranadana cases; NTRVSS cases for further "systems redesign" & "Human factor engineering".

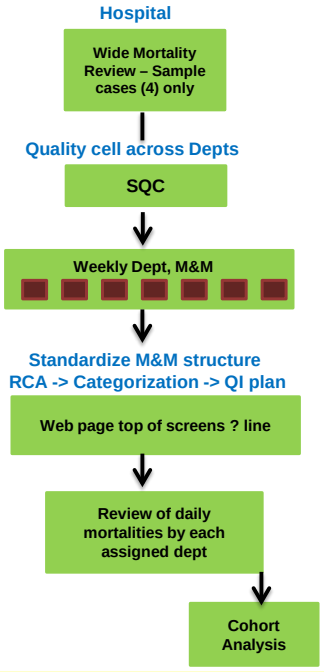

Development of Tools & Analytics

Tools of Trade	Analytics (Pre and Post intervention)
➢ Check lists, SOPs ➢ Rounding tool ➢ Structured hand offs ➢ Structured communication tools ➢ Real case studies/ Scenarios ➢ Simulation models ➢ Root cause analysis models	➢ Hospital patient safety survey ➢ Staff competence, knowledge and satisfaction questionnaires ➢ Mutual performance assessment ➢ Measurable patient related outcomes ➢ Patient and care taker's feedback forms

b) Root Cause Analysis in Health Care: Tools and Techniques , FIFTH EDITION, Joint Commission Resources, Joint Commission International
https://www.jcrinc.com/assets/1/14/EBRCA15Sample.pdf

c) In addition to outlining its unique Quality & Patient Safety initiative through 'SQC', SVIMS took a major step on June 12th 2016, in declaring its accountability & transparency in quality improvement and patient-centered care by announcing voluntary public reporting in four domains on 7/12/16 to start with, and reporting of many other areas to follow sequentially.

The four areas were:

1. **Code Blue**
2. **Never Events**
3. **Healthcare Associated Infections**
4. **Biomedical Equipment List and Performance Report**

On 14.08.2017 in keeping with 71st independence day initiatives and coinciding again with Hon'ble Health Minister, Dr. Kamineni Srinivas garu's visit to SVIMS, an additional domain unveiled : Total Hospital Mortality trended over time.

5. **Mortality Rate: a) Net Death Rate (NDR) b) Gross Death Rate (GDR)**

Each of these can be accessed in this quality portal by **clicking here**.

SVIMS CODE BLUE

It is well recognized that preventable deaths occur in hospitals due to ‘failure to rescue’ a patient with deteriorating condition. When cardiopulmonary arrest or acute deterioration of condition occurs, appropriate resources need to be summoned to resuscitate & rescue the patient. This concept is codified in ‘CODE BLUE’. Code blue teams are in existence for many years in health systems of developed countries, but need emphasis in India. Accordingly, under the leadership of SVIMS Director a working group was formed and **CODE BLUE** is launched in June to establish the process. It is formally unveiled on **12-7-2016** by the **Hon’ble Health Minister**.

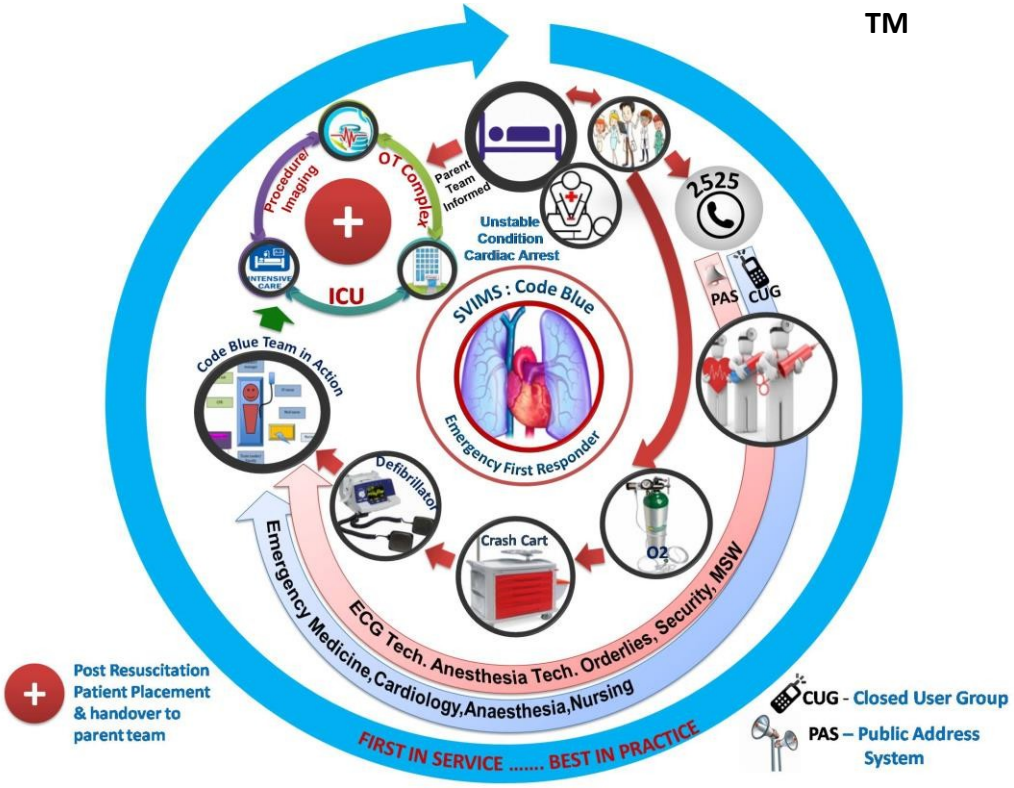

TM Application for registration of trademark for the logo is submitted and accordingly, unauthorized reproduction of the logo is prohibited.

Code Blue is a comprehensive process design for emergency responder team and response process to rescue patients and other personnel in the hospital premises. When the person sustains cardio pulmonary arrest or experiences sudden deterioration on physiologic condition Code Blue activates the afferent limb of recruiting the necessary personnel and equipments and medicines as well as the efferent limb of the response and post – response management.

Code Blue has been evolved for integration of all the stakeholders i.e., Emergency physician, Cardiologist, Anaesthetist, Emergency Nurse, ICU physician, Orderly for transportation, Pharmacist, as well as Nurse Manager, Security Officer, Medico Social Worker and Telephone Operator while attending to an emergency situation. Necessary resuscitation medicines, gadgets, including defibrillator will be made available with alacrity. Resuscitation training is imparted to all first responders.

Code Blue may be initiated from any in patient or out patient service areas of the SVIMS hospital by dialing 2525 in the intercom. The 2525 call is only for code blue to mobilize emergency responder team and not for other calls.

The process and outcomes will be monitored regularly for iterative improvement.

CPRA Committee

CPRA Committee (formerly known as Code Blue Committee) was constituted and made functional on 12 July, 2016.

Scope:

Identification of Victim, prompt resuscitation as per Basic Life Support (BLS) & Advanced Cardiac Life Support (ACLS) protocols of American Heart Association (AHA) to achieve Return of Spontaneous Circulation (ROSC) and to provide immediate Post-Cardiac Arrest Care.

Purpose:

To ensure the standards of BLS & ACLS through internal Code Blue audits, mock drills, debriefing and continuous Quality Assurance.

CPRA Committee:

Cardiopulmonary Resuscitation Analysis (CPRA) Committee meets once in a month to

- Review Deviations.
- Implement Corrective & Preventive actions.
- Action plan to improve the Quality/Outcome measures.

Members of CPRA Committee:

S.No	Name	Designation	Department	Mobile No
1	Dr. Vanajakshamma	Professor	Cardiology	9493547668
2	Dr. KM Bhargav	Asst. Prof	Medicine	8072784096
3	Dr. Punith Patak	Associate. Prof	Paediatrics	7382114464
4	Dr. Shameem	Asst. Prof	Anaesthesiology	9121021821
5	Dr. P. Subramanyam	Asst. Prof	EMD	9493860490
6	J. Sharada devi	Nur. Supdt.II	Nursing Department	9494891286
7	T. Suseela	Head Nurse	Nursing Department	9441995124
8	N. Ravanamma	Head Nurse	Nursing Department	9666588297
9	Y. Nirmala	Head Nurse	Nursing Department	9491779904
10	L. Haritha	Head Nurse	Nursing Department	9908837224
11	N. Afrin	Staff Nurse	ITC	9347689542
12	M. Sujatha	Staff Nurse	Code Blue	6302257676
13	M. Soni	Staff Nurse	Code Blue	8374213931
14	Gayathri	Staff Nurse	Code Blue	9052773155
15	B. Divyavani	Staff Nurse	Code Blue	9618746903
16	M. Manoj Kumar	Technician	Code Blue	8309554979
17	B. Prasad	Computer Assistant	Computer Section	9849505070
18	N.V.S. Prasad	MSW	MSW	8985555766
19	N.V. Bhaskar	SO	Security	7382659581
20	N. Krishna Reddy	Secretarial Assistant	Cardiology	9704608060

Code Blue Team:

1. Cardiologist
2. Anaesthesiologist
3. Emergency Physician
4. Anaesthesia Technician
5. Code Blue Sisters
6. Medico Social Worker (MSW)
7. Security Officer

Mock Drills:

- Initiated in October-2019.
- Conducting 2 Mock Drills /month.

Audits:

- Initiated in November-2019.
- ***Structural Audits:*** 02 per month.
- ***Process Audit:*** 6 to 10 per month.

Average number of calls = 537/annum

Cumulative no. of Alive patients after Code-blue revival discharge as on 31.Dec.2020:

Total Number = 177

Year	Revived	Alive cases as on 31.Dec.2020	Expired cases as on 31.Dec.2020	No communication
2016	**45**	**21**	**6**	**18**
2017	**71**	**41**	**9**	**21**
2018	**112**	**41**	**13**	**58**
2019	**107**	**32**	**15**	**60**
2020	**86**	**42**	**44**	**0**

BLS & ACLS AHA training within the Organization:

- Trained = 630 including
  - ✓ Doctors
  - ✓ Nurses
  - ✓ Staff &
  - ✓ Students

	Provider (n=608)	Instructor (n=22)
BLS (n=490)	479	11
ACLS (n=140)	129	11

✓ AHA trained instructors available in the institution = 14

Institutional training given:

- BLS - 680
- ACLS -240

Community CPR training given:65,000

Preventive & Corrective Actions:

- Community CPR
- Training of In-house staff in BLS & ACLS
- Mock drills,
- Internal Audits
- Debriefing

Sri Venkateswara Institute of Medical Sciences (SVIMS), Tirupati

CODE BLUE DATA

June 2016 – December 2016

PERIOD (June 2016 to Dec 2016)	NUMBER OF CALLS			OUTCOMES	
	Total	Initial	Repeat	Survived	Died
June	33	29	4	6	23
July	58	55	3	12	43
August	35	33	2	8	25
September	33	25	8	3	22
October	33	30	3	6	24
November	28	27	1	3	24
December	39	36	3	7	29
Total	**259**	**235**	**24**	**45**	**190**

Sri Venkateswara Institute of Medical Sciences (SVIMS), Tirupati

CODE BLUE DATA

January 2017 – December 2017

PERIOD (Jan 2017-Dec 2017)	NUMBER OF CALLS			OUTCOMES	
	Total	Initial	Repeat	Survived	Died
January	41	38	3	5	33
February	39	36	3	6	30
March	36	35	1	5	30
April	46	36	10	2	34
May	43	38	5	5	33
June	34	31	3	5	26
July	41	40	1	6	34
August	49	44	5	4	40
September	45	39	6	2	37
October	67	58	9	12	46
November	70	63	7	13	50
December	53	45	8	6	39
TOTAL	**484**	**429**	**55**	**71**	**369**

Sri Venkateswara Institute of Medical Sciences (SVIMS), Tirupati

CODE BLUE DATA

January 2018 – December 2018

PERIOD (Jan 2018-Dec 2018)	NUMBER OF CALLS			OUTCOMES	
	Total	Initial	Repeat	Survived	Died
January	45	36	9	6	30
February	49	34	15	0	34
March	65	56	9	11	45
April	46	46	0	18	28
May	61	58	3	8	50
June	56	56	0	16	40
July	52	47	5	6	41
August	64	57	7	7	50
September	56	53	3	14	39
October	73	67	6	8	59
November	54	51	3	8	43
December	70	66	4	10	56
TOTAL	**691**	**627**	**64**	**112**	**515**

Sri Venkateswara Institute of Medical Sciences (SVIMS), Tirupati

CODE BLUE DATA

January 2019 – December 2019

PERIOD (Jan 2019-Feb 2019)	NUMBER OF CALLS			OUTCOMES	
	Total	Repeat	Initial	Survived	Died
January	60	03	57	09	48
February	48	01	47	11	36
March	52	02	50	06	44
April	53	04	49	11	38
May	59	04	55	10	45
June	50	03	47	06	37
July	52	09	43	02	41
August	56	05	51	07	44
September	74	10	64	12	52
October	73	--	73	11	62
November	60	01	59	10	49
December	74	08	66	12	54
TOTAL	**711**	**50**	**661**	**107**	**554**

Sri Venkateswara Institute of Medical Sciences (SVIMS), Tirupati

CODE BLUE DATA

January 2020 – December 2020

	Total	Repeat	Initial	Survived	Died
January	71	04	67	17	50
February	71	07	64	09	55
March	96	12	84	19	65
April	27	01	26	08	18
May	16	0	16	03	13
June	39	01	38	06	32
July	25	0	25	07	18
August	07	0	07	01	06
September	08	0	08	02	06
October	14	0	14	03	11
November	42	06	36	05	31
December	46	07	39	06	33
TOTAL	**462**	**38**	**424**	**86**	**338**

STATISTICS

Observation Spell	Number of Calls	Initial	Repeat	Died	Revived (%)
July-Dec 16	259	235	24	190	45 (19.1%)
Jan-Dec 17	564	503	61	432	71 (14.1%)
Jan-Dec 18	691	627	64	515	112 (17.9%)
Jan-Dec 19	711	661	50	554	107 (16.2%)
Jan-Dec 20	462	424	38	338	86 (20.3%)

Improving the effectiveness and long term survival analysis after Code Blue

SVIMS is currently performing 'Analysis of Code Blue outcomes in Long term Survivors'. SVIMS is also conducting audit of the effectiveness of resuscitation as well as instituting 'Debriefing' after each Code Blue call. Further, all Code Blue responders are being trained in BLS/ACLS protocol of American Heart Association, through SVIMS International Training Center, designated by AHA.

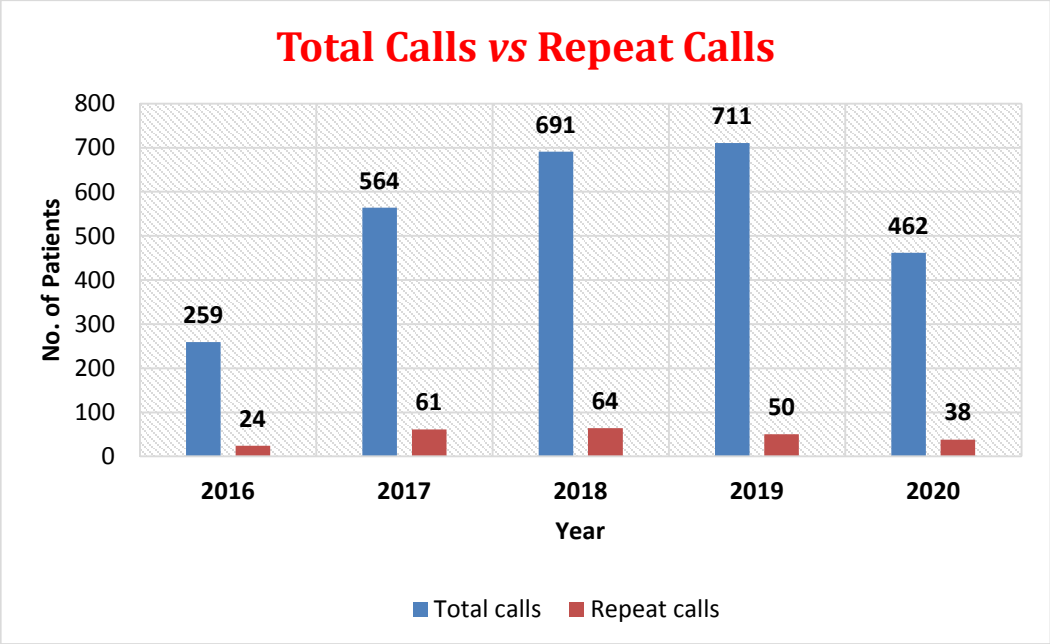

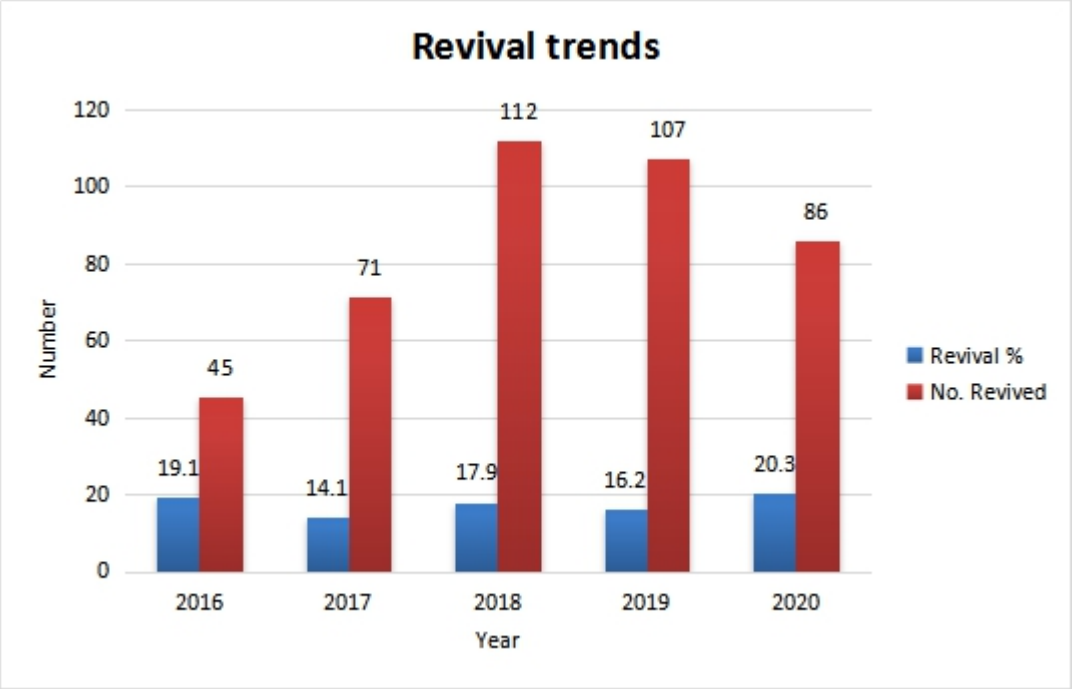

REVIVAL PERCENTAGE

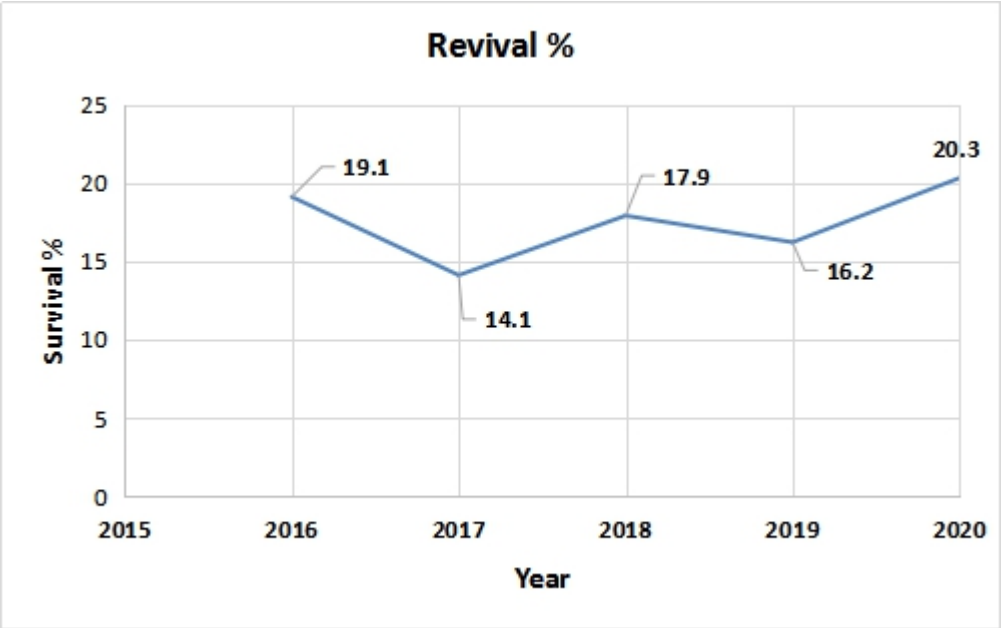

CME on CPR conducted on 23.Dec.2019

- Organized with an objective to understand the common mistakes that are being done and to give practical knowledge regarding correct CPR practices.
- Around **250 members** were attended.
- **2 Code Blue simulation practical** sessions were conducted.
- **6 topics were presented** by various members of the CPRA committee.

Topic	Speaker
Assessment of Cardiac Arrest	Dr. P. Subramanyam
High Quality CPR	Miss. N. Afrin
Air way Management	Dr. S. Shameem
Team Dynamics	Dr. K.M. Bhargav
Paediatric life support	Dr. P. Punith
Near Death Experience in CKD Patients	Dr. P. L. Aishwarya

CME ON
PULMONARY RESUSCITATION
23 - 12 - 2019
ESWARA INSTITUTE OF MEDICAL SCIENCES
mala Tirupati Devasthanams

CME ON
CARDIOPULMONARY RESUSCITATION
23-12-2019
SRI VENKATESWARA INSTITUTE OF MEDICAL SCIENCES

SVIMS NEVER EVENTS

First introduced in 2001, the term 'Never Events' refers to shocking, egregious, unambiguous and measurable **events that should never occur in healthcare**. During the last 15 years, a list of such highly serious adverse events have been catalogued in many countries. These events result in death or significant disability and are preventable. SVIMS has started measuring each of these 'Never Events' and has put in place safety parameters to mitigate any harm with the goal to eliminate them. Thus, SVIMS become the First Health Care System in India, to voluntarily report safety record, towards continuous quality improvement. Never Events indicate fundamental safety problems within an organization or system. They are grouped into 7 categories SVIMS will choose one from each of these groupings as outlined above & will methodically put in place safety measures to eliminate them:

Never Event Category	Indicator	
	Description	Benchmark
Care Management Events	Stage 3 & 4 Decubitus ulcer during hospital	**0**
Administration of drug or biological	Mismatched Blood Transfusion with serious harm.	0
Radiological Events	Metallic object in MRI suite causing injury	0
Environmental Events	Falls in hospital premises with serious injury	1
Procedure Events	Wrong site/wrong patient procedure	0
Device Events	Foreign object unintentionally left inside body during surgery	0
Patient Protection Events	Misidentification or missing baby	0

On 12-07-2016, Hon'ble Health Minister, Dr. Kamineni Srinivas garu unveiled SVIMS Website reporting of **one such never event, namely stage 3/4 Decubitus Ulcer.**

NEVER EVENTS AT SVIMS : SERIOUS SEVEN

i. Decubitus Ulcer - stage 3 /4

Decubitus Ulcer is also known as Pressure sore/bed sore. Since the monitoring started in September 2015 after the arrival of the new Director and **during the period Sep 2015 to 31st January, 2021, no stage 3 / 4 Decubitus Ulcer has developed in any patient as a result of stay at SVIMS.**

Even though only stage 3 and 4 Decubitus Ulcer are considered as never events, at SVIMS nursing section has started following all patients for the identification and corrective measures for stage 1 and stage 2 Decubitus Ulcer in order to prevent them progressing to stage 3 or 4. It is to be noted that stage 2 ulcers are observed only in patients who are transferred in with decubitus ulcers and no patients at SVIMS developed any stage 2 ulcers.

Definition:

Stage I: Redness without skin breakdown.
Stage II: Skin breakdown – Epidermis and Dermis.
Stage III: Full thickness destruction through dermis into subcutaneous tissue
Stage IV: Deep tissue destruction through subcutaneous tissue to fascia muscle, bone.

Decubitus Ulcers Report Stage 1 (January 2020 to 31st January 2021)

Note : Total Hospital Census :	29422	
ICU patients	**5238**	**20.69%**
Stage 1 & 2 Decubitus ulcer incidence:		
Developed at SVIMS For the Year 2020	60	0.23%
Present on Admission For the Year 2020	90	0.38%

Decubitus Ulcers Report Stage 1 (January to December 2019)

Note : Total Hospital Census :	34078	
ICU patients	**7108**	**20.69%**
Stage 1 & 2 Decubitus ulcer incidence:		
Developed at SVIMS For the Year 2019	56	0.23%
Present on Admission For the Year 2019	76	0.38%

Decubitus Ulcers Report Stage 1 (Sept 2015 to 31st December 2018)

Note : Total Hospital Census :	31968	
ICU patients	6783	21.94%
Stage 1 & 2 Decubitus ulcer incidence:		
Developed at SVIMS For the Year 2018	55	0.17%
Present on Admission For the Year 2018	74	0.24%

	Ulcers Developed at		
Year	**SVIMS**	**Outside**	**Total**
2015	15	22	37
2016	51	82	133
2017	52	85	137
2018	55	77	132
2019	70	150	220
2020	22	117	139
Total	**265**	**533**	**798**

Decubitus Ulcers Report Stage I

Month	Ulcers Developed		
	SVIMS	Outside	Total
Sept,2015	05	13	18
Oct,2015	05	02	07
Nov,2015	01	0	01
Dec,2015	04	07	11
Total (A)	**15**	**22**	**37**
Jan,16	09	09	18
Feb,16	05	08	13
Mar,16	03	03	06
Apr,16	09	05	14
May,16	02	07	09
Jun,16	01	06	07
Jul,16	06	08	14
Aug,16	02	04	06
Sep,16	06	08	14
Oct,16	01	05	06
Nov,16	04	08	12
Dec,16	03	11	14
Total (B)	**51**	**82**	**133**
Jan,17	06	14	20
Feb,17	05	08	13
Mar,17	06	08	14
Apr,17	03	06	09
May,17	05	06	11
Jun,17	09	10	19
Jul,17	04	07	11
Aug,17	02	04	06
Sep,17	04	06	10
Oct,17	04	07	11
Nov,17	02	02	04
Dec,17	02	07	09
Total (C)	**52**	**85**	**137**
Jan,18	06	08	14
Feb,18	07	06	13
Mar,18	04	03	07
Apr,18	06	08	14
May,18	02	06	08
Jun,18	02	12	14
July,18	0	04	04
Aug,18	04	07	11
Sep,18	11	08	19
Oct,18	05	07	12
Nov,18	05	05	10
Dec,18	03	03	06
TOTAL(D)	**55**	**77**	**132**

Month	Ulcers Developed		
	SVIMS	Outside	Total
January,2019	4	11	15
February,2019	10	5	15
March, 2019	09	12	21
April, 2019	3	20	23
May, 2019	16	12	28
June,2019	09	07	16
July, 2019	05	09	14
August,2019	03	11	14
September,2019	01	10	11
October,2019	04	18	22
November,2019	02	18	20
December,2019	04	17	21
Total (E)	**70**	**150**	**220**
January,2020	02	10	12
February,2020	03	16	19
March, 2020	02	16	18
April, 2020	02	12	14
May, 2020	02	13	15
June,2020	02	12	14
July, 2020	01	14	15
August,2020	04	11	15
September,2020	00	05	05
October,2020	01	04	05
November,2020	02	05	07
December,2020	01	04	05
Total (F)	**22**	122	**144**
Grand Total (A+B+C+D+E+F)	**265**	**538**	**803**

Measures taken for preventing stage III & IV. Never events incidence none.

Mismatched Blood Transfusions causing serious harm

Protocol for Prevention of Mismatched Blood Transfusion

1. Scope & Application

Never events are serious medical errors or adverse events that should never happen to a patient. Consequences include both patient harm and increased cost to the institution. Technicians and nurses provide a critical role in preventing never events through risk anticipation and adoption of evidence-based practice. Mismatched blood transfusion is one of the never events which should never happen in a hospital

2. Responsibility

- Staff nurse in donor section to correctly label the blood bag.
- The technician on duty in Red Cell Laboratory to correctly receive the blood sample and to issue the blood for which requisition is received.
- The staff concerned in the ward/OT to correctly label the sample and to transfuse the blood unit.

3. Reference

- Technical Manual, Directorate General for Health Services-2nd edition
- Model standard operating procedures for blood transfusion services, WHO
- NACO guidelines2015

4. Protocol

Checks at the donor blood collection section

- Each donor will be given a unique number and once his blood is collected, it is identified by that number only.
- Verify the donor's identity by tallying with the name on the donor card and the donor number.
- Write the segment number of the blood bag on to the donor card as a second check.
- Cross check the numbers on the bag, pilot tubes and donor card to ensure identity. Record the entry in the donor registers using the same number.

Checks while doing blood grouping and typing:

- One technician should do forward grouping from the segment of the blood bag by correlating the segment number and unique donor number with that entered in the donor card. Enter the results in the donor unit and in the donor cell grouping register.
- Another technician should do reverse grouping from the pilot tubes collected, by identifying the unique donor number. Enter the result in the serum grouping register. Both the forward and reverse grouping result should correlate each other

Checks at the component storage section

- All untested units should be kept in the unscreened Refrigerator / agitator.
- After testing is over, release the fully tested. Write clearly the unit number, date of collection and expiry and the volume on each colour coded label as per the grouping register records.
- After the bags are labelled, ask a second technician to double check the number and group on the bags tallying them with the records.

Checks in the cross matching section:

- Receive the requisition form along with the patient's blood sample. Check for patient's identity.
  Name of the patient, UHID number, age and sex should correlate with the blood sample and requisition form. Check the blood group with that of the blood group entered in the request. If there is any discrepancy, check the blood group of the received blood sample. If it correlates with the hospital information system, then ask the concerned ward staff to change in the request before proceeding with the cross matching.
- If there is no discrepancy between the HIS and the blood group in the request, proceed with the blood grouping of the patient with the currently received sample
- If there is no discrepancy then proceed with the cross matching. If still discrepancy persists, then the old blood sample might be a wrong sample. Trace back the old details and investigate where the fault is.
- Carry out compatibility testing using departmental SOP. In order to avoid outdating, implement FIFO policy
- The technician who is issuing blood should make entries in the cross matching form with counter sign from the medical officer.
- Make entries in the issue register and in the request.
- The receiving person should check the blood unit and the cross matching report from for any discrepancy

Checks at the ward/OT:

- Before administering blood component, FINAL IDENTITY -check of the patient, blood unit compatibility tag and the complete documentation should be done.
- Ask the patient, if conscious, to identify himself/ herself by name, spouse name, age or any other identification.
- If unconscious, ask relatives or any other staff to verify the patient's identity.
- Check that details on the compatibility tag exactly match with the documentation.
- Check the blood unit for any leakage and for any visible discoloration & expiry date
- Two different persons should do the check for patient's identity and the same should be documented.

5. Documentation

- Make necessary entries in donor register, grouping register, cross matching register, issue register, incident report register, critical value reporting register, cross matching form, case file.

STATISTICS OF WHOLE BLOOD/BLOOD COMPONENTS ISSUES AND NEVER EVENTS

S.No.	Year	Total No. of Whole Blood/ Blood Components Issued	Never events Record
1.	2014	18,062	Nil
2.	2015	17,109	Nil
3.	2016	17,807	Nil
4.	2017*	23,548	Nil
5.	2018	26,287	Nil
6.	2019**	27704	01
7.	2020	15222	Nil

*2017: One patient received blood components in 2017 minor subtype mismatched blood treated with steroid promptly without any sequelae and discharged in normal condition.

**2019: Date of Mismatch: 13th June 2019
Patient Developed Renal Failure and now recovered. Root cause analysis is in progress to identify Causative Factors and implement corrective action plans.

iii. Metallic Object in MRI Suite causing injury

MRI SAFETY REPORT

The last unexpected event in MRI occurred on 10th January 2015 at 2.30 PM where in Oxygen cylinder was pulled in the magnet. However **no patient / personnel injury** or hardware loss was suffered. **No adverse MRI events during 2016, 2017 & also upto January 31st 2021.**

To totally avoid such situation in future following steps are being followed :-

1. Oxygen lines are made available in preparation area
2. Screening at inlet for oxygen cylinders is being done
3. Maintenance of routine duly signed MRI safety check list for all the patients is being done since from that time no such incident has occurred in our department.

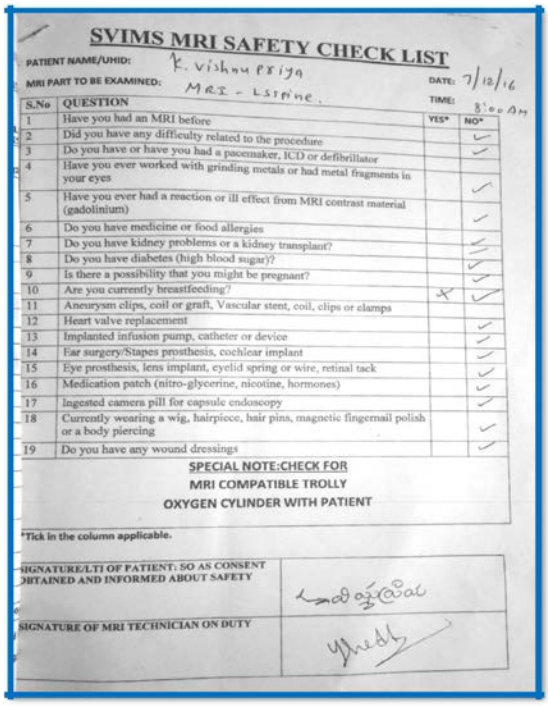

SVIMS MRI SAFETY CHECK LIST

PATIENT NAME/UHID: K. vishnu priya
MRI PART TO BE EXAMINED: MRI - LS spine.
DATE: 7/12/16
TIME: 3:00 PM

S.No	QUESTION	YES*	NO*
1	Have you had an MRI before		✓
2	Did you have any difficulty related to the procedure		✓
3	Do you have or have you had a pacemaker, ICD or defibrillator		✓
4	Have you ever worked with grinding metals or had metal fragments in your eyes		✓
5	Have you ever had a reaction or ill effect from MRI contrast material (gadolinium)		✓
6	Do you have medicine or food allergies		✓
7	Do you have kidney problems or a kidney transplant?		✓
8	Do you have diabetes (high blood sugar)?		✓
9	Is there a possibility that you might be pregnant?		✓
10	Are you currently breastfeeding?	✗	✓
11	Aneurysm clips, coil or graft, Vascular stent, coil, clips or clamps		✓
12	Heart valve replacement		✓
13	Implanted infusion pump, catheter or device		✓
14	Ear surgery/Stapes prosthesis, cochlear implant		✓
15	Eye prosthesis, lens implant, eyelid spring or wire, retinal tack		✓
16	Medication patch (nitro-glycerine, nicotine, hormones)		✓
17	Ingested camera pill for capsule endoscopy		✓
18	Currently wearing a wig, hairpiece, hair pins, magnetic fingernail polish or a body piercing		✓
19	Do you have any wound dressings		✓

SPECIAL NOTE:CHECK FOR
MRI COMPATIBLE TROLLY
OXYGEN CYLINDER WITH PATIENT

*Tick in the column applicable.

SIGNATURE/LTI OF PATIENT: SO AS CONSENT OBTAINED AND INFORMED ABOUT SAFETY

SIGNATURE OF MRI TECHNICIAN ON DUTY

sample checklist

iv. Falls in Hospital Premises Causing Serious Injury or Death

Fall Huddle Report from Nov 2015 to January31st 2021

Year	Falls	Fracture	Mild Injuries
2015 (Nov & Dec)	02	01	01
2016	16	09	07
2017	07	03	04
2018	08	-	08
2019	06	01	05
2020	2	-	03
Total	41	14	28

Fractures & Mild Injuries from Nov 2015 to January 31st 2021

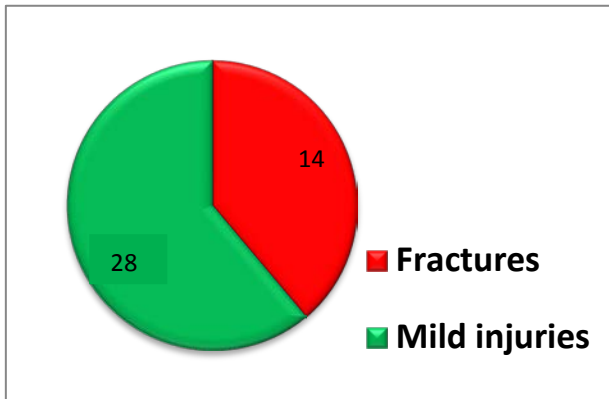

Huddle Report on 1st November, 2015 to January 31st 2021

Month	Fracture	Type of Fracture	Injury	Type of Injury
Nov,15	1	Patella transversa	-	-
Dec,15	-	-	1	Patella swelling & back pain
Jan,16	1	Ulnar bone fracture	1	Mild head injury.
Feb,16	-	-	-	-
Mar,16	1	Lt.humerus fracture	1	Injury over chin.
Apr,16	-	-	1	Injury over Rt.eye brow.
May,16	1	Rt.femur fracture	2	1.Rt.parietal region injury. 2.Mild back pain.
Jun,16	-	-	1	Injury over occipital region
July,16	1	Lt.femur fracture	-	-
Aug,16	1	Left elbow ulnar region	1	Laceration over occipital region.
Sep,16	2	Medical condyle of Lt.humerus. Rt.prosthetic femur	-	-
Oct,16	-	-	-	-
Nov,16	2	Lt.distal radial & ulnar fracture. Bilateral fracture calcaneum.	-	-
Dec,16	-	-	-	-
Jan,17	-	-	-	-
Feb,17	-	-	-	-
Mar,17	1	Rt.temporal bone fracture	-	-
Apl,17	-	-	-	-
May,17	-	-	1	Mild laceration over the frontal region.
Jun,17	-	-	-	-
Jul,17	-	-	2	Swelling over left arm &occipital region. Swelling over left leg ankle.
Aug,17	-	-	-	-
Sep,17	1	Left tibia fibula fracture	-	-
Oct,17	1	Right femur fracture	-	-
Nov,17	-	-	-	-
Dec,17	-	-	1	Laceration over chin.
Jan,18	-	-	-	-
Feb,18	-	-	1	Meniscus tear.
Mar,18	-	-	-	-
Apr, 18	-	-	-	-
May'18	-	-	3	No Fall Injuries. Laceration over parietal region. Laceration over left frontal region.

Jun,18	-	-	-	-
Jul,18	-	-	-	-
Aug,18	-	-	1	
Sep 18		No falls in Sep 2018		
Oct' 18	-	Scalp hematoma at occipital region	1	Slight laceration over Rt.cheek.
Nov'18	1	Lt.side fracture	-	-
Dec'18		No falls in the month of December 2018		
Jan,19			1	
Feb,2019		No falls in the month February,2019		
Mar,2019	-	No falls in the month March,2019 (since 79 days)		
Apr, 2019	-	No falls in the month of April,2019 (since 109 days)		
May,2019	1	Open reduction internal fixation with plating for Lt.radius & ulna	1	
June, 2019	No falls in the month of June,2019 (last fall 39 days back)			
July, 2019	No falls in the month of July,2019 (last fall 68 days back)			
August,2019	No falls in the month of August, 2019 (last fall 109 days back)			
September,19	No falls in the month of September, 2019 (last fall 139 days back)			
October,19 to January,20	No falls from October,19 to January,20,			
February,2020	**-**	**-**	**1**	Injury in temporal region
March,20 to 15th September,20	No falls from March,20 to 15th September,2020,			
October, 2020 to December, 2020	**-**	**-**	**2**	Head Injury (Temporal Region) & Right ankle pain
Total	**14**		**28**	

Since starting the record in Nov 2015 to till date, no deaths in the hospital premises reported. However, the fractures and injuries are shown below.

Detailed Fall Huddle Report from 1st November 2015 to 31st January 2021

	2015						
S.No	**Name of the Resident**	**Injury after fall**	**Diagnosis**	**Date of fall**	**Time**	**Cause of fall**	**Treatment & status at discharge**
1	Patient attender	Patella transverse #	Not Applicable	November 2015	7.30 pm	Rain water stagnation & pt not taken diet more than 10 hrs	T.Dolo 650, Ranctac, Physiotherapy & shifted to BIRRD OT
2	Staff Nurse	Patella swelling and back pain	N.A	December 2015	1.15 pm	Due to water stagnation	Strict bedrest 14 days, Volini gel, myospase
	2016						
3	Fessy worker	Fracture ulnar bone ,	N.A	January, 19th 2016	5.30 pm	Slip from trolley while cleaning Roof	POP applied, Immobilisation of hand, voveran, Rantac, myospase
4	Patient Attender	Head injury	N.A	January, 17th, 2016	12.30pm	Giddiness due to not taken diet	Inj –Rantac, Inj-Diclofenac- 1 Taxim given
5	Patient Attender	Injury over chin 3x2 cms	N.A	March,8th 2016	3.45 pm	Phobia regarding hospital instruments	Suturing done, minor dressing,voveron, antacids
6	Patient	Left humerus #	N.A	March, 22nd 2016	7 am	Hypertension sudden giddiness	POP applied & shifted to BIRRD
7	Patient	Injury over Rt.eyebrow	Metabolic Encepahal opathy	April, 26th 2016	11.45am	Hypertension sudden giddiness	Suturing done, minor dressing, voveron, antacids
8	Patient	Rt.parietal region injury	Meningoma	May, 4th 2016	5.30 pm	Giddiness, reoccurrence history of fall	Suturing done, minor dressing, voveron, antacids
9	Patient	Fracture Rt.femur	Dcmp with Afwith FVR	28th, May, 16	10.30pm	Giddiness, vomitings	Skin traction, bird consultation sent plan for sub trachetic extension
10	Patient Attender	Mild back pain	CKD,HTN on MHD	29th, May, 2016	10:45pm	Dizziness	Tab;ultracet;local application of diclo gel
11	Patient	Injury over Lt.fore head	Right occipital infract in parietal region	9th ,June, 2016	4.00am	Sudden loss of muscle control, parathesia	Suturing done, minor dressing, voveron, antacids
12	Patient	Fracture Left femur	Rt.Lung consolidation	7th, July, 2016	7.00am	Obstructed dhoti of patient leads fall	Skin traction with 3kgs of weight
13	Patient Attender	Fracture at Lt.elbow ulnar region	-	August, 20, 2016	12.30pm	Slip while walk	Pop applied on left elbow, Aceclopara, Rantac, Chymoralforte
14	Patient Attender	Injury Occipital region	-	August, 29, 2016	10.30am	Went to wash room for washing cloths, slipped slippers.	Tab. Cefixime 200mg Tab. Aceclopara Inj.T.T IM given.
15	Student	Fracture medical condyle of Lt.humerus	-	Sep 19th, 2016	2.30pm	Slipped leg	Pop applied Tab. Dolpal Tab. Chymoral forte
16	Staff	Fractured Rt. periprosthatic femur.	-	Sept 26th, 2016	9.30am	Slipped leg.	1.Reffered to BIRRD. 2.Rt.LCLCP fixation.
17	Patient attender	Fracture communitedLt. distal radius & ulnar fracture.	-	5th Nov,2016	6.20am	Experienced electrical shock in bath room tap.	

S.No	Name of the Resident	Injury after fall	Diagnosis	Date of fall	Time	Cause of fall	Treatment & status at discharge
18	Patient	Laceration in parietal region, Calcaneum B/L, D2-L1 fracture.	Pre CRHD, Post op 7th MVR.	9th, Nov, 2016	8.30pm	Fear about ICU events. She attempt to go outside & unfortunately fell down.	Post op slab applied. Suturing & dressing done.
	2017						
19	Patient	Rt.temporal bone fracture with laceration over lower lip	CKD diabetic nepphropathy HTN, DM, HBs AG+ve	11/03/17	At 6.30 am	Patient went to bath room for jugular access preparation due to wet area in bath room fell down	-Neurosurgery consculation done. -Tab.Chymoral forte BD -Tab.Ultracet SOS -Tab.Augmentin 625mg
20	Patient	Mild laceration over the left & Right frontal region	CKD	17/05/17	At 12 noon	Patient went to NTRVSS room.101 for approval & the surrounding area was digged and step behind	-Dressing & suffering done over laceration & patient stable and fall injury lacerated.
21	Patient	Swelling over left arm& occipital region	Ca. vagina & retroving positive	21/7/17	At 6.45am	Patient went to bath room repeatedly due to 3-4 episodes of loose stools. She went to bath room & fall down	-Neurosurgery dressing. -Tab.chymoral forte BD,Lokome-BD, Sporolac TID
22	Patient	Swelling over Left ankle	Recurrent ankle pancreatitis	24/7/17	At 1.30am	Patient went to bath room suddenly slip his foot while walking & fell down.	-Inj.Tramodal SOS, Emset SOS, Gel
23	Patient Attender	Left fibia fibula fracture	NA	27/9/17		Resident while walking through near NTRVSS R.No.101 she wearing slippers, the slippers are slipped .	-Inj.Pan 40mg BD -Inj.Dynapar 40mg IM - BIRRD consultation done. Cost applied over the fracture. Bed rest.
24	Patient	Inter trocheonic fracture Rt.femur	Ca. recurrent meningioma Post op excision of tumor (in our Hosp 2011, Mar, 2017) with Rt.hemiplegia	02/10/17		While going to bathroom with support of assistive device (walker) suddenly he felt slight massive ramp slipped infront of bathroom and fell down.	-Tab.chymoral forte TID,Ultracet BD -Cap.OMZ 20mg OD. Plan for closed reduction & slided TID screw fixation.
25	Patient	Laceration over chin	CLD with splenomegaly	23/12/17		While walking slippery foot slipped over floor mat & fell down & he was fasting since night.	-Inj.TT IM given. -Dressing done. -Tab.Ultracent BD, -Patient observe 1/2hrly & not to wear.
S.No	**Name of the Resident**	**Injury after fall**	**Diagnosis**	**Date of fall**	**Time**	**Cause of fall**	**Treatment & status at discharge**
	2018						
26	Staff	Meniscus tear & swelling	-	06.02.18	9.45 pm	The Resident went to washroom for hand washing, after that she returned & while walking she missed step behind	Orthopaedic consultation. Ortho consultation done. Tab.Chymoral forte TID,.Limcee OD

						the room and unfortunately fell down.	Knee support trace. Avoid bending, using steps & speed walk. Advised Medical leave for 3 weeks.
27	Patient	No Fall Injuries	Lt.Buccal mucosa	03.05.18	07.50 pm	The Resident shift to Radiotherapy while walking she missed step behind the room and unfortunately fell down. There is no fall injuries.	CT Brain Plain done, Reports shows normal. Tab. Ultracet BD.
28	Patient	Laceration over parietal region.	Primi with epilepsy with IUGR, Pop:EMLSC S.	05.05.18	7.00 am	The Resident went to wash room to brush her teeth she suddenly attack of seizure at bath room and fell down.	Dressing & Suturing done. Inj.Levera 1gm IV.
29	Patient	Laceration over left frontal region.	Acute on CKD.	08.05.18	1.45 pm.	The Resident was restrained with bandage then she was try to sit on the bed and may be had pre syncope and fell down. Patient has psychiatric problem.	CT Brain done. Report shows normal. Tab.Chymoral forte TID, Ultracet OD
30	Patient	Small laceration over nose and left ear pinna.	Infarct Rt.occipital region. Rayanoands phenomenon	07.08.18	3.45 pm	The resident shifted to radiology for the purpose of Doppler. While waiting at corridor, the resident underwent to call her attender, unfortunately she slipped from wheel chair.	CT Brain done. Report shows normal. Mild dressing done.
31	Patient	Slight laceration over Rt.cheek	Acute Gastritis,	09.10.18	At 7am	The resident trying to stepping down from trolley suddenly she fell down.	CT Brain done. Report shows normal. Mild dressing done. Dressing over laceration.
32	Patient	Scalp hematoma at occipital region	Ca ovary	30.10.18	At 7.50am	The resident has sudden fall due to giddiness.	CT Brain done. Report shows a scalp hematoma at occipital region.
33	Patient	Lt.side fracture	Bilateral lobar infarct	19.11.18	At 3.30pm	The resident went to bathroom, after that to get she takes support of door and fell down.	X-ray hip AP & Lat.view shows Lt.side fracture.

	2019						
S/No	**Name of the Resident**	**Injury after fall**	**Diagnosis**	**Date of fall**	**Time**	**Cause of fall**	**Treatment & status**
34	Patient	SDH	Uterus sarcoma, staging laporatomy done on 03-1-19.	11-01-19	3.20pm	Giddiness.	Rt.fronto temporo parietal craniotomy & SDH Evacuation done on 17-1-19.
35	No falls in the month February,2019						
36	No falls in the month March,2019 (since 79 days)						
37	No falls in the month of April,2019 (since 109 days)						
38	No falls in the month of May,2019 (since 140 days)						
39	Staff Nurse	Both bones fracture at Lt.fore arm	-	16-05.-19	2.05pm	The resident has sudden fall due to slippage of slipper.	Open reduction internal fixation with plating for Lt.radius and ulna.

40	Doctor Staff	NO INJURIES	-	23-05-19	9.45am	Skid from chair (chair was broken while sitting)	NO INJURIES.
41	No falls in the month of June, 2019 (last fall 39 days back)						
42	No falls in the month of July, 2019 (last fall 68 days back)						
43	No falls in the month of August, 2019 (last fall 109 days back)						
44	No falls in the month of September, 2019 (last fall 139 days back)						
45	P.A (Pharmacology)	No injuries	-	16.11.2019	11.30AM	Fell down while taking the phone from the switch board	-
46	Patient	No injuries	CKD	28.11.2019	2PM	Fell down in washroom due to giddiness	CT Brain Plain done, Report shows normal, Tab. Ultracet BD.
47	Patient	Pain left at hip region	Ca cervix	17.12.2019	5.40PM	Fell down in washroom	Hip X-ray was done, injection Tremadal IV given
48	Patient	Injury in temporal region	CA cervix	25.02.2020	11.30AM	Fell down in washroom	X-Ray done, small injuries identified, Ortho consultation done, CT brain normal.
49	Patient	Head Injury (Temporal Region)	CA left breast	29.11.2020	12pm	While coming from washroom with attender	CT brain done, X-Ray done, General Surgery consultation done.
50	Patient	Right ankle pain	CA Rectum	19.12.2020	5am	While coming from washroom	X-Ray done and report is normal.

No. of Patients : 28
Patient Attenders : 09
Staff : 07
Student : 01

TOTAL : 45

Preventive Measures & Corrective Actions:

1. Side rails fixed to all trolleys in EMD & decided to be procured side rails Trolleys in future.
2. Fixed support handles in all toilets
3. Fixed support handles to ramps.
4. For construction of new bathrooms/toilets anti-skid tiles arranged.
5. Arranged caution boards while mopping the floors.
6. Education programmes regarding prevention of falls to nursing, physicians, allied health & administrative staff.

V. Procedure Events

In order to prevent wrong site/wrong patient procedure, SVIMS has begun implementation of WHO surgical checklist in all procedure areas. Members of SVIMS quality council (SQC) group assigned this task, will monitor & report data monthly.

Department of Anaesthesiology and Critical care	**WHO SURGICAL SAFETY CHECK LIST**

Hand over S/N **Ward----------** **Date----- Time----** **----**	**Take over S/N** **OT----------** **Date-------- Time ------**	**Hand over S/N/Anaesth Tech.** **RR---------- Date----------Time----------**

BEFORE INDUCTION OF ANAESTHESIA (SIGN IN)								
Patient has confirmed	**Yes**	**No**	**Relevant Lab result**	**Yes**	**No**	**Anaesthesia safety check list**	**Yes**	**No**
Identity			ECG/ECHO/Angio			Known allergy		
Site marked/Not applicable			CXR/CT/MRI			Airway/Aspiration risk		
Consent obtained			Biochemistry			If, yes assistance/equipment available		
Procedure			Haematology			Risk of > 0.5L(>7mL/kg in children) blood loss		
Part preparation done			Microbiology			If, yes IV access and fluid planned		
Denture/Jewellery/contact lenses removed			Xylocaine/Antibiotic test dose given and encircled					
Double hair bun prepared for females			DVT Prophylaxis					
NPO status(write no of hours)			Patient warming system/Need for active warming					
Blood group and cross matching done			Blood and blood product availability					

BEFORE SKIN INCISION (TIME OUT)				
Entire surgical team confirms	**Yes**	**No**	**Surgeon shares**	**Nursing /Anaesthesia technician reviews**
Patient's name			Critical/Unexpected step	Sterility, including indicator results
Surgical procedure to be performed			Expected duration	Equipment Issues
Surgical site			Expected blood loss	Working suction
Essential imaging available			**Anaesthesiologist shares**	Baby tray/Crash cart
Antibiotic prophylaxis within the last 60 minutes			Anaesthesia plan	Catheter/Tube/Lines
Antibiotic re-dosing plan			Patient specific concerns	Other concerns

BEFORE PATIENT LEAVES OPERATING ROOM (SIGN OUT)			
Nurse reviews with Team	**Yes**	**No**	Equipment problems that need to be addressed.
Instrument, sponge and needle counts are correct			Entire team discusses concerns for patient recovery and management
Specimen labelling			
Name of the procedure recorded			

WHO check list implemented in stages starting in 2016 and monitoring continued till date.

vi. Device Events

No Foreign object unintentionally left inside body during surgery at SVIMS during 2016 to till date.

vii. Patient Protection Events

Measures taken in SPMC Hospital to prevent baby abduction

- Standard Operating Procedures have been developed for security& ward staff in order to prevent baby abduction.
- ID tags tied to the wrist of the mother and baby immediately after delivery.
- Foot prints of the baby taken in the Case sheet/File immediately after delivery in the case sheet along with signature of responsible patient attender.
- Transfer out/discharge forms developed to transfer the baby with in hospital (Intra hospital) and outside hospital (Inter hospital), also for normal discharge.
- Baby will not be allowed to move outside of the ward without proper transfer out/discharge form and also without responsible attendant along with hospital staff.
- At the time of transfer out/discharge of the baby from the post natal ward/NICU the duty nurse along with doctor on duty and baby mother will sign on the transfer out/discharge slip which will be checked by security at Post natal ward &main entrance along with baby ID tag.
- Security guards at the Post natal ward and main entrance will record the details of the baby along with attendant details at the time of transfer out/discharge.
- CC Camera's were fixed at the entrance of the Post natal ward and at maintenance.
- Failure Modes Effects & Analysis (FMEA) done for baby abduction in July 2018 & surveillance through mock drills regularly conducted.

CODE PINK MOCK DRILL

EVENTS:

- Code Pink Mock drill has conducted on 29.11.2019 at 03:00 p.m. to 03:30 p.m. at OBS Ward, SVIMS- SPMC (W) Hospital for awareness on Baby abduction.

PHOTOS:

Ward sister & Security alerting about **CODE PINK** to Main gate Security

Main gate Security receiving call about **CODE PINK**

Alerting about **CODE PINK** though Public Addressing System

Commencement of searching process from all entrance & exit points

NO BABY ABDUCTION / MISIDENTIFICATION TILL DATE AT SVIMS

***

Biomedical Equipment List and Performance Report

SVIMS and SPMC Hospital

In order to improve efficiency, effectiveness and reduce Non Performing Assets (NPA) in the health system, SVIMS has put forth an accountable system of making a full list of Biomedical Equipment and enumerate the functional status of each and every equipment. The goal is to ensure that 99-100% of equipmentare functional and repairs are done in a timely fashion according to benchmark (days in disrepair). In addition all equipment will be listed with their price and date of commissioning in the website. As on 31st JANUARY 2020 the following functional equipment benchmark is shown. The details are listed in nextpage.

SVIMS
Bio-Medical Equipment Status List

Total No. of Equipments	1301
No. of functional Equipments	1293
No. of non-functional Equipments	08
Percentage functional	1293/1301 *100 = 99%

SVIMS SPMC (W) IPW
Bio-Medical Equipment Status List

Total No. of Medical Equipments	145
Total No. of Medical Equipments Working	144
Total No. of Medical Equipments Not Working	01
Percentage functional	144/145 *100 =99%

Equipment status Report on 31st JANUARY, 2020- SVIMS

Total Number of Equipment = 1301
Number functional Equipment = 1293
Number non functional Equipment =08
Percentage = 1301 /1293 *100 = 99%

Action Report

Sl No	Equipment	Manufacturer	Days of Disrepair	Value	Remarks
1	Syringe Pump	Plenum tech	18/11/2020	Rs 24,489	Needs Parts -Under process
2	Syringe Pump	Plenum tech	18/11/2020	Rs 24,489	Needs Parts -Under process
3	Syringe Pump	Plenum tech	18/11/2020	Rs 24,489	Needs Parts -Under process
4	Syringe Pump	Plenum tech	18/11/2020	Rs 24,489	Needs Parts -Under process
5	Syringe Pump	Plenum tech	18/11/2020	Rs 24,489	Needs Parts -Under process
6	Syringe Pump	Plenum tech	18/11/2020	Rs 24,489	Needs Parts -Under process
7	Syringe Pump	Plenum tech	18/11/2020	Rs 24,489	Needs Parts -Under process
8	Monitor	BioNet	15/12/2020	Rs 1,64,052	Needs Parts -Under process

Equipment List - SVIMS Hospital

	Sl No	Index No		Department	C / NC	Equipment	Manufacturer	Model	Serial Num,ber	Supplier	War	War Start	War End	Purchased By	Status
1	1	SVIMS/cardio/08/2007/0001/C	IRS 2,56,03,586	**Cardiology**	**C**	**Cath Lab**	Philips	Allura	723	Philips	3Y	27.09.2018	30.09.2021	SVIMS	Working
2	2	SVIMS/cardio/05/2010/0002/NC	IRS 4,36,94,875	Cardiology	**NC**	**Cath Lab With Ablator & Stimulator**	Siemens	Artis Sensis	135430	Siemens	5Y	05-01-10	30/5/2015	PMSSY-HLL	Working
3	3	SVIMS/cardio/09/2002/0003/NC	IRS 37,31,550	Cardiology	**NC**	**Echo System**	Philips	Sonos 4500	US60210973	Philips	3Y	09-01-02	31/9/2005	SVIMS	Working
5	5	SVIMS/cardio/05/2008/0005/NC	IRS 57,99,957	Cardiology	**C**	**Echo System**	Philips	IE 33	O2XDG3	Philips	3Y	23-05-08	22/05/11	SVIMS	Working
6	6	SVIMS/cardio/06/2014/0006/NC	IRS 19,00,000	Cardiology	**NC**	**Echo System**	Esaote	MyLab25 Gold	7382	Esaote India	5Y	06-03-14	06-02-19	SVIMS	Working
7	7	SVIMS/cardio/06/2015/0007/NC	IRS 15,49,400	Cardiology	**NC**	**Echo System**	Esaote	MyLab 40	40-13075	Esaote India	3Y	06-01-15	31/05/2018	SVIMS	Working
8	8	SVIMS/cardio/01/2018/0008/C	Rs 3,25,000	Cardiology	C	Defibrillator	Philips	DFM 100	CN32610805	Alliance	1Y	01-10-18	01-09-19	SVIMS	Working
9	9	SVIMS/cardio/12/2003/0009/C	US$5812	Cardiology	C	Defibrillator	Philips	Heart Start XL	US00122519	Philips	3Y	18-12-03	17/02/06	SVIMS	Working
10	10	SVIMS/cardio/04/2010/0010/C	IRS 3,54,079	Cardiology	C	Defibrillator	Philips	Heart Start MRX	US00537834	Philips	2y	28/04/2010	27/04/2012	PMSSY-HLL	Working
11	11	SVIMS/cardio/09/2012/0011/C	IRS 2,96,595	Cardiology	C	Debifrillator	Medtronics	LifePak	40173623	Instromedix	2Y	21/09/12	20/09/14	PMSSY-HLL	Working
12	12	SVIMS/cardio/09/2012/0012/C	IRS 2,96,595	Cardiology	C	Debifrillator	Medtronics	LifePak	40173631	Instromedix	2Y	21/09/12	20/09/14	PMSSY-HLL	Working
13	13	SVIMS/cardio/06/2005/0013/C	US$6493	Cardiology	C	Patient Monitor	Philips	MP 20	DE50405111	Philips	3Y	20/06/05	19/06/08	SVIMS	Working
17	17	SVIMS/cardio/06/2005/0017/C	US$6493	Cardiology	C	Patient Monitor	Philips	MP 20	DE50405104	Philips	3Y	20/06/05	19/06/08	SVIMS	Working
18	18	SVIMS/cardio/06/2005/0018/C	US$6493	Cardiology	C	Patient Monitor	Philips	MP 20	DE50405110	Philips	3Y	20/06/05	19/06/08	SVIMS	Working
19	19	SVIMS/cardio/06/2005/0019/C	US$6493	Cardiology	C	Patient Monitor	Philips	MP 20	DE50405109	Philips	3Y	20/06/05	19/06/08	SVIMS	Working
20	20	SVIMS/cardio/06/2005/0020/C	US$6493	Cardiology	C	Patient Monitor	Philips	MP 20	DE50405095	Philips	3Y	20/06/05	19/06/08	SVIMS	Working
21	21	SVIMS/cardio/04/2010/0021/C	IRS 4,04,683	Cardiology	C	Multi Para Monitor	Mindray	Beneview T8	CF-99103984	Instromedic	2Y	04-02-10	04-01-12	PMSSY-HLL	Working
22	22	SVIMS/cardio/04/2010/0022/C	IRS 4,04,683	Cardiology	C	Multi Para Monitor	Mindray	Beneview T8	CF-99103985	Instromedic	2Y	04-02-10	04-01-12	PMSSY-HLL	Working
23	23	SVIMS/cardio/04/2010/0023/C	IRS 4,04,684	Cardiology	C	Multi Para Monitor	Mindray	Beneview T8	CF-99103996	Instromedic	2Y	04-02-10	04-01-12	PMSSY-HLL	Working
24	24	SVIMS/cardio/04/2010/0024/C	IRS 4,04,685	Cardiology	C	Multi Para Monitor	Mindray	Beneview T8	CF-99104002	Instromedic	2Y	04-02-10	04-01-12	PMSSY-HLL	Working
25	25	SVIMS/cardio/04/2010/0025/C	IRS 4,04,686	Cardiology	C	Multi Para Monitor	Mindray	Beneview T8	CF-99104019	Instromedic	2Y	04-02-10	04-01-12	PMSSY-HLL	Working
26	26	SVIMS/cardio/04/2010/0026/C	IRS 4,04,687	Cardiology	C	Multi Para Monitor	Mindray	Beneview T8	CF-99104022	Instromedic	2Y	04-02-10	04-01-12	PMSSY-HLL	Not Working
27	27	SVIMS/cardio/04/2010/0027/C	IRS 4,04,688	Cardiology	C	Multi Para Monitor	Mindray	Beneview T8	CF-9A104642	Instromedic	2Y	04-02-10	04-01-12	PMSSY-HLL	Working

28	28	SVIMS/cardio/04/2010/0028/C	IRS 4,04,689	Cardiology	C	Multi Para Monitor	Mindray	Beneview T8	CF-9A104647	Instromedic	2Y	04-02-10	04-01-12	PMSSY-HLL	Working
29	29	SVIMS/cardio/04/2010/0029/C	IRS 4,04,690	Cardiology	C	Multi Para Monitor	Mindray	Beneview T8	CF-9A104662	Instromedic	2Y	04-02-10	04-01-12	PMSSY-HLL	Working
30	30	SVIMS/cardio/09/2008/0030/NC	IRS 1,97,600	Cardiology	NC	Tread Mill System	Recorders	MARK II	V2-AH490	Recorders	2y	09-09-08	09-08-10	PMSSY-HLL	Working
31	31	SVIMS/cardio/03/2011/0031/NC	IRS 12,21,221	Cardiology	NC	Tread Mill System	Marquet	Case state TM2100	SBC104069070SA	Wipro GE	2Y	18/03/2011	17/03/2013	PMSSY-HLL	Working
32	32	SVIMS/cardio/03/2011/0032/NC	IRS 12,21,221	Cardiology	NC	Tread Mill System	Marquet	Case state TM2101	SBC104069 19SA	Wipro GE	2Y	18/03/2011	17/03/2013	PMSSY-HLL	Working
33	33	SVIMS/cardio/10/2007/0033/NC	US$13,585	Cardiology	NC	Hoter System	Delmer	Impreserio	LX17hhap5	Instromedix	3y	16/10/07	15/10/10	SVIMS	Working
34	34	SVIMS/cardio/11/2009/0035/NC	IRS 24,181	Cardiology	NC	Syringe Pump	Neuron BioMed	SP 102	0609-101	L & T	2Y	11-10-09	11-09-11	PMSSY-HLL	Working
35	35	SVIMS/cardio/11/2009/0036/NC	IRS 24,181	Cardiology	NC	Syringe Pump	Neuron BioMed	SP 102	0609-232	L & T	2Y	11-10-09	11-09-11	PMSSY-HLL	Working
36	36	SVIMS/cardio/11/2009/0038/NC	IRS 24,181	Cardiology	NC	Syringe Pump	Neuron BioMed	SP 102	0609-242	L & T	2Y	11-10-09	11-09-11	PMSSY-HLL	Working
37	37	SVIMS/cardio/11/2009/0039/NC	IRS 24,181	Cardiology	NC	Syringe Pump	Neuron BioMed	SP 102	0609-270	L & T	2Y	11-10-09	11-09-11	PMSSY-HLL	Working
38	38	SVIMS/cardio/11/2009/0040/NC	IRS 24,181	Cardiology	NC	Syringe Pump	Neuron BioMed	SP 102	0609-273	L & T	2Y	11-10-09	11-09-11	PMSSY-HLL	Working
39	39	SVIMS/cardio/11/2009/0041/NC	IRS 24,181	Cardiology	NC	Syringe Pump	Neuron BioMed	SP 102	0609-275	L & T	2Y	11-10-09	11-09-11	PMSSY-HLL	Working
40	40	SVIMS/cardio/11/2009/0043/NC	IRS 24,181	Cardiology	NC	Syringe Pump	Neuron BioMed	SP 102	0609-272	L & T	2Y	11-10-09	11-09-11	PMSSY-HLL	Working
41	41	SVIMS/cardio/02/2010/0044/NC	IRS 97,256	Cardiology	NC	ECG Recorder	Motorora	ELI-250	28271	Compamedic	2Y	02-06-10	02-05-12	PMSSY-HLL	Working
42	42	SVIMS/cardio/02/2010/0045/NC	IRS 97,256	Cardiology	NC	ECG Recorder	Motorora	ELI-250	28272	Compamedic	2Y	02-06-10	02-05-12	PMSSY-HLL	Working
43	43	SVIMS/cardio/02/2010/0046/NC	IRS 97,256	Cardiology	NC	ECG Recorder	Motorora	ELI-250	28276	Compamedic	2Y	02-06-10	02-05-12	PMSSY-HLL	Working
44	44	SVIMS/cardio/02/2010/0047/NC	IRS 97,256	Cardiology	NC	ECG Recorder	Motorora	ELI-250	28277	Compamedic	2Y	02-06-10	02-05-12	PMSSY-HLL	Working
45	45	SVIMS/cardio/11/2009/0048/C	IRS 11,18,928	Cardiology	C	ICU Ventilator	GE Datex Ohmeda	Engstrom	CBCN01004	GE Datex Ohmeda	2Y	30/11/2009	29/11/2011	PMSSY-HLL	Working
46	46	SVIMS/cardio/11/2009/0049/C	IRS 11,18,928	Cardiology	C	ICU Ventilator	GE Datex Ohmeda	Engstrom	CBCN01005	GE Datex Ohmeda	2Y	30/11/2009	29/11/2011	PMSSY-HLL	Working
47	47	SVIMS/cardio/11/2009/0050/C	IRS 11,18,928	Cardiology	C	ICU Ventilator	GE Datex Ohmeda	Engstrom	CBCN 01009	GE Datex Ohmeda	2Y	30/11/2009	29/11/2011	PMSSY-HLL	Working
48	48	SVIMS/cardio/11/2009/0051/NC	IRS 11,18,928	Cardiology	NC	ICU Ventilator	GE Datex Ohmeda	Engstrom	CBCN 01001	GE Datex Ohmeda	2Y	30/11/2009	29/11/2011	PMSSY-HLL	Working
49	49	SVIMS/cardio/06/2007/0052/C	US$ 38,500	Cardiology	NC	IABP	Datacope	CS300	SI281635F8	Maquet India	5 Y	28.11.2018	27.11.2023	SVIMS	Working
50	50	SVIMS/cardio/05/2012/0053/NC	IRS 24,500	Cardiology	NC	Syringe Pump	Orange Medical	Prima	1112351Z	Orange Medical	2Y	18/05/2012	17/05/2014	SVIMS	Working
51	51	SVIMS/cardio/05/2012/0054/NC	IRS 24,500	Cardiology	NC	Syringe Pump	Orange Medical	Prima	1112356Z	Orange Medical	2Y	18/05/2012	17/05/2014	SVIMS	Working
52	52	SVIMS/cardio/05/2012/0055/NC	IRS 24,500	Cardiology	NC	Syringe Pump	Orange Medical	Prima	1112358Z	Orange Medical	2Y	18/05/2012	17/05/2014	SVIMS	Working
53	53	SVIMS/cardio/05/2012/0056/NC	IRS 24,500	Cardiology	NC	Syringe Pump	Orange Medical	Prima	1112363Z	Orange Medical	2Y	18/05/2012	17/05/2014	SVIMS	Working
54	54	SVIMS/cardio/05/2	IRS 24,500	Cardiology	NC	Syringe Pump	Orange	Prima	1112361Z	Orange	2Y	18/05/20	17/05/2014	SVIMS	Working

		012/0057/NC					Medical			Medical		12			
55	55	SVIMS/cardio/05/2012/0058/NC	IRS 24,500	Cardiology	NC	Syringe Pump	Orange Medical	Prima	1112346-Z	Organge Medical	2Y	18/05/2012	17/05/2014	SVIMS	Working
56	56	SVIMS/cardio/05/2013/0059/NC	IRS 24,500	Cardiology	NC	Syringe Pump	Organge	Flow Prima	13050531-Z	Organge Medical	2Y	23/05/13	22/05/15	SVIMS	Working
57	57	SVIMS/cardio/05/2013/0060/NC	IRS 24,500	Cardiology	NC	Syringe Pump	Organge	Flow Prima	13050532-Z	Organge Medical	2Y	23/05/13	22/05/15	SVIMS	Working
58	58	SVIMS/cardio/05/2013/0061/NC	IRS 24,500	Cardiology	NC	Syringe Pump	Organge	Flow Prima	13050533-Z	Organge Medical	2Y	23/05/13	22/05/15	SVIMS	Working
59	59	SVIMS/cardio/05/2013/0062/NC	IRS 24,500	Cardiology	NC	Syringe Pump	Organge	Flow Prima	13050534-Z	Organge Medical	2Y	23/05/13	22/05/15	SVIMS	Working
60	60	SVIMS/cardio/05/2013/0063/NC	IRS 24,500	Cardiology	NC	Syringe Pump	Organge	Flow Prima	13050535-Z	Organge Medical	2Y	23/05/13	22/05/15	SVIMS	Working
61	61	SVIMS/cardio/05/2013/0064/NC	IRS 24,500	Cardiology	NC	Syringe Pump	Organge	Flow Prima	13050536-Z	Organge Medical	2Y	23/05/13	22/05/15	SVIMS	Working
62	62	SVIMS/cardio/05/2013/0065/NC	IRS 24,500	Cardiology	NC	Syringe Pump	Organge	Flow Prima	13050537-Z	Organge Medical	2Y	23/05/13	22/05/15	SVIMS	Working
63	63	SVIMS/cardio/05/2013/0066/NC	IRS 24,500	Cardiology	NC	Syringe Pump	Organge	Flow Prima	13050538-Z	Organge Medical	2Y	23/05/13	22/05/15	SVIMS	Working
64	64	SVIMS/cardio/05/2013/0067/NC	IRS 24,500	Cardiology	NC	Syringe Pump	Organge	Flow Prima	13050539-Z	Organge Medical	2Y	23/05/13	22/05/15	SVIMS	Working
65	65	SVIMS/cardio/05/2013/0068/NC	IRS 24,500	Cardiology	NC	Syringe Pump	Organge	Flow Prima	13050540-Z	Organge Medical	2Y	23/05/13	22/05/15	SVIMS	Working
66	66	SVIMS/cardio/12/2014/0069/NC	Reagent Rental	Cardiology	NC	Cardiac reader/Analyzer	RadioMeter	AQT90 FLEX	838R0200N0006	RadioMeter	-	12-11-14		Reagent rental	Working
67	67	SVIMS/cardio/12/2014/0070/NC	Reagent Rental	Cardiology	NC	Cardiac reader/Analyzer	RadioMeter	AQT90 FLEX	838R0273N0002	RadioMeter	-	12-11-14		Reagent rental	Working
68	68	SVIMS/cardio/03/2012/0071/NC	Rs20,75,625	Cardiology	NC	EO Gas sterilizer	Anderson	AN310	111762	Agama	5Y	28/03/2012	27/03/2017	SVIMS	Working
69	69	SVIMS/cardio/10/2009/0072/NC	IRS 4,04,250	Cardiology	NC	Deep Freezer - 40 Deg C	Terumo	Df40u	908115	Terumo	3Y	10-06-09	10-05-12	SVIMS	Working
70	70	SVIMS/cardio/06/2016/0073/NC	RS 75,00,000/-	Cardiology	NC	Intra Vaqscular Ultra Sound	Boston Scientic	Mdu MDU5Plus	32065	Lakshi	5Y	15/06/2016	14/06/2021	SVIMS	Working
71	71	SVIMS/cardio/03/2013/0074/NC	IRS 1,90,000	Cardiology	NC	Blood Pressure monitor	Kody Medical	TM 2655	2N0818813	Kody Medical	1Y	22/03/2013	21/03/2014	Donation	Working
72	72	SVIMS/cardio/08/2016/0075/NC	IRS23,08,950/-	Cardiology	NC	F F R	St Jude Medical	Quantian	Q01784	Excel	5Y	24/08/2016	23/08/2021	SVIMS	Working
73	73	SVIMS/cardio/02/2017/0076/NC	Rs.33,60,000/-	Cardiology	NC	Rotablator	Boston Scientic	RC5000	RC400921	Lakshi	5Y	16/02/2017	15/02/2022	SVIMS	Working
74	74	SVIMS/cardio/02/2017/0077/NC	IRs1,18,50,000	Cardiology	NC	Echo Machine	Siemens	SC2000	403018	Iris	5Y	02-01-17	31/01/2022	SVIMS	Working
75	75	SVIMS/cardio/03/2009/0078/NC	Euro 585	Cardiology-cath lab	NC	Syringe Pump	Fresenius	injectomat/Agilia	20497448					SVIMS	Working
76	76	SVIMS/cardio/02/2017/0079/NC		Cardiology-cath lab	NC	Syringe Pump	Plenum Tech Pvt Ltd	Zion+	1400					SVIMS	Working
77	77	SVIMS/cardio/02/2017/0080/NC		Cardiology-cath lab	NC	Syringe Pump	Plenum Tech Pvt Ltd	Zion+	1399					SVIMS	Working
78	78	SVIMS/cardio/00/2000/0081/NC		Cardiology-cath lab	NC	Syringe Pump	Bbraun	Perfusor Compact	63601					SVIMS	Working

79	79	SVIMS/Cardio/05/2013/1111/NC	IRS 6,40,500	Cardiology-cath lab	NC	Dicom Storage & Dicom CD/DVD		ML 110-G7		Cyone Med	3 Y	15.05.2013	14.05.2016	SVIMS	Working
80	80	SVIMS/Cardio/06/2018/1114/C	IRS 2,09,821	Cardiology-ICU	C	Defibrillator	Mindray		EI-84000505	Green Apple	5Y	07.06.2018	06.06.2023	SVIMS	Working
81	81	SVIMS/Cardio/05/2013/1115/C	IRS 2,09,821	Cardiology-cath lab	C	Defibrillator	Mindray		EI-84000843	Green Apple	5Y	07.06.2018	06.06.2023	SVIMS	Working
82	82	SVIMS/Cardio/06/2018/1126/C	Irs 1,20,000/-	Cardiology	C	ECG Recorder	GE Healthcare	MAC 2000	SRR18150307PA	Wipro GE	1Y	06-06-18	06-05-19	SVIMS	Working
83	83	SVIMS/Cardio/06/2018/1127/C	Irs 1,20,000/-	Cardiology	C	ECG Recorder	GE Healthcare	MAC 2000	SRR18150308PA	Wipro GE	1Y	06-06-18	06-05-19	SVIMS	Working
84	84	SVIMS/cardio/10/2018/1132 /NC		Cardiology	Nc	Ultrasound System	Philips	CX50	SG61800158	Philips	3 Y	05.10.2018	04.10.2021	SVIMS	Working
85	85	SVIMS/Cardio/02/2019/1141	Irs 1,20,000/-	Cardiology	NC	ECG Recorder	GE Healthcare	MAC 2000	SRR18420144PA	Wipro GE	1Y	02-02-19	02-01-20	SVIMS	Working
86	86	SVIMS/Cardio/06/2019/1176		Cardiology - ICU	NC	Syringe Pump	Smiths Medical	Grese by C9	18320 2889	M M Medical	5 Y	17.06.2019	16.06.2024	SVIMS	Working
87	87	SVIMS/Cardio/06/2019/1177		Cardiology - ICU	NC	Syringe Pump	Smiths Medical	Grese by C9	18320 2922	M M Medical	5 Y	17.06.2019	16.06.2024	SVIMS	Working
88	88	SVIMS/Cardio/06/2019/1178		Cardiology - ICU	NC	Syringe Pump	Smiths Medical	Grese by C9	18320 2910	M M Medical	5 Y	17.06.2019	16.06.2024	SVIMS	Working
89	89	SVIMS/Cardio/06/2019/1179		Cardiology - ICU	NC	Syringe Pump	Smiths Medical	Grese by C9	18320 2912	M M Medical	5 Y	17.06.2019	16.06.2024	SVIMS	Working
90	90	SVIMS/Cardio/06/2019/1180		Cardiology - ICU	NC	Syringe Pump	Smiths Medical	Grese by C9	18320 2805	M M Medical	5 Y	17.06.2019	16.06.2024	SVIMS	Working
91	91	SVIMS/Cardio/06/2019/1181		Cardiology - ICU	NC	Syringe Pump	Smiths Medical	Grese by C9	18320 2808	M M Medical	5 Y	17.06.2019	16.06.2024	SVIMS	Working
92	92	SVIMS/Cardio/06/2019/1182		Cardiology - ICU	NC	Syringe Pump	Smiths Medical	Grese by C9	18320 2904	M M Medical	5 Y	17.06.2019	16.06.2024	SVIMS	Working
93	93	SVIMS/Cardio/06/2019/1183		Cardiology - ICU	NC	Syringe Pump	Smiths Medical	Grese by C9	18320 2896	M M Medical	5 Y	17.06.2019	16.06.2024	SVIMS	Working
94	94	SVIMS/Cardio/06/2019/1184		Cardiology - ICU	NC	Syringe Pump	Smiths Medical	Grese by C9	18320 2906	M M Medical	5 Y	17.06.2019	16.06.2024	SVIMS	Working
95	95	SVIMS/Cardio/06/2019/1185		Cardiology - ICU	NC	Syringe Pump	Smiths Medical	Grese by C9	18320 2897	M M Medical	5 Y	17.06.2019	16.06.2024	SVIMS	Working
96	96	SVIMS/Cardio/06/2019/1186		Cardiology - ICU	NC	Syringe Pump	Smiths Medical	Grese by C9	18320 2911	M M Medical	5 Y	17.06.2019	16.06.2024	SVIMS	Working
97	97	SVIMS/Cardio/06/2019/1187		Cardiology - ICU	NC	Syringe Pump	Smiths Medical	Grese by C9	18320 2925	M M Medical	5 Y	17.06.2019	16.06.2024	SVIMS	Working
98	98	SVIMS/Cardio/06/2019/1188		Cardiology - ICU	NC	Syringe Pump	Smiths Medical	Grese by C9	18320 2894	M M Medical	5 Y	17.06.2019	16.06.2024	SVIMS	Working
99	99	SVIMS/Cardio/06/2019/1189		Cardiology - ICU	NC	Syringe Pump	Smiths Medical	Grese by C9	18320 2909	M M Medical	5 Y	17.06.2019	16.06.2024	SVIMS	Working
100	100	SVIMS/Cardio/06/2019/1190		Cardiology - ICU	NC	Syringe Pump	Smiths Medical	Grese by C9	18320 2892	M M Medical	5 Y	17.06.2019	16.06.2024	SVIMS	Working
101	101	SVIMS/Cardio/00/0000/1229		Cardiology	NC	Syringe Pump	Neuron BioMed	SP 102	0610 101						
102	102	SVIMS/Cardio/00/0000/1230		Cardiology Cath Lab	NC	ECG Recorder	Motorora	ELI-250	1094200 2827528271						
103	103	SVIMS/Cardio/00/0000/1231		Cardiology	NC	ECG Recorder	GE	MAC 1200ST	550048031						
104	104	SVIMS/Cardio/00/0000/1232		Cardiology	NC	Defibrillator	Philips	Heart start XL	Usoo452722						

105	105	SVIMS/Cardio/02/2012/1233		Cardiology	NC	Pulse Oximeter	Mediaid	900P	E49G00165	Adv. Micronic	2Y	02-06-10	02-05-12	PMSSY-HLL	
106	106	SVIMS/Cardio/02/2012/1234		Cardiology	NC	Pulse Oximeter	Mediaid	900P	E49G00198	Adv. Micronic	2Y	02-06-10	02-05-12	PMSSY-HLL	
107	107	SVIMS/Cardio/02/2012/1235		Cardiology	NC	Pulse Oximeter	Mediaid	900P	E49G00197	Adv. Micronic	2Y	02-06-10	02-05-12	PMSSY-HLL	
108	108	SVIMS/Cardio/02/2012/1236		Cardiology	NC	Pulse Oximeter	Mediaid	900P	E49G00175	Adv. Micronic	2Y	02-06-10	02-05-12	PMSSY-HLL	
109	109	SVIMS/Cardio/02/2012/1237		Cardiology	NC	TMT	RMS	MARK 11	V2AH490	Recor der & Medicare	2Y	02-06-10	02-05-12	PMSSY-HLL	
110	110	SVIMS/Cardio/ /2020/1321		Cardiology		Multi Para Monitor	Schiller	Truscope III	M080002373	Schiller India	5Y				
111	111	SVIMS/Cardio/ /2020/1322		Cardiology		Multi Para Monitor	Schiller	Truscope III	M080002374	Schiller India	5Y				
112	112	SVIMS/Cardio/ /2020/1323		Cardiology		Multi Para Monitor	Schiller	Truscope III	M080002375	Schiller India	5Y				
113	113	SVIMS/Cardio/ /2020/1324		Cardiology		Multi Para Monitor	Schiller	Truscope III	M080002376	Schiller India	5Y				
114	114	SVIMS/Cardio/ /2020/1325		Cardiology		Multi Para Monitor	Schiller	Truscope III	M080002377	Schiller India	5Y				
115	115	SVIMS/Cardio/ /2020/1326		Cardiology		Multi Para Monitor	Schiller	Truscope III	M080002378	Schiller India	5Y				
116	116	SVIMS/Cardio/ /2020/1327		Cardiology		Multi Para Monitor	Schiller	Truscope III	M080002379	Schiller India	5Y				
117	117	SVIMS/Cardio/ /2020/1328		Cardiology		Multi Para Monitor	Schiller	Truscope III	M080002380	Schiller India	5Y				
118	1	SVIMS/Nephro/01/2009/0085/C		Nephrology		Dialysis Machine	Fresenius	4008S	8VCALF06	Trivitron	3Y	01-07-09	01-06-12	SVIMS	Working
119	2	SVIMS/Nephro/01/2009/0086/C	US$10,625	Nephrology	c	Dialysis Machine	Fresenius	4008S	8VCALF07	Trivitron	3Y	01-07-09	01-06-12	SVIMS	Working
120	3	SVIMS/Nephro/01/2009/0087/C	US$10,625	Nephrology	c	Dialysis Machine	Fresenius	4008S	8VCALF73	Trivitron	3Y	01-07-09	01-06-12	SVIMS	Working
121	4	SVIMS/Nephro/01/2009/0088/C	US$10,625	Nephrology	c	Dialysis Machine	Fresenius	4008S	8V5AK532	Trivitron	3Y	01-07-09	01-06-12	SVIMS	Working
122	5	SVIMS/Nephro/01/2009/0089/C	US$10,625	Nephrology	c	Dialysis Machine	Fresenius	4008S	8V5AK531	Trivitron	3Y	01-07-09	01-06-12	SVIMS	Working
123	6	SVIMS/Nephro/09/2010/0090/C	Rs 6,42,015	Nephrology	c	Dialysis Machine	Fresenius	4008S	OVCAQST80	Fresenius India	5Y	22/09/2010	21/09/2015	SVIMS	Working
124	7	SVIMS/Nephro/09/2010/0091/C	Rs 6,42,015	Nephrology	c	Dialysis Machine	Fresenius	4008S	OVCAST71	Fresenius India	5Y	22/09/2010	21/09/2015	SVIMS	Working
125	8	SVIMS/Nephro/09/2010/0092/C	Rs 6,42,015	Nephrology	c	Dialysis Machine	Fresenius	4008S	OVCASW34	Fresenius India	5Y	22/09/2010	21/09/2015	SVIMS	Working
126	9	SVIMS/Nephro/09/2010/0093/C	Rs 6,42,015	Nephrology	c	Dialysis Machine	Fresenius	4008S	0VCAST58	Fresenius India	5Y	22/09/2010	21/09/2015	SVIMS	Working
127	10	SVIMS/Nephro/09/2010/ 0094/C	Rs 6,42,015	Nephrology	c	Dialysis Machine	Fresenius	4008S	OVCASW16	Fresenius India	5Y	22/09/2010	21/09/2015	SVIMS	Working
128	11	SVIMS/Nephro/09/2010/ 0095/C	Rs 6,42,015	Nephrology	c	Dialysis Machine	Fresenius	Art Plus	OVRA0470	Fresenius India	5Y	22/09/2010	21/09/2015	SVIMS	Working
129	12	SVIMS/Nephro/03/2013/0096/C	Rs 523000	Nephrology	c	Dialysis Machine	Fresenius	4008S	2SXAB696	Fresenius India	5Y	14/03/2013	13/03/2018	SVIMS	Working
130	13	SVIMS/Nephro/03/2013/0097/C	Rs 523000	Nephrology	c	Dialysis Machine	Fresenius	4008S	2SXAB700	Fresenius India	5Y	14/03/2013	13/03/2016	SVIMS	Working
131	14	SVIMS/Nephro/03/	Rs 523000	Nephrology	c	Dialysis	Fresenius	4008S	2SXAB702	Fresenius	5Y	14/03/20	13/03/2016	SVIMS	Working

		2013/0098/C				Machine				India		13			
132	15	SVIMS/Nephro/03/ 2013/ 0099/C	Rs 523000	Nephrology	c	Dialysis Machine	Fresenius	4008S	2SXAB703	Fresenius India	5Y	14/03/20 13	13/03/2016	SVIMS	Working
133	16	SVIMS/Nephro/03/ 2013/ 0100/C	Rs 523000	Nephrology	c	Dialysis Machine	Fresenius	4008S	2SXAB704	Fresenius India	5Y	14/03/20 13	13/03/2016	SVIMS	Working
134	17	SVIMS/Nephro/03/ 2013/ 0101/C	Rs 523000	Nephrology	c	Dialysis Machine	Fresenius	4008S	2SXAB705	Fresenius India	5Y	14/03/20 13	13/03/2016	SVIMS	Working
135	18	SVIMS/Nephro/03/ 2013/ 0102/C	Rs 523000	Nephrology	c	Dialysis Machine	Fresenius	4008S	2SXAB706	Fresenius India	5Y	14/03/20 13	13/03/2016	SVIMS	Working
136	19	SVIMS/Nephro/03/ 2013/ 0103/C	Rs 523000	Nephrology	c	Dialysis Machine	Fresenius	4008S	2SXAB707	Fresenius India	5Y	14/03/20 13	13/03/2016	SVIMS	Working
137	20	SVIMS/Nephro/03/ 2013/0104/C	Rs 523000	Nephrology	c	Dialysis Machine	Fresenius	4008S	2SXAB708	Fresenius India	5Y	14/03/20 13	13/03/2016	SVIMS	Working
138	21	SVIMS/Nephro/03/ 2013/ 0105/C	Rs 523000	Nephrology	c	Dialysis Machine	Fresenius	4008S	2SXAB709	Fresenius India	5Y	14/03/20 13	13/03/2016	SVIMS	Working
139	22	SVIMS/Nephro/07/ 2012/0106/C	Rs5,75,000	Nephrology	c	Dialysis Machine	Fresenius	4008S	2SXAB498	Fresenius India	3Y	28/07/20 12	27/07/2015	SVIMS	Working
140	23	SVIMS/Nephro/07/ 2012/ 0107/C	Rs5,75,000	Nephrology	c	Dialysis Machine	Fresenius	4008S	2SXAB499	Fresenius India	3Y	28/07/20 12	27/07/2015	SVIMS	Working
141	24	SVIMS/Nephro/04/ 2012/0108/NC	Rs6,50,000	Nephrology	c	Dialysis Machine	Fresenius	ARTPLUS	1VRAO745	Trivitron	2Y	18/04/20 12	17/04/2014	SVIMS	Working
142	25	SVIMS/Nephro/12/ 2014/ 0109/NC		Nephrology	c	Dialysis Machine	Fresenius	Art Plus	4VRAO925	Fresenius India	5Y	12-10-14	12-09-19	SVIMS	Working
143	26	SVIMS/Nephro/04/ 2012/0110/C	IRS 8,09,524	Nephrology	c	CRRT	GAMBRO	PRISMAFLE X	4752	Gambro India	2y	04-04-12	04-03-14	SVIMS	Working
144	27	SVIMS/Nephro/07/ 2015/0111/C	IRS 8,09,524	Nephrology	c	CRRT	GAMBRO	PRISMAFLE X	14942	Gambro India	1Y	07-02-15	07-01-16	Donati on	Working
145	28	SVIMS/Nephro/07/ 2015/0112/NC		Nephrology	NC	PD CYCLER	Baxter	R5C 8320	620010	Gambro India	1y	07-02-15	07-01-16	SVIMS	Working
146	29	SVIMS/Nephro/03/ 2010/0113/NC	IRS 3,74,063	Nephrology	NC	PD CYCLER	Baxter	R5C 8320	621109	HC Pro cycler	1y	24/03/10	23/03/11	SVIMS	Working
147	30	SVIMS/Nephro/02/ 2014/0114/NC	IRS 3,74,063	Nephrology	NC	PD CYCLER	Baxter	R5C 8320	301349	Banafar pharma	1Y	24/2/201 4	23/2/2015	SVIMS	Working
148	31	SVIMS/Nephro/12/ 2008/0115/C	IRS 1,29,150	Nephrology	C	Defibrillator	BPL	DF 2509R	AAMD4H2 240	Bharat Medi	1Y	12-12-08	12-11-09	SVIMS	Working
149	32	SVIMS/Nephro/12/ 2008/0116/C	IRS 1,29,150	Nephrology	C	Defibrillator	BPL	DF 2509R	BYMD7J2 812	Bharat Medi	1Y	12-12-08	12-11-09	SVIMS	Working
150	33	SVIMS/Nephro/02/ 2014/ 0117/NC	IRS 85,000	Nephrology	NC	Bi-Corb Mixer	SR Med	200L		SR Med	1Y	02-01-14	31/1/2015	SVIMS	Working
151	34	SVIMS/Nephro/02/ 2005/0118/NC	IRS 85,000	Nephrology	NC	Bi-Corb Mixer	SR Med	200L		SR Med	3Y	02-01-05	31/1/2008	SVIMS	Working
152	35	SVIMS/Nephro/10/ 1998/0119/NC		Nephrology	NC	Digital Weighing Scale	Tulaman	115Es		Tulaman	1Y	28/10/98	27/10/99	SVIMS	Working
153	36	SVIMS/Nephro/09/ 2005/0120/NC		Nephrology	NC	Digital Weighing Scale	Tulaman	115Es		Tulaman	1Y	21/09/05	20/09/06	SVIMS	Working
154	37	SVIMS/Nephro/11/ 2009/0121/C	IRS 11,18,928	Nephrology	C	ICU Ventilator	GE Datex Ohmeda	Anaesthesia	CBCN 00998	Engstrom	2Y	30/11/20 09	29/11/2011	PMSS Y-HLL	Working
155	38	SVIMS/Nephro/11/ 2010/0122/C	IRS 11,18,928	Nephrology	C	ICU Ventilator	GE Datex Ohmeda	Anaesthesia	CBCN 00999	Engstrom	2Y	30/11/20 10	29/11/2011	PMSS Y-HLL	**Workin g**
156	39	SVIMS/Nephro/11/ 2009/0123/NC	IRS 24,181	Nephrology	NC	Syringe Pump	Neuron BioMed	SP 102		L & T	2Y	11-02-09	11-01-11	PMSS Y-HLL	Working
157	40	SVIMS/Nephro/11/2009/0124/NC			IRS 24,1	Nephrology	NC	Syringe Pump	Neuron BioMed	SP 102		L & T	2Y	11-02-09	11-01-11

					81										
158	41	SVIMS/Nephro/04/ 2010/0125/C	IRS 4,04,683	Nephrology	c	Multi Para Monitor	Mindray	Beneview T8	CF-99104018	Instromedic	2Y	04-02-10	04-01-12	PMSSY-HLL	Working
159	42	SVIMS/Nephro/04/ 2010/0126/	IRS 4,04,683	Nephrology	c	Multi Para Monitor	Mindray	Beneview T8	CF-99104016	Instromedic	2Y	04-02-10	04-01-12	PMSSY-HLL	Working
160	43	SVIMS/Nephro/04/ 2010/0127	IRS 4,04,683	Nephrology	c	Multi Para Monitor	Mindray	Beneview T8	CF-99104001	Instromedic	2Y	04-02-10	04-01-12	PMSSY-HLL	Working
161	44	SVIMS/Nephro/04/ 2010/0128	IRS 4,04,683	Nephrology	c	Multi Para Monitor	Mindray	Beneview T8	CF-99104655	Instromedic	2Y	04-02-10	04-01-12	PMSSY-HLL	Working
162	45	SVIMS/Nephro/04/ 2010/0129	IRS 4,04,683	Nephrology	c	Multi Para Monitor	Mindray	Beneview T8	CF-99103988	Instromedic	2Y	04-02-10	04-01-12	PMSSY-HLL	Working
163	46	SVIMS/Nephro/04/ 2010/0130	IRS 4,04,683	Nephrology	c	Multi Para Monitor	Mindray	Beneview T8	CF-99104011	Instromedic	2Y	04-02-10	04-01-12	PMSSY-HLL	Working
164	47	SVIMS/Nephro/04/ 2010/0131	IRS 4,04,683	Nephrology	c	Multi Para Monitor	Mindray	Beneview T8	CF-99103979	Instromedic	2Y	04-02-10	04-01-12	PMSSY-HLL	Working
165	48	SVIMS/Nephro/04/ 2010/0132	IRS 4,04,683	Nephrology	c	Multi Para Monitor	Mindray	Beneview T8	CF-99103998	Instromedic	2Y	04-02-10	04-01-12	PMSSY-HLL	Working
166	49	SVIMS/Nephro/11/ 2014/0133	IRS 97,500	Nephrology	c	Microscope	Nikon	E-200	610543	Towa Optics	1Y	14/11/2014	13/11/2015	SVIMS	Working
167	50	SVIMS/Nephro/11/ 2014/0134	IRS 19,00,000	Nephrology	NC	Ultra Sound Scanner	Esote	MyLab 25 Gold	3867	Esote India	5Y	12-03-15	12-02-20	SVIMS	Working
168	51	SVIMS/Nephro/06/ 2016/0135	Rs 29,252.71	Nephrology	NC	Syringe Pump	Plenum Tech Pvt Ltd	Zion +	1834	Plenum Tech	3Y	15/06/2016	14/06/2018	SVIMS	Working
169	52	SVIMS/Nephro/06/ 2016/0136	Rs 29,252.71	Nephrology	NC	Syringe Pump	Plenum Tech Pvt Ltd	Zion +	1423	Plenum Tech	3Y	15/06/2016	14/06/2018	SVIMS	Working
170	53	SVIMS/Nephro/06/ 2016/0137	Rs 29,252.71	Nephrology	NC	Syringe Pump	Plenum Tech Pvt Ltd	Zion +	1424	Plenum Tech	3Y	15/06/2016	14/06/2018	SVIMS	Working
171	54	SVIMS/Nephro/11/ 2009/0138	IRS 24,181	Nephrology	NC	Syringe Pump	Neuron BioMed	SP 102	0609-230	L & T	2Y	11-04-09	11-03-11	PMSSY-HLL	Working
172	55	SVIMS/Nephro/02/ 2010/0139	IRS 97,256	Nephrology	NC	ECG Recorder	Motorora	ELI-250	28269	Compamedic	2Y	02-06-10	02-05-12	PMSSY-HLL	Working
173	56	SVIMS/Nephro/02/ 2010/0140	IRS37,146	Nephrology	NC	Pulse Oximeter	Mediaid	900P	EGo9G00172	Adv. Micronic	2Y	02-06-10	02-05-12	PMSSY-HLL	Working
174	57	SVIMS/Nephro/02/ 2010/0141	IRS37,146	Nephrology	NC	Pulse Oximeter	Mediaid	900P	EGo9G00177	Adv. Micronic	2Y	02-06-10	02-05-12	PMSSY-HLL	Working
175	58	SVIMS/Nephro/02/ 2010/0142	IRS37,146	Nephrology	NC	Pulse Oximeter	Mediaid	900P	EGo9G00178	Adv. Micronic	2Y	02-06-10	02-05-12	PMSSY-HLL	Working
176	59	SVIMS/Nephro/02/ 2010/0143	IRS37,146	Nephrology	NC	Pulse Oximeter	Mediaid	900P	**EGO9G00199**	Adv. Micronic	2Y	02-06-10	02-05-12		Working
177	60	SVIMS/Nephro/02/ 2010/0144		Nephrology	NC	Syringe Pump	Organge	Flow Prima	13051373Z						
178	61	SVIMS/Nephro/06/ 2019/1191		Nephrology-Medicine Ward	NC	Syringe Pump	Smiths Medical	Grase by C9	183200263	M M Medical	5 Y	17.06.2019	16.06.2024	SVIMS	Working
179	62	SVIMS/Nephro/06/ 2019/1192		Nephrology-Medicine Ward	NC	Syringe Pump	Smiths Medical	Grase by C9	183202919	M M Medical	5 y	17.06.2019	16.06.2024	SVIMS	Working
180	63	SVIMS/Nephro/09/ 2019/1214		Nephrology	C	Defibrillator	BPL Medical	DF 2509 R	BZMN8C5874	Mukta Medi	1 Y	09.09.2019	08.09.2020	SVIMS	Working
181	1	SVIMS/Neurol/07/2005/0145/M	INR 41,04,797/-	**Neurology**	NC	**EEG Video Digital-128 Channel**	EB Neuro	Gaiieo 128	51	Shibumi	3Y	16/07/05	15-07-08	SVIMS	Working

182	2	SVIMS/Neurol/01/2015/0147	IRS 18,99,000	Neurology	NC	**EEG Video 40 Channel**	EB Neuro	Gaiieo Mizar 40	22514	Shibumi	5Y	01-01-15	31-12-2019	SVIMS	Working
183	3	SVIMS/M/Neurol/09/2009/0148/M			Rs.37,90,000/-	Neurology	NC	**8 Channel ENMG**	Nicolet	Medelec Synngy	90790	Allied	3Y	09-11-09	08-10-12
184	4	SVIMS/Neurol/05/2015/0149/M	Rs 66,01,754/-	Neurology	NC	**ENMG**	Nicolet	Medelec Synngy	RZ 154587G	Allied	5y	05-06-15	05-05-20	SVIMS	Working
185	5	SVIMS/Neurol/09/2009/0150/M	IRS 33,72,875	Neurology	NC	**Trans cranial Mag. Stimulator**		Magstim rapid 2	c0514/a0205	HospiMedical	3Y	26/09/09	25/09/2012	PMSSY-APHMHIDC	Working
186	6	SVIMS/Neurol/11/2009/0151/C	IRS 11,18,928	Neurology	C	**ICU Ventilator**	GE Datex Ohmeda	Engstrom	CBCN01012	Mindray	2Y	30/11/2009	29/11/2011	PMSSY-HLL	Working
187	7	SVIMS/Neurol/11/2009/0152/C	IRS 11,18,928	Neurology	C	**ICU Ventilator**	GE Datex Ohmeda	Engstrom	CBCN01014	Mindray	2Y	30/11/2009	29/11/2011	PMSSY-HLL	Working
188	8	SVIMS/Neurol/11/2009/0153/C	IRS 11,18,928	Neurology	C	**ICU Ventilator**	GE Datex Ohmeda	Engstrom	CBCN00997	Mindray	2Y	30/11/2009	29/11/2011	PMSSY-HLL	Working
189	9	SVIMS/Neurol/11/2009/0154/C	IRS 11,18,928	Neurology	C	**ICU Ventilator**	GE Datex Ohmeda	Engstrom	CBCN00995	Mindray	2Y	30/11/2009	29/11/2011	PMSSY-HLL	Working
190	10	SVIMS/Neurol/02/2010/0155	IRS 4,04,683	Neurology	c	Multi Para Monitor	Mindray	Beneview T8	CF-99103983	Instromedic	2Y	02-04-10	01-03-12	PMSSY-HLL	Working
191	11	SVIMS/Neurol/02/2010/0156	IRS 4,04,683	Neurology	c	Multi Para Monitor	Mindray	Beneview T8	CF-99103977	Instromedic	2Y	02-04-10	01-03-12	PMSSY-HLL	Working
192	12	SVIMS/Neurol/02/2010/0157	IRS 4,04,683	Neurology	c	Multi Para Monitor	Mindray	Beneview T8	CF-99103972	Instromedic	2Y	02-04-10	01-03-12	PMSSY-HLL	Working
193	13	SVIMS/Neurol/02/2010/0158	IRS 4,04,683	Neurology	c	Multi Para Monitor	Mindray	Beneview T8	CF-99104021	Instromedic	2Y	02-04-10	01-03-12	PMSSY-HLL	Working
194	14	SVIMS/Neurol/02/2010/0159	IRS 4,04,683	Neurology	c	Multi Para Monitor	Mindray	Beneview T8	CF-99104020	Instromedic	2Y	02-04-10	01-03-12	PMSSY-HLL	Working
195	15	SVIMS/Neurol/02/2010/0160	IRS 4,04,683	Neurology	c	Multi Para Monitor	Mindray	Beneview T8	CF-99104023	Instromedic	2Y	02-04-10	01-03-12	PMSSY-HLL	Working
196	16	SVIMS/Neurol/02/2010/0161	IRS 4,04,683	Neurology	c	Multi Para Monitor	Mindray	Beneview T8	CF-99104000	Instromedic	2Y	02-04-10	01-03-12	PMSSY-HLL	Working
197	17	SVIMS/Neurol/02/2010/0162	IRS 4,04,683	Neurology	c	Multi Para Monitor	Mindray	Beneview T8	CF-99104024	Instromedic	2Y	02-04-10	01-03-12	PMSSY-HLL	Working
198	18	SVIMS/Neurol/06/2016/0163	RS 18, 99, 000/-	Neurology	NC	EEG Video 40 Channel	EB Neuro	Gaiieo Mizar 40	22526	Shibumi	5Y	13/06/2016	06-12-21	SVIMS	Working
199	19	SVIMS/Neurol/02/2009/0164	IRS 7,87,050/-	Neurology	C	Defibrillator	BPL	DF2509	BYMD9A3629	BPL	1Y	02-06-09	01-05-10	SVIMS	Working
200	20	SVIMS/Neurol/03/2009/0165	Euro585	Neurology	NC	Syringe Pump	Fresenius	Injectomat/Agilia	20497421	Medi	5Y	19/03/09	18-03-14	SVIMS	Working
201	21	SVIMS/Neurol/03/2009/0166	Euro585	Neurology	NC	Syringe Pump	Fresenius	Injectomat/Agilia	20497450	Medi	5y	19/03/09	18-03-14	SVIMS	Working
202	22	SVIMS/Neuolr/03/2009/0167	Euro585	Neurology	NC	Syringe Pump	Fresenius	Injectomat/Agilia	20497462	Medi	5Y	19/03/09	18-03-14	SVIMS	Working
203	23	SVIMS/Neurol/03/2009/0168	Euro585	Neurology	NC	Syringe Pump	Fresenius	Injectomat/Agilia	20497427	Medi	5y	19/03/09	18-03-14	SVIMS	Working
204	24	SVIMS/Neurol/03/2009/0169	Euro585	Neurology	NC	Syringe Pump	Fresenius	Injectomat/Agilia	20497439	Medi	5Y	19/03/09	18-03-14	SVIMS	Working
205	25	SVIMS/Neurol/03/2009/0170	Euro585	Neurology	NC	Syringe Pump	Fresenius	Injectomat/Agilia	20497459	Medi	5Y	19/03/09	18-03-14	SVIMS	Working
206	26	SVIMS/Neurol/01/2020/1276	Euro585	ANCU - Neurology		Syringe Pump	Smiths Medical	Grese by C9	18320 2956	M M Medical	5Y	06.01.2020	05.01.2025	SVIMS	Working

207	27	SVIMS/Neurol/01/2020/1320		Neurology		Infusion Pump	Minday	BenefusionVP1	SK-90605744	Green Apple	5Y	27.01.2020	26.01.2025	SVIMS	Working
208	1	SVIMS/casual/02/2003/0172		**Casuality**	**C**	Defibrillator	Philips	Heart start	US 122180	Philips	3y	18-02-03	17/02/06	SVIMS	Working
209	2	SVIMS/casual/04/2014/0173	IRS 2,69.500	Casuality	C	Defibrillator	Schiller	Defigard-400	J14Bo67	Schiller	2Y	04-02-14	04-01-16	SVIMS	Working
210	3	SVIMS/casual/02/2010/0174	IRS 4,04,683	Casuality	c	Multi Para Monitor	Mindray	PM-8000	AA-99121311	Instromedic	2y	02-07-10	02-06-12	PMSSY-HLL	Working
211	4	SVIMS/casual/02/2010/0175	IRS 4,04,683	Casuality	c	Multi Para Monitor	Mindray	PM-8000	AA-99121312	Instromedic	2y	02-07-10	02-06-12	PMSSY-HLL	Working
212	5	SVIMS/casual/02/2010/0176	IRS 4,04,683	Casuality	c	Multi Para Monitor	Mindray	PM-8000	AA-99121314	Instromedic	2y	02-07-10	02-06-12	PMSSY-HLL	Working
213	6	SVIMS/casual/02/2010/0177	IRS 4,04,683	Casuality	c	Multi Para Monitor	Mindray	PM-8000	AA-99121315	Instromedic	2y	02-07-10	02-06-12	PMSSY-HLL	Working
214	7	SVIMS/casual/02/2010/0178	IRS 4,04,683	Casuality	c	Multi Para Monitor	Mindray	PM-8000	AA-99121316	Instromedic	2y	02-07-10	02-06-12	PMSSY-HLL	Working
215	8	SVIMS/casual/02/2010/0179	IRS 4,04,683	Casuality	c	Multi Para Monitor	Mindray	PM-8000	AA-99121317	Instromedic	2y	02-07-10	02-06-12	PMSSY-HLL	Working
216	9	SVIMS/casual/02/2010/0180	IRS 4,04,683	Casuality	c	Multi Para Monitor	Mindray	PM-8000	AA-99121318	Instromedic	2y	02-07-10	02-06-12	PMSSY-HLL	Working
217	10	SVIMS/Caual/10/2011/0181/C	IRS 11,18,929	Casuality	C	**ICU Ventilator**	Tecme	Grpahnet	9101 114 1080	Meditronic	2y	10-01-11	31/09/2013	PMSSY-HLL	Working
218	11	SVIMS/Casual/10/2011/0182/C	IRS 11,18,929	Casuality	C	**ICU Ventilator**	Tecme	Grpahnet	9101 126 1080	Meditronic	2y	10-01-11	31/09/2013	PMSSY-HLL	Working
219	12	SVIMS/Casual/10/2011/0183/C	IRS 11,18,929	Casuality	C	**ICU Ventilator**	Tecme	Grpahnet	9101 105 1080	Meditronic	2y	10-01-11	31/09/2013	PMSSY-HLL	Working
220	13	SVIMS/Casual/10/2011/0184/C	IRS 11,18,929	Casuality	C	**ICU Ventilator**	Tecme	Grpahnet	9101 120 1080	Meditronic	2y	10-01-11	31/09/2013	PMSSY-HLL	Working
221	14	SVIMS/Casual/11/2009/0185	IRS 24,181	Casuality	NC	Syringe Pump	Neuron BioMed	SP 102	0609-185	L & T	2Y	11-04-09	11-03-11	PMSSY-HLL	Working
222	15	SVIMS/Casual/11/2009/0186	IRS 24,181	Casuality	NC	Syringe Pump	Neuron BioMed	SP 102	0609-225	L & T	2Y	11-04-09	11-03-11	PMSSY-HLL	Working
223	16	SVIMS/Casual/11/2009/0189	IRS 24,181	Casuality	NC	Syringe Pump	Neuron BioMed	SP 102	0609-234	L & T	2Y	11-04-09	11-03-11	PMSSY-HLL	Working
224	17	SVIMS/Casual/11/2009/0192	IRS 24,181	Casuality	NC	Syringe Pump	Neuron BioMed	SP 102	0609-276	L & T	2Y	11-04-09	11-03-11	PMSSY-HLL	Working
225	18	SVIMS/Casual/11/2009/0193	IRS 24,181	Casuality	NC	Syringe Pump	Neuron BioMed	SP 102	0609-282	L & T	2Y	11-04-09	11-03-11	PMSSY-HLL	Working
226	19	**SVIMS/casual/11/2009/0194**	IRS 24,181	Casuality	NC	Syringe Pump	Neuron BioMed	SP 102	0609-283	L & T	2Y	11-04-09	11-03-11	PMSSY-HLL	Working
227	20	SVIMS/casual/04/2014/0195	IRS 24,500	Casuality	NC	Syringe Pump	Organge	Flow Prima	14026008-Z	Organge Medical	2Y	04-02-14	04-01-16	SVIMS	Working
228	21	SVIMS/casual/04/2014/0196	IRS 24,500	Casuality	NC	Syringe Pump	Organge	Flow Prima	14026009-Z	Organge Medical	2Y	04-02-14	04-01-16	SVIMS	Working
229	22	SVIMS/casual/04/2014/0197	IRS 24,500	Casuality	NC	Syringe Pump	Organge	Flow Prima	14026010-Z	Organge Medical	2Y	04-02-14	04-01-16	SVIMS	Working
230	23	SVIMS/casual/04/2014/0198	IRS 24,500	Casuality	NC	Syringe Pump	Organge	Flow Prima	14026011-Z	Organge Medical	2Y	04-02-14	04-01-16	SVIMS	Working
231	24	SVIMS/casual/04/2014/0199	IRS 24,500	Casuality	NC	Syringe Pump	Organge	Flow Prima	14026012-Z	Organge Medical	2Y	04-02-14	04-01-16	SVIMS	Working
232	25	SVIMS/casual/04/2014/0200	IRS 24,500	Casuality	NC	Syringe Pump	Organge	Flow Prima	14026013-Z	Organge Medical	2Y	04-02-14	04-01-16	SVIMS	Working
233	26	SVIMS/casual/04/2	IRS 24,500	Casuality	NC	Syringe Pump	Organge	Flow Prima	14026014-	Organge	2Y	04-02-14	04-01-16	SVIMS	Working

		014/0201							Z	Medical					
234	27	SVIMS/casual/04/2014/0202	IRS 24,500	Casuality	NC	Syringe Pump	Organge	Flow Prima	14026015-Z	Organge Medical	2Y	04-02-14	04-01-16	SVIMS	Working
235	28	SVIMS/casual/04/2014/0203	IRS 24,500	Casuality	NC	Syringe Pump	Organge	Flow Prima	14026016-Z	Organge Medical	2Y	04-02-14	04-01-16	SVIMS	Working
236	29	SVIMS/casual/04/2014/0204	IRS 24,500	Casuality	NC	Syringe Pump	Organge	Flow Prima	14026017-Z	Organge Medical	2Y	04-02-14	04-01-16	SVIMS	Working
237	1	SVIMS/EmeMed/01/2016/0205	IRS 15,49,400	**Emergence Medicine**	NC	Ultra Sound Scanner	Esote	Mylab 40	40-13554	Esote India	3Y	15/01/2016	14/01/2019	SVIMS	Working
238	2	SVIMS/EmeMed/12/2016/0206	Rs 29,252.71	Emergence Medicine	NC	Syringe Pump	Plenum Tech Pvt Ltd	Zion +	1821	Plenum Tech	3Y	15/06/2016	14/06/2019	SVIMS	Not Working
239	3	SVIMS/EmeMed/12/2016/0207	Rs 29,252.71	Emergence Medicine	NC	Syringe Pump	Plenum Tech Pvt Ltd	Zion +	1788	Plenum Tech	3Y	15/06/2016	14/06/2019	SVIMS	Working
240	4	SVIMS/EmeMed/12/2016/0208	Rs 29,252.71	Emergence Medicine	NC	Syringe Pump	Plenum Tech Pvt Ltd	Zion +	1787	Plenum Tech	3Y	15/06/2016	14/06/2019	SVIMS	Working
241	5	SVIMS/EmeMed/12/2016/0209	Rs 29,252.71	Emergence Medicine	NC	Syringe Pump	Plenum Tech Pvt Ltd	Zion +	1841	Plenum Tech	3Y	15/06/2016	14/06/2019	SVIMS	Working
242	6	SVIMS/EmeMed/12/2016/0210	Rs 29,252.71	Emergence Medicine	NC	Syringe Pump	Plenum Tech Pvt Ltd	Zion +	1796	Plenum Tech	3Y	15/06/2016	14/06/2019	SVIMS	Working
243	7	SVIMS/EmeMed/12/2016/0211	Rs 29,252.71	Emergence Medicine	NC	Syringe Pump	Plenum Tech Pvt Ltd	Zion +	1789	Plenum Tech	3Y	15/06/2016	14/06/2019	SVIMS	Working
244	8	SVIMS/EmeMed/12/2016/0212	Rs 29,252.71	Emergence Medicine	NC	Syringe Pump	Plenum Tech Pvt Ltd	Zion +	1889	Plenum Tech	3Y	15/06/2016	14/06/2019	SVIMS	Working
245	9	SVIMS/EmeMed/12/2016/0213	Rs 29,252.71	Emergence Medicine	NC	Syringe Pump	Plenum Tech Pvt Ltd	Zion +	1811	Plenum Tech	3Y	15/06/2016	14/06/2019	SVIMS	Not Working
246	10	SVIMS/EmeMed/12/2016/0214	Rs 29,252.71	Emergence Medicine	NC	Syringe Pump	Plenum Tech Pvt Ltd	Zion +	1901	Plenum Tech	3Y	15/06/2016	14/06/2019	SVIMS	Not Working
247	11	SVIMS/EmeMed/12/2016/0215	Rs 29,252.71	Emergence Medicine	NC	Syringe Pump	Plenum Tech Pvt Ltd	Zion +	1824	Plenum Tech	3Y	15/06/2016	14/06/2019	SVIMS	Working
248	12	SVIMS/EmeMed/12/2016/0216	Rs 29,252.71	Emergence Medicine	NC	Syringe Pump	Plenum Tech Pvt Ltd	Zion +	1900	Plenum Tech	3Y	15/06/2016	14/06/2019	SVIMS	Working
249	13	SVIMS/EmeMed/12/2016/0217	Rs 29,252.71	Emergence Medicine	NC	Syringe Pump	Plenum Tech Pvt Ltd	Zion +	1818	Plenum Tech	3Y	15/06/2016	14/06/2019	SVIMS	Not Working
250	14	SVIMS/EmeMed/12/2016/0218	Rs 29,252.71	Emergence Medicine	NC	Syringe Pump	Plenum Tech Pvt Ltd	Zion +	1802	Plenum Tech	3Y	15/06/2016	14/06/2019	SVIMS	Not Working
251	15	SVIMS/EmeMed/12/2016/0219	Rs 29,252.71	Emergence Medicine	NC	Syringe Pump	Plenum Tech Pvt Ltd	Zion +	1803	Plenum Tech	3Y	15/06/2016	14/06/2019	SVIMS	Not Working
252	16	SVIMS/EmeMed/12/2016/0220	Rs 29,252.71	Emergence Medicine	NC	Syringe Pump	Plenum Tech Pvt Ltd	Zion +	1834	Plenum Tech	3Y	15/06/2016	14/06/2019	SVIMS	Not Working

253	17	SVIMS/EmeMed/07/2016/0221		Emergence Medicine	NC	Syringe Pump	L&T	SP102	609266	L&T	2Y	11-04-09	11-03-11	PMSSY-HLL	Working
254	18	SVIMS/EmeMed/02/2010/0222		Emergence Medicine	NC	Syringe Pump	Fresenius	Injectomat/Agilia	20497428	Medi	5Y	19/03/09	18/03/14	SVIMS	Working
255	19	SVIMS/EmeMed/02/2010/0223		Emergence Medicine	C	Defibrillator	Mindray	BeneHeart D3	EL-65027002	Green Apple	2Y	19/07/2016	18/07/2018	SVIMS	Working
256	20	SVIMS/EmeMed/02/2010/0224	IRS 4,04,683	Emergence Medicine	C	Multi Para Monitor	Mindray	Beneview T8	CF-9A104651	Instromedic	2y	02-04-10	02-03-12	SVIMS	Working
257	21	SVIMS/EmeMed/02/2010/0225	IRS 4,04,683	Emergence Medicine	C	Multi Para Monitor	Mindray	Beneview T8	CF-9A104652	Instromedic	2y	02-04-10	02-03-12	SVIMS	Working
258	22	SVIMS/EmeMed/09/2016/0226		Emergence Medicine	C	Multi Para Monitor	Bionet	BM 5	D8N 0300109	Vijetha	1Y	28/09/16	27/09/17	SVIMS	Working
259	23	SVIMS/EmeMed/09/2016/0227		Emergence Medicine	C	Multi Para Monitor	Bionet	BM 5	D8N 0300106	Vijetha	1Y	28/09/16	27/09/17	SVIMS	Not Working
260	24	SVIMS/EmeMed/09/2016/0228		Emergence Medicine	C	Multi Para Monitor	Bionet	BM 5	D8N 0300110	Vijetha	1Y	28/09/16	27/09/17	SVIMS	Working
261	25	SVIMS/EmeMed/09/2017/0229		Emergence Medicine	C	Multi Para Monitor	Bionet	BM 5	D8R 0300064	Jk Medical	1Y	09-06-17	09-05-18	SVIMS	Working
262	26	SVIMS/EmeMed/09/2017/0230		Emergence Medicine	C	Multi Para Monitor	Bionet	BM 5	D8R 0300066	Jk Medical	1Y	09-06-17	09-05-18	SVIMS	Working
263	27	SVIMS/EmeMed/09/2017/0231		Emergence Medicine	C	Multi Para Monitor	Bionet	BM 5	D8R 0300068	Jk Medical	1Y	09-06-17	09-05-18	SVIMS	Working
264	28	SVIMS/MedMed/02/2010/0232	IRS 4,04,683	Emergence Medicin Ex	C	Multi Para Monitor	Mindray	Beneview T8	CF-99103989	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
265	29	SVIMS/EmeMed/02/2010/0233	IRS 4,04,683	Emergence Medicine Ex	C	Multi Para Monitor	Mindray	Beneview T8	CF-99104010	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
266	30	SVIMS/EmeMed/02/2010/0234	IRS 4,04,683	Emergence Medicin Ex	C	Multi Para Monitor	Mindray	Beneview T8	CF-9A104663	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
267	31	SVIMS/EmeMed/02/2010/0235	IRS 4,04,683	Emergence Medicine Ex	C	Multi Para Monitor	Mindray	Beneview T8	CF-9A104638	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
268	32	SVIMS/EmeMed/02/2010/0236	IRS 4,04,683	Emergence Medicin Ex	C	Multi Para Monitor	Mindray	Beneview T8	CF-9A104648	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
269	33	SVIMS/EmeMedi/02/2010/0237	IRS 4,04,683	Emergence Medicine Ex	C	Multi Para Monitor	Mindray	Beneview T8	CF-9A104636	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
270	34	SVIMS/EmeMed/02/2010/0238	IRS 4,04,683	Emergence Medicin Ex	C	Multi Para Monitor	Mindray	Beneview T8	CF-9A104661	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
271	35	SVIMS/EmeMed/02/2010/0239	IRS 4,04,683	Emergence Medicine Ex	C	Multi Para Monitor	Mindray	Beneview T8	CF-9A104631	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
272	36	SVIMS/EmeMed/02/2010/0240	IRS 4,04,683	Emergence Medicin Ex	C	Multi Para Monitor	Mindray	Beneview T8	CF-9A104646	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
273	37	SVIMS/EmeMed/06/2018/1117	Irs 1,29,074/-	Emergence Medicin Ex	C	Multi Para Monitor	Mindray	UMEC 12	KQ-84011706	Green apple	5Y	06-07-18	06-06-23	SVIMS	Working
274	38	SVIMS/EmeMed/06/2018/1118	Irs 1,29,074/-	Emergence Medicin Ex	C	Multi Para Monitor	Mindray	UMEC 12	KQ-84011707	Green apple	5Y	06-07-18	06-06-23	SVIMS	Working

275	39	SVIMS/EmeMed/06/2018/1119	Irs 1,29,074/-	Emergence Medicin Ex	C	Multi Para Monitor	Mindray	UMEC 12	KQ-84011708	Green apple	5Y	06-07-18	06-06-23	SVIMS	Working
276	40	SVIMS/EmeMed/06/2018/1120	Irs 1,29,074/-	Emergence Medicin Ex	C	Multi Para Monitor	Mindray	UMEC 12	KQ-84011709	Green apple	5Y	06-07-18	06-06-23	SVIMS	Working
277	41	SVIMS/EmeMed/06/2018/1121	Irs 1,29,074/-	Emergence Medicin Ex	C	Multi Para Monitor	Mindray	UMEC 12	KQ-84011711	Green apple	5Y	06-07-18	06-06-23	SVIMS	Working
278	42	SVIMS/EmeMed/06/2018/1122	Irs 1,29,074/-	Emergence Medicin Ex	C	Multi Para Monitor	Mindray	UMEC 12	KQ-84011712	Green apple	5Y	06-07-18	06-06-23	SVIMS	Working
279	43	SVIMS/EmeMed/06/2018/1123	Irs 1,29,074/-	Emergence Medicin Ex	C	Multi Para Monitor	Mindray	UMEC 12	KQ-84011713	Green apple	5Y	06-07-18	06-06-23	SVIMS	Working
280	44	SVIMS/EmeMed/03/2018/1112		Emergence Medicin	NC	Flexi.Intubating Video Endo	Karl stroz			Medi Focus	5y	26.03.2018	25.03.2023	SVIMS	Working
281	45	SVIMS/EmeMed/03/2018/1104		Emergence Medicin Ex	c	Defibrillator	Mindray	BeneHeart D2	EI-82000342	Green Apple	5Y	30.03.2018	29.03.2023	SVIMS	Working
282	46	SVIMS/EmeMed/04/2019/1164		Emergence Medicin (New Ambulance)	c	Defibrillator	Mindray	Bene heart D2	EI-92003259	Green Apple	5Y	13.04.2019	12.04.2024	SVIMS	Working

283	47	SVIMS/EmeMed/11/2019/1275		Emergence Medicine		ECG Machine	Wipro GE	MAC 2000	SRR19040091 PA	Suntech Medical	1 y	27.11.2019	26.11.2019	SVIMS	Working
284	48	SVIMS/EmeMed/01/2020/1306		Emergence Medicine		Syringe Pump	Smiths Medical	Graseby C9	18320 2891	M M Medical	5 Y	06.01.2020	05.01.2025	SVIMS	Working
285	49	SVIMS/EmeMed/01/2020/1307		Emergence Medicine		Syringe Pump	Smiths Medical	Graseby C10	18320 2890	M M Medical	5 Y	06.01.2020	05.01.2025	SVIMS	Working
286	50	SVIMS/EmeMed/01/2020/1308		Emergence Medicine		Syringe Pump	Smiths Medical	Graseby C11	18320 2913	M M Medical	5 Y	06.01.2020	05.01.2025	SVIMS	Working
287	51	SVIMS/EmeMed/01/2020/1309		Emergence Medicine		Syringe Pump	Smiths Medical	Graseby C12	18320 2917	M M Medical	5 Y	06.01.2020	05.01.2025	SVIMS	Working
288	52	SVIMS/EmeMed/01/2020/1310		Emergence Medicine		Syringe Pump	Smiths Medical	Graseby C13	18320 2968	M M Medical	5 Y	06.01.2020	05.01.2025	SVIMS	Working
289	53	SVIMS/EmeMed/01/2020/1311		Emergence Medicine		Syringe Pump	Smiths Medical	Graseby C14	18320 2893	M M Medical	5 Y	06.01.2020	05.01.2025	SVIMS	Working
290	54	SVIMS/EmeMed/01/2020/1312		Emergence Medicine		Syringe Pump	Smiths Medical	Graseby C15	18320 2924	M M Medical	5 Y	06.01.2020	05.01.2025	SVIMS	Working
291	55	SVIMS/EmeMed/01/2020/1313		Emergence Medicine		Syringe Pump	Smiths Medical	Graseby C16	18320 2908	M M Medical	5 Y	06.01.2020	05.01.2025	SVIMS	Working
292	56	SVIMS/EmeMed/01/2020/1314		Emergence Medicine		Syringe Pump	Smiths Medical	Graseby C16	18320 2918		5 Y	06.01.2020	05.01.2025	SVIMS	Working
293	1	SVIMS/Medici/03/2009/0241		**Medicine/MICU**	NC	**Sleep Lab System**	Natus medical	Sleep Scan	APE 082383	Sleep Scan	2y	26/03/09	25/03/11	PMSSY-HLL	Working
294	2	SVIMS/Medici/08/2003/0242		Medicine/MICU	NC	**PFT System**	Morgan	Bench Mark	384	PK Morgon	3y	26/08/03	25/08/06	SVIMS	Working
295	3	SVIMS/MedIici/10/2016/0243		Medicine/MICU	NC	**PFT System**	NDD	Easyone Pro Lab	600446	Jk Med	5Y	10-01-16	31/09/2021	SVIMS	Working
296	4	SVIMS/MedICU/02/2010/0244	IRS 4,04,683	Medicine/MICU	C	Multi Para Monitor	Mindray	Beneview T8	CF-99103987	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
297	5	SVIMS/MedICU/02/2010/0245	IRS 4,04,683	Medicine/MICU	C	Multi Para Monitor	Mindray	Beneview T8	CF-99103976	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
298	6	SVIMS/MedICU/02/2010/0246	IRS 4,04,683	Medicine/MICU	C	Multi Para Monitor	Mindray	Beneview T8	CF-99104017	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
299	7	SVIMS/MedICU/02/2010/0247	IRS 4,04,683	Medicine/MICU	C	Multi Para Monitor	Mindray	Beneview T8	CF-9A104629	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
300	8	SVIMS/MedICU/02/2010/0248	IRS 4,04,683	Medicine/MICU	C	Multi Para Monitor	Mindray	Beneview T8	CF-9A104667	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
301	9	SVIMS/MedICU/02/2010/0249	IRS 4,04,683	Medicine/MICU	C	Multi Para Monitor	Mindray	Beneview T8	CF-9A104658	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Not Working
302	10	SVIMS/MEDICU/02/2010/0250	IRS 4,04,683	Medicine/ENDO Ward	C	Multi Para Monitor	Mindray	Beneview T8	CF-9A104666	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
303	11	SVIMS/MedICU/02/2010/0251	IRS 4,04,683	Medicine /ENDO Ward	C	Multi Para Monitor	Mindray	Beneview T8	CF-9A104633	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
304	12	SVIMS/MedICU/01/2010/0252		Medicine/MICU	NC	Spectro Photometer	Elico	BL-200		Sri Vijaya	3y	23/01/10	22/01/12	PMSSY-APHMHIDC	Working
305	13	SVIMS/MedICU/08/2014/0253		Medicine/MICU	NC	ECG Recorder	BioNet	Cardio 7	T7N1200015	Vijetha	1Y	27/08/2014	26/08/2015	SVIMS	Working
306	14	SVIMS/MedICU/10	IRS	Medicine/MIC	C	ICU Ventilator	Tecme	Grpahnet	9101 118	Meditronic	2y	10-01-11	31/09/2013	PMSS	Working

		/2011/0254/C	11,18,929	U					1080					Y-HLL	
307	15	SVIMS/MedICU/10/2011/0255/C	IRS 11,18,929	Medicine/MICU	C	ICU Ventilator	Tecme	Grpahnet	9101 121 1080	Meditronic	2y	10-01-11	31/09/2013	PMSSY-HLL	Working
308	16	SVIMS/MedICU/10/2011/0256/C	IRS 11,18,929	Medicine/MICU	C	ICU Ventilator	Tecme	Grpahnet	9101 110 1080	Meditronic	2y	10-01-11	31/09/2013	PMSSY-HLL	Working
309	17	SVIMS/MedICU/10/2011/0257/C	IRS 11,18,929	Medicine/MICU	C	ICU Ventilator	Tecme	Grpahnet	9101 129 1080	Meditronic	2y	10-01-11	31/09/2013	PMSSY-HLL	Working
310	18	SVIMS/Medici/02/2013/0258		Medicine/MICU	NC	Deep Freezer - 86	Forma	991	826493-1202	Vijaya	5y	02-04-13	02-03-18	SVIMS	Working
311	19	SVIMS/Medici/09/2013/0259		Medicine/MICU	NC	Deep Freezer - 40	Terumo penpol	Df 40U	1304309	Terumo	5Y	09-05-13	09-04-18	SVIMS	Working
312	20	SVIMS/Medici/09/2013/0260		Medicine/MICU	NC	Deep Freezer - 40	Terumo penpol	Df 40U	1304311	Terumo	5Y	09-05-13	09-04-18	SVIMS	Working
313	21	SVIMS/MedICU/00/0000/0261/C		Medicine/MICU	C	Defibrillator	BPL	DF 2509R	BYMD72986	Bharat Medi	1Y			SVIMS	Working
314	22	SVIMS/MedICU/11/2009/0262	IRS 24,181	Medicine/MICU	NC	Syringe Pump	L&T	SP102	609278	L&T	2Y	11-04-09	11-03-11	PMSSY-HLL	Working
315	23	SVIMS/MedICU/03/2009/0263		Medicine/MICU	NC	Syringe Pump	Fresenius	Injectomat/Agilia	20497447	Medi	5Y	19/03/09	18/03/14	SVIMS	Working
316	24	SVIMS/Medici/12/2016/0264		Medicine/MICU	NC	Syringe Pump	Plenum Tech Pvt Ltd	Zion +	1387	Plenum Tech	3Y	16/12/16	15/12/19	SVIMS	Working
317	25	SVIMS/Medici/12/2016/0265		Medicine/MICU	NC	Syringe Pump	Plenum Tech Pvt Ltd	Zion +	1389	Plenum Tech	3Y	16/12/16	15/12/19	SVIMS	Working
318	26	SVIMS/Medici/12/2016/0266		Medicine/MICU	NC	Syringe Pump	Plenum Tech Pvt Ltd	Zion +	2269	Plenum Tech	3Y	16/12/16	15/12/19	SVIMS	Working
319	27	SVIMS/Medici/12/2016/0267		Medicine/MICU	NC	Syringe Pump	Plenum Tech Pvt Ltd	Zion +	2270	Plenum Tech	3Y	16/12/16	15/12/19	SVIMS	Working
320	28	SVIMS/Medici/12/2016/0268		Medicine/MICU	NC	Syringe Pump	Plenum Tech Pvt Ltd	Zion +	2271	Plenum Tech	3Y	16/12/16	15/12/19	SVIMS	Working
321	29	SVIMS/Medici/12/2016/0269		Medicine/MICU	NC	Syringe Pump	Plenum Tech Pvt Ltd	Zion +	2274	Plenum Tech	3Y	16/12/16	15/12/19	SVIMS	Working
322	30	SVIMS/Medici/00/0000/1238		Medicine/MICU	NC	Syringe Pump	B Braun	Perfusor compact							
323	31	SVIMS/Medici/00/0000/1239		Medicine/MICU	NC	Syringe Pump	B Braun	Perfusor compact							
324	32	SVIMS/Medici/00/0000/1240		Medicine/MICU	NC	Syringe Pump	B Braun	Perfusor compact							
325	33	SVIMS/Medici/00/0000/1241		Medicine/MICU	NC	Syringe Pump	B Braun	Perfusor compact							
326	34	SVIMS/Medici/00/0000/1242		Medicine/MICU	NC	Pulse Oximeter	BCI	3180	AG06100015						
327	35	SVIMS/Medici/00/0000/1243		Medicine/MICU	NC	Pulse Oximeter	BCI	3180	AG06100052						
328	36	SVIMS/Medici/02/2020/1318		Medicine/MICU		Infusion Pump	Mindray	BenefusionVP1	SK-90605757	Green apple	5y	27.01.2020	26.01.2025		
329	37	SVIMS/Medici/02/2020/1319		Medicine/MICU		Infusion Pump	Mindray	BenefusionVP1	SK-90605761	Green apple	5y	27.01.2020	26.01.2025		

330	1	SVIMS/PraDha/02/ 2010/0270	IRS 4,04,683	**Pranadhana ward**	C	Multi Para Monitor	Mindray	Beneview T8	CF-9A104653	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
331	2	SVIMS/PraDha/02/ 2010/0271		Pranadhana ward	C	Multi Para Monitor	Mindray	PM-8000	AA-99121313	Instromedic	2y	02-07-10	02-06-12	PMSSY-HLL	Working
332	3	SVIMS/PraDha/11/ 2009/0272	IRS 24,181	Pranadhana ward	NC	Syringe Pump	Neuron BioMed	SP 102	609226	L & T	2Y	11-04-09	11-03-11	PMSSY-HLL	Working
333	4	SVIMS/PraDha/11/ 2009/0273	IRS 24,181	Pranadhana ward	NC	Syringe Pump	Neuron BioMed	SP 102	609244	L & T	2Y	11-04-09	11-03-11	PMSSY-HLL	Working
334	1	SVIMS/AshisW/11/ 2009/0274	IRS 24,181	**Ashis Ward**	NC	Syringe Pump	Neuron BioMed	SP 102	609228	L & T	2Y	11-04-09	11-03-11	PMSSY-HLL	Working
335	2	SVIMS/AshisW/11/ 2009/0275	IRS 24,181	Ashis Ward	NC	Syringe Pump	Neuron BioMed	SP 102	609243	L & T	2Y	11-04-09	11-03-11	PMSSY-HLL	Working
336	1	SVIMS/EndLab/01/ 1997/0276		**Endo crinology** -Lab	NC	Auto Beta Counter	Wallac	1409		Pharmacia	3Y	1997	2000	SVIMS	working
337	2	SVIMS/EndLab/01/ 1997/0277		Endo crinology -Lab	NC	Manual Gamma Counter	ECIL	W76415	076-415	ECIL	1Y	1997	1998	SVIMS	Working
338	3	SVIMS/EndLab/01/ 1997/0278		Endo crinology -Lab	NC	Centrifuge	Remi	R8C	JNLC-6837	Remi	1Y	1997	1998	SVIMS	Working
339	4	SVIMS/EndLab/01/ 1997/0279		Endo crinology -Lab	NC	Centrifuge	Remi	R8C	ILCO-2487	Remi	1Y	1997	1998	SVIMS	Working
340	5	SVIMS/EndLab/10/ 2000/0280		Endo crinology -Lab	NC	Cooling Centrifuge	Remi		HOCI-5821	Indian Scientific	1y	21/10/00	20/10/01	SVIMS	Working
341	6	SVIMS/EndoC/02/2 007/0281		Endo crinology -Lab	NC	Bone Densitometer	Hologic	Discovry-A	SQ9844	ADS Medical	3Y	02-02-07	02-01-10	SVIMS	Working
342	7	SVIMS/EndLab/12/ 2014/0282		Endo crinology -Lab	NC	PCR System	Eppendorf	MasterCycler Nexus	6333DQ10 8630	Eppendorf	5Y	23/12/20 14	22/12/2019	SVIMS	Working
343	8	SVIMS/EndLab/07/ 2009/0283		Endo crinology -Lab	NC	Deep Freezer - 40 Deg C	Terumo	DF40u	906108	Terumo	3Y	18/07/09	17/07/12	SVIMS	Working
344	9	SVIMS/EndLab/09/ 2016/0284		Endo crinology -Lab	NC	Deep Freezer - 40 Deg C	Terumo	DF40u	201608538	Terumo	3Y	30/09/16	29/09/19	SVIMS	Working
345	10	SVIMS/EndLab/09/ 2016/0285		Endo crinology -Lab	NC	Deep Freezer - 40 Deg C	Terumo	DF40u	201608541	Terumo	3Y	30/09/16	29/09/19	SVIMS	Working
346	11	SVIMS/EndLab/03/ 2013/0286		Endo crinology -Lab	NC	Chemi Illuminance syatem	Beckman	Acess-2	502630	Beckman India		03-05-13		Reagent Rental	Working
347	12	SVIMS/EndLab/10/ 2016/0287		Endo crinology -Lab	NC	Chemi Illuminance syatem	Beckman	Acess-2	511676	Beckman India		15/10/20 16		Reagent Rental	Working
348	13	SVIMS/EndLab/02/ 2012/0288		Endo crinology -Lab	NC	A1C Analyzer	BioRad	D-10	DC2G7323 16	Pooja Medical	5Y	23/2/12		Reagent Rental	Working
349	14	SVIMS/EndLab/02/ 2012/0289		Endo crinology -Lab	NC	A1C Analyzer	BioRad	D-10	DB7E1310 01	Pooja Medical	5Y	23/2/12		Reagent Rental	Working
350	15	SVIMS/EndLab/03/ 2010/0290		Endo crinology -Lab	NC	Elisa Reder	Bio Tek	Max 200	236604	MediSoec	5y	23/03/10	22/03/15	SVIMS	Working
351	16	SVIMS/EndLab/11// 2016/0291		Endo crinology -Lab	NC	Cooling Centrifuge	Remi	CPR-30 Plus	ZCU-26725	Medicoy	5Y	16/11/20 16	15/11/2021	SVIMS	Working
352	17	SVIMS/EndLab/04/ 2018/1101	2,44,720	Endo crinology -Lab	NC	Cardiac Autonomic Neuropathy System Analyser	Royal Medi System	CANS 504	C51803176	Royal Medi System	1 Y	05.04.20 18	04.04.2019	SVIMS	Working

353	18	SVIMS/EndoWa/02/2010/0292	IRS 4,04,683	ENDO Ward	C	Multi Para Monitor	Mindray	Beneview T8	CF-9A104660	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
354	19	SVIMS/EndoWa/02/2010/0293	IRS 4,04,683	ENDO Ward	NC	Multi Para Monitor	Mindray	Beneview T8	CF-9A104665	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
355	20	SVIMS/EndoWa/02/2010/0294	IRS 4,04,683	ENDO Ward	C	Multi Para Monitor	Mindray	Beneview T8	CF-9A104634	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
356	21	SVIMS/EndoWa/02/2010/0295	IRS 4,04,683	ENDO Ward	NC	Multi Para Monitor	Mindray	Beneview T8	CF-9A104649	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
357	22	SVIMS/EndoWa/02/2010/0296	IRS 4,04,683	ENDO Ward	C	Multi Para Monitor	Mindray	Beneview T8	CF-9A104664	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
358	23	SVIMS/EndoWa/03/2009/0297	Euro 585	ENDO Ward	NC	Syringe Pump	Fresenius	Injectomat/Agilia	20497418	Medi	5Y	19/03/09	18/03/14	SVIMS	Working
359	24	SVIMS/EndoWa/03//2009/0298	Euro 585	ENDO Ward	C	Syringe Pump	Fresenius	Injectomat/Agilia	20497354	Medi	5Y	19/03/09	18/03/14	SVIMS	Working
360	25	SVIMS/EndoWa/03//2009/0299	IRS 24,181	ENDO Ward	NC	Syringe Pump	Neuron BioMed	SP 102	609236	L & T	2Y	11-03-09	18/03/14	PMSSY-HLL	Working
361	26	SVIMS/EndoWa/03/2009/0300	IRS 24,181	ENDO Ward	C	Syringe Pump	Neuron BioMed	SP 102	609245	L & T	2Y	11-03-09	18/03/14	PMSSY-HLL	Working
362	27	SVIMS/EndoWa/01/2010/0301	IRS 37,146	ENDO Ward	NC	Pulse Oximeter	MediAid		EGO9G00194	Micronic	2Y	23/01/2010	22/01/2012	PMSSY-HLL	Working
363	28	SVIMS/EndoWa/08/2018/1133	1,36,800	ENDO Ward	NC	ECG Machine	Wipro GE	MAC 2000	SRR182770105PA	Wipro GE	1 Y	28.08.2018	27.08.2019	SVIMS	
364	29			ENDO Ward		Vascular Doppler	EMCO MEDITEC	D580							
365	1	SVIMS/Radiol/07/2013/0302		**Radiology**	NC	**CR System with Laser printer-Main Block**	Care stream	Classic	4000921	Care Stream	5Y	07-02-13	07-01-18	SVIMS	Working
366	2	SVIMS/Radiol/05/2013/0303		Radiology	NC	**CR System with Laser printer-opd**	Care stream	Classic	4000930	Care Stream	5Y	22/5/2013	21/5/2018	SVIMS	Working
367	3	SVIMS/Radiol/02/2010/0304/C		Radiology	C	**CT Scan - 128 slice with laser printer & Facuty Work Station**	Siemens	Definision As +	64522	Seimens india	5Y	02-10-10	02-09-15	PMSSY-HLL	**Working**
				3.1		**CT-128 Definition +**									
				3.2		**Facuty Work Station**									
				3.3		**0**									
				3.4		**Defibrillator**									
				3.5		**Fluro system**									
				3.6		**Laser Printer-Film**									
				3.7		**UPS**									
368	4	SVIMS/Radiol/01/2014/0305/C		Radiology	C	**MRI Scan 1.5 Tesla**	Siemens	Aera		Seimens	5Y	27/01/2014	26/01/2019	PMSSY-HLL	Working
				4.1		**MRI Scan-1.5Tesla**									
				4.2		**Facuty Work**									

						Station									
				4.3		**Laser Film printer**									
				4.4		**MRI Com Pulse Oximeter**									
				4.5		**Anaesthsia work station with Multi Monitor**									
				4.6		**Metal Detector-Stand type-2Nos**									
				4.7		**Metal Detector-Hand Held type-2Nos**									
				4.8		**Pressure Injector**									
				4.9		**UPS**									
				4.1		**Air Conditioning System**									
369	5	SVIMS/Radiol/03/2008/0306		Radiology	NC	**ultra Sound Scanner**	Siemens	Sonoline G40	303929	siemens	3Y	15/03/08	14/03/11	SVIMS	Working
370	6	SVIMS/Radiol/12/2009/0307		Radiology	C	**Ultra Sound Scanner**	Philips	IU22	03944NY	Philips India	2y	12-01-09	31/11/2011	PMSSY-HLL	Working
371	7	SVIMS/Radiol/03/2011/0308		Radiology	NC	**Ultra Sound Scanner**	G E	Voluson 730 Pro	A43830	GE	2y	24/03/2011	23/03/2013	PMSSY-HLL	Working
372	8	SVIMS/Radiol/01/2016/0309		Radiology	NC	**ultra Sound Scanner**	Esote	Mylab 40	40-13555	Esote India	3Y	15/01/2016	14/01/2019	SVIMS	Working
373	9	SVIMS/Radiol/01/2016/0310		Radiology	NC	**ultra Sound Scanner**	Esote	Mylab 40	40-13556	Esote India	3Y	15/01/2016	14/01/2019	SVIMS	Working
374	10	SVIMS/Radiol/01/2016/0311		Radiology	NC	**ultra Sound Scanner**	Esote	Mylab 40	40-13557	Esote India	3Y	15/01/2016	14/01/2019	SVIMS	Working
375	11	SVIMS/Radiol/07/2016/0312	RS 48, 00, 000/-	Radiology	NC	Ultra Sound Color Doppler	Esote	MYLAB TWICE	9995	Healthware	5y	20/07/2016	19/07/2021	SVIMS	Working
376	12	SVIMS/Radiol/10/2011/0313		Radiology	C	**X-Ray 1000ma OPD**	Listen Korea	1000mA	10-0246	Platinum	2Y	14/10/2011	13/10/2013	PMSSY-HLL	Working
377	13	SVIMS/Radiol/12/2013/0314		Radiology	NC	**Digital X-Ray**	Sedecal/Canon	Prorad 3N	12041072	Pronosysd	2Y	19/12/2013	18/12/2015	PMSSY-HLL	Working
378	14	SVIMS/Radiol/03/2013/0315		Radiology	NC	**X-Ray 500mA OPD**	Medtronics/ Philips	Dignox 4050	11A003	Philips India	2Y	15-03-13	14/03/2015	PMSSY-HLL	Working
379	15	SVIMS/Radiol/02/1992/0316		Radiology	C	**X-Ray 500mA**	Siemens	polyphos	EO 90566	Siemens	3Y	26/02/92	25/02/95	SVIMS	Working
380	16	SVIMS/Radiol/05/2000/0317		Radiology	NC	**X-Ray Mobile**	Siemens	Multi Mobile	3422	Siemens	1.5Y	25/05/00	24/11/01	SVIMS	Working
381	17	SVIMS/Radiol/10/2009/0318		Radiology	NC	**X-Ray Mobile**	Allenger	Opel 3.5/ SBM	2K90503075	Allenger	5Y	10-05-09	10-04-14	SVIMS	Working
382	18	SVIMS/Radiol/10/2009/0319		Radiology	NC	**X-Ray Mobile**	Allenger	Opel 3.5/ SBM	2K90503076	Allenger	5y	10-05-09	10-04-14	SVIMS	Working
383	19	SVIMS/Radiol/10/2009/0320		Radiology	NC	**X-Ray Mobile**	Allenger	Opel 3.5/ SBM	2K90503077	Allenger	5y	10-05-09	10-04-14	SVIMS	Working

384	20	SVIMS/Radiol/03/2016/0321		Radiology	NC	**X-Ray Mobile**	Adonis medica	AE 100 HF	151241	Adonis medica	5y	03-10-16	03-09-21	SVIMS	Working
385	21	SVIMS/Radiol/03/2016/0322		Radiology	NC	X-Ray Mobile	Adonis medica	AE 100 HF	151242	Adonis medica	5y	03-10-16	03-09-21	SVIMS	Working
386	22	SVIMS/Radiol/03/2016/0323		Radiology	NC	X-Ray Mobile	Adonis medica	AE 100 HF	160132	Adonis medica	5y	03-10-16	03-09-21	SVIMS	Working
387	23	SVIMS/Radiol/03/2016/0324		Radiology	NC	X-Ray Mobile	Adonis medica	AE 100 HF	160133	Adonis medica	5y	03-10-16	03-09-21	SVIMS	Working
388	24	SVIMS/Radiol/04/2016/0325	Rs42, 77, 263	Radiology	C	Mamography	Metaltronica	Lylium BYM	0639/CB2	Bet Medical	5Y	29/04/2016	28/04/2021	SVIMS	Working
389	25	SVIMS/Radiol/05/2018/1110	1,30,00,000	Radiology	C	800mA x-ray Machine with Fluoroscopy & Image Intensifier	IRIS Healthcare	Luminous Select	20053	Siemens	5 Y	04-05-18	03-05-23	SVIMS	Working
390	26	SVIMS/Radiol/01/2019/1138		Radiology	NC	Mamography-PINK BUS	Metaltronica	Lylium BYM	LLILHF107251CBZ	Bet Medical	5Y	02.01.2019	01-01-24	SVIMS	Working
391	27	SVIMS/Radiol/01/2019/1139		Radiology	NC	**CR System - Pink Bus**	Care stream	Classic	4004102	Care Stream	5Y	02.01.2019	01-01-24	SVIMS	Working
392	28	SVIMS/Radiol/01/2019/1140		Radiology	NC	Ultra Sound scanner	Mindray	DC 60	8C-89002255	Green apple	5Y	00/01/2019	00/01/2024	SVIMS	Working
393	29	SVIMS/Radiol/02/2019/1147		Radiology	NC	Mamography-Digital	Siemenms	Mamomat Fusion		Rotory Club	1Y	03-04-19	03-03-20	Rotory Club	Working
394	30	SVIMS/Radiol/00/0000/1165		Radiology	NC	Ultrasound System	Philips	HD3-EXP-V225	B07202300006847						
395	1	SVIMS/NuMedi/11/2009/0326		**NUCLEAR MEDICINE**	NC	Gamma Camera with Work station, UPS, laser printer, Schiller make TMT	Siemens	Symbia	1102	Siemens India	5Y	17/11/2009	16/11/2014	SVIMS	Working
396	2	SVIMS/NuMedi/08/1994/0327		NUCLEAR MEDICINE	NC	Dose Calibrator	Capintec	CRC7	71672	Wipro GE	3Y	08-10-94	08-09-97	SVIMS	Working
397	3	SVIMS/NuMedi/08/1994/0328		NUCLEAR MEDICINE	NC	Radiation Monitor	ECIL	RM4564	146	Wipro GE	3Y	08-10-94	08-09-97	SVIMS	Working
398	4	SVIMS/NuMedi/08/1994/0329		NUCLEAR MEDICINE	NC	Radiation Survey meter	ECIL	MR450A	499	Wipro GE	3Y	08-10-94	08-09-97	SVIMS	Working
399	5	SVIMS/NuMedi/10/2010/0330		NUCLEAR MEDICINE	NC	Pet CT - with Laser paper printer, Laser Film printer, Work station, UPS,Contamination monitor extra	Siemens	Biograph	91087	Siemens India	5Y	26/10/2010	25/10/2015	SVIMS	Working
400	6	SVIMS/NuMedi/12/2008/0331		NUCLEAR MEDICINE	C	Defibrillator	BPL	DF-2509	BYMD8C3233	BPL	3Y	12-12-08	12-11-11	SVIMS	Working
401	7	SVIMS/NuMedi/00/2014/0332		NUCLEAR MEDICINE	Nc	Syringe Pump	Plenum Tech Pvt Ltd	Zion +	1382	Plenum Tech	3Y	2014	2017	SVIMS	Working
402	1	SVIMS/Anaest/11/2009/0333/C	IRS 11,18,928	**Anaesthesiology**	**C**	ICU Ventilator	GE Datex Ohmeda	Engstrom	CBCN-01003	GE Datex Ohmeda	2Y	30/11/2009	29/11/2011	PMSSY-HLL	Working
403	2	SVIMS/Anaest/11/2	IRS	Anaesthesiolog	**C**	ICU Ventilator	GE Datex	Engstrom	CBCN-	GE Datex	2Y	30/11/20	29/11/2011	PMSS	Working

		009/0334/C	11,18,929	y			Ohmeda		01013	Ohmeda		09		Y-HLL	
404	3	SVIMS/Anaest/11/2009/0335/C	IRS 11,18,930	Anaesthesiology	**C**	ICU Ventilator	GE Datex Ohmeda	Engstrom	CBCN-01011	GE Datex Ohmeda	2Y	30/11/2009	29/11/2011	PMSS Y-HLL	Working
405	4	SVIMS/Anaest/11/2009/0336/C	IRS 11,18,931	Anaesthesiology	**C**	ICU Ventilator	GE Datex Ohmeda	Engstrom	CBCN-00996	GE Datex Ohmeda	2Y	30/11/2009	29/11/2011	PMSS Y-HLL	Working
406	5	SVIMS/Anaest/11/2009/0337/C	IRS 11,18,932	Anaesthesiology	**C**	ICU Ventilator	GE Datex Ohmeda	Engstrom	CBCN-01010	GE Datex Ohmeda	2Y	30/11/2009	29/11/2011	PMSS Y-HLL	Working
407	6	SVIMS/Anaest/05/2009/0338/C	IRS 11,98,864	Anaesthesiology	**C**	ICU Ventilator	Marquet	Servo-I	41979	Maquet India	5Y	27/05/09	26/05/14	SVIMS	Working
408	7	SVIMS/Anaest/05/2009/0339/C	IRS 11,98,864	Anaesthesiology	**C**	ICU Ventilator	Marquet	Servo-I	41980	Maquet India	5Y	27/05/09	26/05/14	SVIMS	Working
409	8	SVIMS/Anaest/05/2009/0340/C	IRS 11,98,864	Anaesthesiology	**C**	ICU Ventilator	Marquet	Servo-I	41981	Maquet India	5Y	27/05/09	26/05/14	SVIMS	Working
410	9	SVIMS/Anaest/05/2009/0341/C	IRS 11,98,864	Anaesthesiology	**C**	ICU Ventilator	Marquet	Servo-I	41982	Maquet India	5Y	27/05/09	26/05/14	SVIMS	Working
411	10	SVIMS/Anaest/05/2009/0342/C	IRS 11,98,864	Anaesthesiology	**C**	ICU Ventilator	Marquet	Servo-I	41983	Maquet India	5Y	27/05/09	26/05/14	SVIMS	Working
412	11	SVIMS/Anaest/05/2009/0343/C	IRS 11,98,864	Anaesthesiology	**C**	ICU Ventilator	Marquet	Servo-I	41984	Maquet India	5Y	27/05/09	26/05/14	SVIMS	Working
413	12	SVIMS/Anaest/05/2009/0344/C	IRS 11,98,864	Anaesthesiology	**C**	ICU Ventilator	Marquet	Servo-I	41985	Maquet India	5Y	27/05/09	26/05/14	SVIMS	Working
414	13	SVIMS/Anaest/05/2009/0345/C	IRS 11,98,864	Anaesthesiology	**C**	ICU Ventilator	Marquet	Servo-I	41986	Maquet India	5Y	27/05/09	26/05/14	SVIMS	Working
415	14	SVIMS/Anaest/05/2009/0346/C	IRS 11,98,864	Anaesthesiology	**C**	ICU Ventilator	Marquet	Servo-I	41987	Maquet India	5Y	27/05/09	26/05/14	SVIMS	Working
416	15	SVIMS/Anaest/05/2009/0347/C	IRS 11,98,864	Anaesthesiology	**C**	ICU Ventilator	Marquet	Servo-I	41988	Maquet India	5Y	27/05/09	26/05/14	SVIMS	Working
417	16	SVIMS/Anaest/05/2009/0348/C	IRS 11,98,864	Anaesthesiology	**C**	ICU Ventilator	Marquet	Servo-I	41989	Maquet India	5Y	27/05/09	26/05/14	SVIMS	Working
418	17	SVIMS/Anaest/05/2009/0349/C	IRS 11,98,864	Anaesthesiology	**C**	ICU Ventilator	Marquet	Servo-I	41990	Maquet India	5Y	27/05/09	26/05/14	SVIMS	Working
419	18	SVIMS/Anaest/05/2009/0350/C	IRS 11,98,864	Anaesthesiology	**C**	ICU Ventilator	Marquet	Servo-I	41991	Maquet India	5Y	27/05/09	26/05/14	SVIMS	Working
420	19	SVIMS/Anaest/05/2009/0351/C	IRS 11,98,864	Anaesthesiology	**C**	ICU Ventilator	Marquet	Servo-I	41992	Maquet India	5Y	27/05/09	26/05/14	SVIMS	Working
421	20	SVIMS/Anaest/05/2009/0352/C	IRS 11,98,864	Anaesthesiology	**C**	ICU Ventilator	Marquet	Servo-I	41993	Maquet India	5Y	27/05/09	26/05/14	SVIMS	Working
422	21	SVIMS/Anaest/05/2009/0353/C	IRS 11,98,864	Anaesthesiology	**C**	ICU Ventilator	Marquet	Servo-I	41994	Maquet India	5Y	27/05/09	26/05/14	SVIMS	Working
423	22	SVIMS/Anaest/05/2009/0354/C	IRS 11,98,864	Anaesthesiology	**C**	ICU Ventilator	Marquet	Servo-I	41995	Maquet India	5Y	27/05/09	26/05/14	SVIMS	Working
424	23	SVIMS/Anaest/05/2009/0355/C	IRS 11,98,864	Anaesthesiology	**C**	ICU Ventilator	Marquet	Servo-I	41996	Maquet India	5Y	27/05/09	26/05/14	SVIMS	Working
425	24	SVIMS/M/Anae/05/2009/0356/C	IRS 11,98,864	Anaesthesiology	**C**	ICU Ventilator	Marquet	Servo-I	41997	Maquet India	5Y	27/05/09	26/05/14	SVIMS	Working
426	25	SVIMS/Anaest/05/2009/0357/C	IRS 11,98,864	Anaesthesiology	**C**	ICU Ventilator	Marquet	Servo-I	41998	Maquet India	5Y	27/05/09	26/05/14	SVIMS	Working
427	26	SVIMS/Anaest/05/2009/0358/C	IRS 11,98,864	Anaesthesiology	**C**	ICU Ventilator	Marquet	Servo-I	41999	Maquet India	5Y	27/05/09	26/05/14	SVIMS	Working
428	27	SVIMS/Anaest/05/2009/0359/C	IRS 11,98,864	Anaesthesiology	**C**	ICU Ventilator	Marquet	Servo-I	42000	Maquet India	5Y	27/05/09	26/05/14	SVIMS	Working
429	28	SVIMS/Anaest/07/2010/0360	IRS 14,91,674	Anaesthesiology	**C**	Ana Work Station	GE Datex Ohmeda	Aestiva 7900	AMRN01176	GE Datex India	2Y	07-12-10	07-11-12	PMSS Y-HLL	Working

430	29	SVIMS/Anaest/07/2010/0361/C	IRS 14,91,674	Anaesthesiology	**C**	Ana Work Station	GE Datex Ohmeda	Aestiva 7900	AMRN01177	GE Datex India	2Y	07-12-10	07-11-12	PMSSY-HLL	Working
431	30	SVIMS/Anaest/07/2010/0362/C	IRS 14,91,674	Anaesthesiology	**C**	Ana Work Station	GE Datex Ohmeda	Aestiva 7900	AMRN01178	GE Datex India	2Y	07-12-10	07-11-12	PMSSY-HLL	**Working**
432	31	SVIMS/Anaest/08/2010/0363/C	IRS 14,91,674	Anaesthesiology	**C**	Ana Work Station	Drager	Fabius plus	ASAM0033	Drager india	2Y	08-08-10	08-07-12	PMSSY-HLL	Working
433	32	SVIMS/Anaest/08/2010/0364/C	IRS 14,91,674	Anaesthesiology	**C**	Ana Work Station	Drager	Fabius plus	ASAM0036	Drager india	2Y	08-08-10	08-07-12	PMSSY-HLL	Working
434	33	SVIMS/Anaest/08/2010/0365/C	IRS 14,91,674	Anaesthesiology	**C**	Ana Work Station	Drager	Fabius plus	ASAM0037	Drager india	2Y	08-08-10	08-07-12	PMSSY-HLL	Working
435	34	SVIMS/Anaest/08/2010/0366/C	IRS 14,91,674	Anaesthesiology	**C**	Ana Work Station	Drager	Fabius plus	ASAM0038	Drager india	2Y	08-08-10	08-07-12	PMSSY-HLL	Working
436	35	SVIMS/Anaest/08/2010/0367/C	IRS 14,91,674	Anaesthesiology	**C**	Ana Work Station	Drager	Fabius plus	ASAM0040	Drager india	2Y	08-08-10	08-07-12	PMSSY-HLL	Working
437	36	SVIMS/Anaest/01/2012/0368/C	IRS 14,91,674	Anaesthesiology	**C**	Ana Work Station	Drager	Fabius plus	ASAM0032	Drager india	2Y	01-01-12	31/12/2014	PMSSY-HLL	Working
438	37	SVIMS/Anaest/01/2012/0369/C	IRS 14,91,674	Anaesthesiology	**C**	Ana Work Station	Drager	Fabius plus	ASAM0034	Drager india	2Y	01-01-12	31/12/2014	PMSSY-HLL	Working
439	38	SVIMS/Anaest/01/2012/0370/C	IRS 14,91,674	Anaesthesiology	**C**	Ana Work Station	Drager	Fabius plus	ASAM0035	Drager india	2Y	01-01-12	31/12/2014	PMSSY-HLL	Working
440	39	SVIMS/Anaest/01/2012/0371/C	IRS 14,91,674	Anaesthesiology	C	Ana Work Station	Drager	Fabius plus	ASAM0039	Drager india	2Y	01-01-12	31/12/2014	PMSSY-HLL	Working
441	40	SVIMS/Anaest/01/2010/0372	IRS 24,181	Anaesthesiology-RICU	NC	Syringe Pump	Neuron BioMed	SP 102	0609-235	L & T	2Y	23/01/2010	22/01/2012	PMSSY-HLL	Working
442	41	SVIMS/Anaest/01/2010/0373	IRS 24,181	Anaesthesiology-RICu	NC	Syringe Pump	Neuron BioMed	SP 102	0609-240	L & T	2Y	23/01/2010	22/01/2012	PMSSY-HLL	Working
443	42	SVIMS/Anaest/01/2010/0374	IRS 24,181	Anaesthesiology-RICU	NC	Syringe Pump	Neuron BioMed	SP 102	0609-268	L & T	2Y	23/01/2010	22/01/2012	PMSSY-HLL	Working
444	43	SVIMS/Anaest/01/2010/0375	IRS 24,181	Anaesthesiology-RICu	NC	Syringe Pump	Neuron BioMed	SP 102	0609-224	L & T	2Y	23/01/2010	22/01/2012	PMSSY-HLL	Working
445	44	SVIMS/Anaest/01/2010/0376	IRS 24,181	Anaesthesiology-RICU	NC	Syringe Pump	Neuron BioMed	SP 102	0609-239	L & T	2Y	23/01/2010	22/01/2012	PMSSY-HLL	Working
446	45	SVIMS/Anaest/01/2010/0377	IRS 24,181	Anaesthesiology-RICu	NC	Syringe Pump	Neuron BioMed	SP 102	0609-285	L & T	2Y	23/01/2010	22/01/2012	PMSSY-HLL	Working
447	46	SVIMS/Anaest/01/2010/0378	IRS 24,181	Anaesthesiology-RICU	NC	Syringe Pump	Neuron BioMed	SP 102	0609-246	L & T	2Y	23/01/2010	22/01/2012	PMSSY-HLL	Working
448	47	SVIMS/Anaest/01/2010/0379	IRS 24,181	Anaesthesiology-RICu	NC	Syringe Pump	Neuron BioMed	SP 102	0609-274	L & T	2Y	23/01/2010	22/01/2012	PMSSY-HLL	Working
449	48	SVIMS/Anaest/01/2010/0380	IRS 24,181	Anaesthesiology-RICU	NC	Syringe Pump	Neuron BioMed	SP 102	0609-271	L & T	2Y	23/01/2010	22/01/2012	PMSSY-HLL	Working
450	49	SVIMS/Anaest/01/2010/0381	IRS 24,181	Anaesthesiology-RICu	NC	Syringe Pump	Neuron BioMed	SP 102	0609-233	L & T	2Y	23/01/2010	22/01/2012	PMSSY-HLL	Working
451	50	SVIMS/Anaest/06/2013/0382	Rs6,48,375	Anaesthesiology	NC	Vigileo monitor	Edwards life sciences	vigileo		Medical bionic	5Y	06-06-13	06-05-18	SVIMS	Working
452	51	SVIMS/Anaest/03/2009/0383	Euro 585	Anaesthesiology	NC	Syringe Pump	Fresenius	Injectomat/Agilia	20497449	Medi	5Y	19/03/09	18/03/14	SVIMS	Working
453	52	SVIMS/Anaest/03/2009/0384	Euro 585	Anaesthesiology	NC	Syringe Pump	Fresenius	Injectomat/Agilia	20497464	Medi	5Y	19/03/09	18/03/14	SVIMS	Working
454	53	SVIMS/Anaest/03/2009/0385	Euro 585	Anaesthesiology	NC	Syringe Pump	Fresenius	Injectomat/Agilia	20497357	Medi	5Y	19/03/09	18/03/14	SVIMS	Working
455	54	SVIMS/Anaest/03/2009/0386	Euro 585	Anaesthesiology	NC	Syringe Pump	Fresenius	Injectomat/Agilia	20497422	Medi	5Y	19/03/09	18/03/14	SVIMS	Working

456	55	SVIMS/Anaest/03/2009/0387	Euro 585	Anaesthesiology	NC	Syringe Pump	Fresenius	Injectomat/Agilia	20497441	Medi	5Y	19/03/09	18/03/14	SVIMS	Working
457	56	SVIMS/Anaest/03/2009/0388	Euro 585	Anaesthesiology	NC	Syringe Pump	Fresenius	Injectomat/Agilia	20497463	Medi	5Y	19/03/09	18/03/14	SVIMS	Working
458	57	SVIMS/Anaest/03/2009/0389	Euro 585	Anaesthesiology	NC	Syringe Pump	Fresenius	Injectomat/Agilia	20497461	Medi	5Y	19/03/09	18/03/14	SVIMS	Working
459	58	SVIMS/Anaest/03/2009/0390	Euro 585	Anaesthesiology	NC	Syringe Pump	Fresenius	Injectomat/Agilia	20497452	Medi	5Y	19/03/09	18/03/14	SVIMS	Working
460	59	SVIMS/Anaest/03/2009/0391	Euro 585	Anaesthesiology	NC	Syringe Pump	Fresenius	Injectomat/Agilia	20497445	Medi	5Y	19/03/09	18/03/14	SVIMS	Working
461	60	SVIMS/Anaest/03/2009/0392	Euro 585	Anaesthesiology	NC	Syringe Pump	Fresenius	Injectomat/Agilia	20497430	Medi	5Y	19/03/09	18/03/14	SVIMS	Working
462	61	SVIMS/Anaest/10/2008/0393	US$19,283	Anaesthesiology	C	Multi Para Monitor	Philips	MP 60	DE73113034	Philips	3Y	29/10/08	28/10/11	SVIMS	**Working**
463	62	SVIMS/Anaest/10/2008/0394	US$19,283	Anaesthesiology	C	Multi Para Monitor	Philips	MP60	DE73113004	Philips	3Y	29/10/08	28/10/11	SVIMS	Working
464	63	SVIMS/Anaest/10/2008/0395	US$19,283	Anaesthesiology	C	Multi Para Monitor	Philips	MP 60	DE73113000	Philips	3Y	29/10/08	28/10/11	SVIMS	Working
465	64	SVIMS/Anaest/10/2008/0396	US$19,283	Anaesthesiology	C	Multi Para Monitor	Philips	MP 60	DE73113015	Philips	3Y	29/10/08	28/10/11	SVIMS	Working
466	65	SVIMS/Anaest/10/2008/0397	US$19,283	Anaesthesiology	C	Multi Para Monitor	Philips	MP 60	DE73113040	Philips	3Y	29/10/08	28/10/11	SVIMS	Working
467	66	SVIMS/Anaest/10/2008/0398	US$19,283	Anaesthesiology	C	Multi Para Monitor	Philips	MP 60	DE73113030	Philips	3Y	29/10/08	28/10/11	SVIMS	Working
468	67	SVIMS/Anaest/10/2008/0399	US$19,283	Anaesthesiology	C	Multi Para Monitor	Philips	MP60	DE73112985	Philips	3Y	29/10/08	28/10/11	SVIMS	**Working**
469	68	SVIMS/Anaest/10/2008/0400	US$19,283	Anaesthesiology	C	Multi Para Monitor	Philips	MP 60	DE73113022	Philips	3Y	29/10/08	28/10/11	SVIMS	Working
470	69	SVIMS/Anaest/10/2008/0401	US$19,283	Anaesthesiology	C	Multi Para Monitor	Philips	MP 60	DE73113043	Philips	3Y	29/10/08	28/10/11	SVIMS	Working
471	70	SVIMS/Anaest/10/2008/0402	US$19,283	Anaesthesiology	C	Multi Para Monitor	Philips	MP 60	DE73113041	Philips	3Y	29/10/08	28/10/11	SVIMS	Working
472	71	SVIMS/Anaest/10/2008/0403	US$19,283	Anaesthesiology	C	Multi Para Monitor	Philips	X2 MMS	DE73611090	Philips	3Y	29/10/08	28/10/11	SVIMS	Working
473	72	SVIMS/Anaest/10/2008/0404	US$19,283	Anaesthesiology	C	Multi Para Monitor	Philips	X2 MMS	DE73611092	Philips	3Y	29/10/08	28/10/11	SVIMS	Working
474	73	SVIMS/Anaest/10/2008/0405	US$19,283	Anaesthesiology	C	Multi Para Monitor	Philips	X2 MMS	DE73611096	Philips	3Y	29/10/08	28/10/11	SVIMS	Working
475	74	SVIMS/Anaest/10/2008/0406	US$19,283	Anaesthesiology	C	Multi Para Monitor	Philips	X2 MMS	DE73611103	Philips	3Y	29/10/08	28/10/11	SVIMS	Working
476	75	SVIMS/Anaest/10/2008/0407	US$19,283	Anaesthesiology	C	Multi Para Monitor	Philips	X2 MMS	DE73611117	Philips	3Y	29/10/08	28/10/11	SVIMS	Working
477	76	SVIMS/Anaest/02/2010/0408	IRS 4,04,683	Anaesthesiology-RICU	C	Multi Para Monitor	Mindray	Beneview T8	CF-99103967	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
478	77	SVIMS/Anaest/02/2010/0409	IRS 4,04,683	Anaesthesiology-RICU	C	Multi Para Monitor	Mindray	Beneview T8	CF-99103970	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
479	78	SVIMS/Anaest/02/2010/0410	IRS 4,04,683	Anaesthesiology-RICU	C	Multi Para Monitor	Mindray	Beneview T8	CF-99103991	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
480	79	SVIMS/Anaest/02/2010/0411	IRS 4,04,683	Anaesthesiology-RICU	C	Multi Para Monitor	Mindray	Beneview T8	CF-99103997	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
481	80	SVIMS/Anaesti/02/2010/0412	IRS 4,04,683	Anaesthesiology-RICU	C	Multi Para Monitor	Mindray	Beneview T8	CF-99103999	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working

482	81	SVIMS/Anaest/02/2010/0413	IRS 4,04,683	Anaesthesiology-RICU	C	Multi Para Monitor	Mindray	Beneview T8	CF-99104012	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
483	82	SVIMS/Anaest/02/2010/0414	IRS 4,04,683	Anaesthesiology-RICU	C	Multi Para Monitor	Mindray	Beneview T8	CF-99104273	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
484	83	SVIMS/Anaest/02/2010/0415	IRS 4,04,683	Anaesthesiology-RICU	C	Multi Para Monitor	Mindray	Beneview T8	CF-99104274	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
485	84	SVIMS/Anaest/02/2010/0416	IRS 4,04,683	Anaesthesiology-RICU	C	Multi Para Monitor	Mindray	Beneview T8	CF-99104275	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
486	85	SVIMS/Anaest/02/2010/0417	IRS 4,04,683	Anaesthesiology-RICU	C	Multi Para Monitor	Mindray	Beneview T8	CF-99104276	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
487	86	SVIMS/Anaest/02/2010/0418	IRS 4,04,683	Anaesthesiology-RICU	C	Multi Para Monitor	Mindray	Beneview T8	CF-99104277	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
488	87	SVIMS/Anaest/02/2010/0419	IRS 4,04,683	Anaesthesiology-RICU	C	Multi Para Monitor	Mindray	Beneview T8	CF-99104278	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
489	88	SVIMS/Anaest/02/2010/0420	IRS 4,04,683	Anaesthesiology-RICU	C	Multi Para Monitor	Mindray	Beneview T8	CF-99104279	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
490	89	SVIMS/Anaest/02/2010/0421	IRS 4,04,683	Anaesthesiology-RICU	C	Multi Para Monitor	Mindray	Beneview T8	CF-99104280	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
491	90	SVIMS/Anaest/02/2010/0422	IRS 4,04,683	Anaesthesiology-RICU	C	Multi Para Monitor	Mindray	Beneview T8	CF-99104281	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
492	91	SVIMS/Anaest/02/2010/0423	IRS 4,04,683	Anaesthesiology-RICU	C	Multi Para Monitor	Mindray	Beneview T8	CF-99104282	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
493	92	SVIMS/Anaest/06/2016/0424	Reagent Rental	Anaesthesiology-RICU	C	Blood Gas Analyzer	RadioMeter	ABL 800	754R2258N007	JK Medical		28/06/2016		Reagent Rental	Working
494	93	SVIMS/Anaest/00/0000/0425		Anaesthesiology-RICU	C	Defibrillator	Philips	Heartstart XL	US00465720	Philips					Working
495	94	SVIMS/Anaest/12/2017/1100		Anaesthesiology	NC	Flexible Intubating Video Endoscope	Karl-Storz		XS13663/XS13496/41168/49733/53813	Medifocus (I)	5 Y	26-12-17	25-12-22	SVIMS	Working
496	95	SVIMS/Anaest/12/2017/1130		Anaesthesiology	C	Ana Work Station	Drager	Fabius C	ARXF0119	Drager india	3y				
497	96	SVIMS/Anaest/08/2020/1331		Anaesthesiology		High Frequency Nasal Cannual	Smith Medical	Inspire 02 FLO	2025041805	Vijetha	3y	28.08.2020	27.08.2023	SVIMS	Working
498	97	SVIMS/Anaest/08/2020/1332		Anaesthesiology		High Frequency Nasal Cannual	Smith Medical	Inspire 02 FLO	2025041465	Vijetha	3y	28.08.2020	27.08.2023	SVIMS	Working
499	98	SVIMS/Anaest/08/2020/1333		Anaesthesiology		High Frequency Nasal Cannual	Smith Medical	Inspire 02 FLO	2025040172	Vijetha	3y	28.08.2020	27.08.2023	SVIMS	Working
500	100	SVIMS/Anaest/08/2020/1334		Anaesthesiology		High Frequency Nasal Cannual	Smith Medical	Inspire 02 FLO	2025041754	Vijetha	3y	28.08.2020	27.08.2023	SVIMS	Working
501	101	SVIMS/Anaest/08/2020/1335		Anaesthesiology		High Frequency Nasal Cannual	Smith Medical	Inspire 02 FLO	2025041347	Vijetha	3y	28.08.2020	27.08.2023	SVIMS	Working
502	1	SVIMS/CT. OT /01/1993/0426/C		**CT SURGERY** OT	c	Heart Lung Machine	Sarns	System 8000 pumps	1106	J.Mitra	3Y	18/01/93	17/01/96	svims	Working
503	2	SVIMS/CT.OT /04/2007/0427/C		CT SURGERY OT	c	Heart Lung Machine	Maquet	HL 20	100243	Olympus	3y	18/04/2007	17/04/2010	svims	Working
					c	Heater Cooler Unit	Maquet	HUC 30	93101207	Olympus					Working
504	3	SVIMS/CT.OT /01/2016/0428/C		CT SURGERY OT	c	Heart Lung Machine	Maquet	HL 20	94002657	Maquet India	5y	20/01/2016	19/01/2021	svims	Working
					c	Heater Cooler Unit	Maquet	HCU 40	90440503						Working

505	4	SVIMS/CT.OT /01/2016/0429		CT SURGERY OT	c	Heater Cooler Unit	Sorin	HCU 3T	16S16514	ARCOM	5Y	01-08-16	01-07-21	svims	Working
506	5	SVIMS/CT.OT /01/2016/0430		CT SURGERY OT	c	Heater Cooler Unit	Sorin	HCU 3T	16S16515	ARCOM	5Y	01-08-16	01-07-21	svims	Working
507	6	SVIMS/CT.OT /06/2009/0431		CT SURGERY OT	NC	OT Light	Martin	V16 + V 10	1678, 1679	Vishal	3Y	26/06/09	25/06/11	PMSS Y-HLL	Working
508	7	SVIMS/CT.OT /06/2009/0432		CT SURGERY OT	NC	OT Light	Martin	V16 + V 10	1,66,61,667	Vishal	3Y	26/06/09	25/06/11	PMSS Y-HLL	Working
509	8	SVIMS/CT.OT /09/2012/0433		CT SURGERY OT	NC	OT Light	Martin	V16 + V 10	2088, 2089	Vishal	5Y	21/09/12	20/09/17	SVIMS	Working
510	9	SVIMS/CT.OT /10/2006/0434		CT SURGERY OT	NC	OT Table	Takeuchi	TS-103	TS-01068	Vishal	3Y	10-10-06	10-09-09	SVIMS	Working
511	10	SVIMS/CT.OT /10/2006/0435		CT SURGERY OT	NC	OT Table	Takeuchi	TS-103	TS-01067	Vishal	3Y	11-10-06	09-10-09	SVIMS	Working
512	11	SVIMS/CT.OT /11/2007/0437		CT SURGERY OT	NC	Surgical Diathermy	Valley Lab	Force RX	16998A	Asian	3Y	14/11/07	13/11/10	SVIMS	Working
513	12	SVIMS/CT.OT /04/2008/0438		CT SURGERY OT	NC	Surgical Diathermy	Valley Lab	Force RX	F54743A	Asian	3Y	04-10-08	04-09-11	SVIMS	Working
514	13	SVIMS/CT.OT /02/2005/0439		CT SURGERY OT	NC	Surgical Diathermy	Alsa	EXCEL 350 MCD	4974	Advanced Med	3Y	02-04-05	02-03-08	SVIMS	Working
515	14	SVIMS/CT.OT /05/2012/0440		CT SURGERY OT	NC	Electro Surgical Diathermy	Div Labs	Trinity-QRF	TY-011087	Div Labs	2Y	25/05/20 12	24/05/2014	Pmssy-HLL	Working
516	15	SVIMS/CT.OT /05/2012/0441		CT SURGERY OT	NC	Electro Surgical Diathermy	Div Labs	Trinity-QRF	TY-011088	Div Labs	2Y	25/05/20 12	24/05/2014	Pmssy-HLL	Working
517	16	SVIMS/CT.OT /12/2015/0442		CT SURGERY OT	NC	ACT Macine	Meditronics	ACT 200	ACT20052 76	medtronic india	1Y	15/12/20 15	14/12/2016	SVIMS	Working
518	17	SVIMS/CT.OT /07/20		CT SURGERY OT	NC	Brahco Scope	Pentex	EB-1975K	H120880		5 Y	25.04.20 18	24.05.2023	SVIMS	Working
519	18	SVIMS/CT.OT /06/2007/0444/C		CT SURGERY OT	C	IABP	Datacope	CS100	SA06576-D7	Advanced Micronic	3y	06-01-07	05-01-10	SVIMS	Working
520	19	SVIMS/CT.OT /06/2013/0445/C		CT SURGERY OT	C	IABP	Datacope	CS300	SI222047A 3	Advanced Micronic	5y	28/06/20 13	27/06/2018	SVIMS	Working
521	20	SVIMS/CT.OT /07/2005/0446		CT SURGERY OT	NC	Stenum Saw-Manman	Sisco			Sisco	1y	01-07-05	05-06-06	SVIMS	Working
522	21	SVIMS/CT.OT /12/2015/0447/C		CT SURGERY OT	C	Defibrillator	Mindray	BeneHeart D3	EL-5B023605	Green Apple	5Y	30/12/20 15	29/12/2020	SVIMS	Working
523	22	SVIMS/CT.OT /04/2019/0448/C		CT SURGERY OT	C	Defibrillator	Mindray	Bene heart D2	EI - 92003248	Green apple	5Y	16/04/20 19	15/04/2024	SVIMS	**Workin g**
524	23	SVIMS/CT.OT /02/2017/0449		CT SURGERY OT	NC	Stenum Saw-Manman	Sisco		B 770	Sisco	1y	14/02/17	13/02/18	SVIMS	Working
525	24	SVIMS/CT.OT /02/2017/0450		CT SURGERY OT	NC	Resternotomy-Redo-Saw	Sisco		A991	Sisco	1Y	14/02/17	13/02/18	SVIMS	Working
526	25	SVIMS/CT.OT /02/2017/0451		CT SURGERY OT	NC	Resternotomy-Redo-Saw	Sisco		B174	Sisco	1Y	14/02/17	13/02/18	SVIMS	Working
527	26	SVIMS/CT.OT /11/2017/0452		CT SURGERY OT	NC	Harmonic Scapel	J&J	Gen 11	111165127 3	J&J india	1Y	11-10-17	11-09-18	SVIMS	Working
528	27	SVIMS/CT.OT /07/2005/0453	US$6493	CT Surgery RR	C	Patient Monitor	Philips	MP 20	DE6222300 7	Philips	3Y	14/07/05	13/07/08	SVIMS	Working
529	28	SVIMS/CT.OT /07/2005/0454	US$6493	CT Surgery RR	C	Patient Monitor	Philips	MP20	DE5040506 0	Philips	3Y	14/07/05	13/07/08	SVIMS	Working
530	29	SVIMS/CT.OT /07/2005/0455	US$6493	CT Surgery RR	C	Patient Monitor	Philips	MP 20	DE6222298 9	Philips	3Y	14/07/05	13/07/08	SVIMS	Working

531	30	SVIMS/CT.OT /07/2005/0456	US$6493	CT Surgery RR	C	Patient Monitor	Philips	MP 20	DE6222308 4	Philips	3Y	14/07/05	13/07/08	SVIMS	Working
532	31	SVIMS/CT.OT /07/2005/0457	US$6493	CT Surgery RR	C	Patient Monitor	Philips	MP 20	DE5040506 6	Philips	3Y	14/07/05	13/07/08	SVIMS	Working
533	32	SVIMS/CT.OT /07/2005/0458	US$6493	CT Surgery RR	C	Patient Monitor	Philips	MP 20	DE6222305 3	Philips	3Y	14/07/05	13/07/08	SVIMS	Working
534	33	SVIMS/CT.OT /07/2005/0459	US$6493	CT Surgery RR	C	Patient Monitor	Philips	MP 20	DE6222298 2	Philips	3Y	14/07/05	13/07/08	SVIMS	Working
535	34	SVIMS/CT.RR /10/2008/0460	US$19,283	CT Surgery RR	C	Patient Monitor	Philips	MP 60	DE7311304 4	Philips	3Y	29/10/08	28/10/11	SVIMS	Working
536	35	SVIMS/CT.RR /10/2008/0461	US$19,283	CT Surgery RR	C	Patient Monitor	Philips	MP 60	DE7311303 5	Philips	3Y	29/10/08	28/10/11	SVIMS	Working
537	36	SVIMS/CT.RR /10/2008/0462	US$19,283	CT Surgery RR	C	Patient Monitor	Philips	MP 60	DE7311299 6	Philips	3Y	29/10/08	28/10/11	SVIMS	Working
538	37	SVIMS/CT.RR /10/2008/0463	US$19,283	CT Surgery RR	C	Patient Monitor	Philips	MP 60	DE7311304 7	Philips	3Y	29/10/08	28/10/11	SVIMS	Working
539	38	SVIMS/CT.RR /10/2008/0464	US$19,283	CT Surgery RR	C	Patient Monitor	Philips	MP 60	DE7311302 5	Philips	3Y	29/10/08	28/10/11	SVIMS	Working
540	39	SVIMS/CT.RR /10/2008/0465	US$19,283	CT Surgery RR	C	Patient Monitor	Philips	MP 60	DE7311304 2	Philips	3Y	29/10/08	28/10/11	SVIMS	Working
541	40	SVIMS/CT.RR /10/2008/0470	US$19,283	CT Surgery RR	C	Patient Monitor	Philips	MP60	DE7311303 1	Philips	3Y	29/10/08	28/10/11	SVIMS	Working
542	41	SVIMS/CT.RR /10/2008/0467	US$19,283	CT Surgery RR	C	Patient Monitor	Philips	MP 60	DE7311302 8	Philips	3Y	29/10/08	28/10/11	SVIMS	Working
543	42	SVIMS/CT.RR /10/2008/0468	US$19,283	CT Surgery RR	C	Patient Monitor	Philips	MP 60	DE7311303 9	Philips	3Y	29/10/08	28/10/11	SVIMS	Working
544	43	SVIMS/CT.RR /10/2008/0469	US$19,283	CT Surgery RR	C	Patient Monitor	Philips	MP 60	DE7311303 7	Philips	3Y	29/10/08	28/10/11	SVIMS	Working
545	44	SVIMS/CT.RR /10/2008/0470	US$19,283	CT Surgery RR	C	Patient Monitor	Philips	MP 60	DE7311302 6	Philips	3Y	29/10/08	28/10/11	SVIMS	Working
546	45	SVIMS/CT.RR /09/2014/0471	IRS 24,500	CT Surgery RR	NC	ECG Recorder	BioNet	Cardio 7	T7M11000 47	Vijetha	1Y	01-09-14	31/8/2015	SVIMS	Working
547	46	SVIMS/CT.RR /05/2013/0472	IRS 24,500	CT Surgery RR	NC	Syringe Pump	Organge	Flow Prima	13050541-Z	Organge Medical	2Y	23/05/13	22/05/15	SVIMS	Working
548	47	SVIMS/CT.RR /05/2013/0473	IRS 24,500	CT Surgery RR	NC	Syringe Pump	Organge	Flow Prima	13050542-Z	Organge Medical	2Y	23/05/13	22/05/15	SVIMS	Working
549	48	SVIMS/CT.RR /05/2013/0474	IRS 24,500	CT Surgery RR	NC	Syringe Pump	Organge	Flow Prima	13050543-Z	Organge Medical	2Y	23/05/13	22/05/15	SVIMS	Working
550	49	SVIMS/CT.RR /05/2013/0475	IRS 24,500	CT Surgery RR	NC	Syringe Pump	Organge	Flow Prima	13050544-Z	Organge Medical	2Y	23/05/13	22/05/15	SVIMS	Working
551	50	SVIMS/CT.RR /05/2013/0476	IRS 24,500	CT Surgery RR	NC	Syringe Pump	Organge	Flow Prima	13050545-Z	Organge Medical	2Y	23/05/13	22/05/15	SVIMS	Working
552	51	SVIMS/CT.RR /05/2013/0477	IRS 24,500	CT Surgery RR	NC	Syringe Pump	Organge	Flow Prima	13050546-Z	Organge Medical	2Y	23/05/13	22/05/15	SVIMS	Working
553	52	SVIMS/CT.RR /05/2013/0478	IRS 24,500	CT Surgery RR	NC	Syringe Pump	Organge	Flow Prima	13050547-Z	Organge Medical	2Y	23/05/13	22/05/15	SVIMS	Working
554	53	SVIMS/CT.RR /05/2013/0479	IRS 24,500	CT Surgery RR	NC	Syringe Pump	Organge	Flow Prima	13050548-Z	Organge Medical	2Y	23/05/13	22/05/15	SVIMS	Working
555	54	SVIMS/CT.RR /05/2013/0480	IRS 24,500	CT Surgery RR	NC	Syringe Pump	Organge	Flow Prima	13050549-Z	Organge Medical	2Y	23/05/13	22/05/15	SVIMS	Working
556	55	SVIMS/CT.RR /05/2013/0481	IRS 24,500	CT Surgery RR	NC	Syringe Pump	Organge	Flow Prima	13050550-Z	Organge Medical	2Y	23/05/13	22/05/15	SVIMS	Working
557	56	SVIMS/CT.RR	IRS 24,500	CT Surgery RR	NC	Syringe Pump	Organge	Flow Prima	13050577-	Organge	2Y	03-09-13	02-09-15	SVIMS	Working

		/09/2013/0482							Z	Medical					
558	57	SVIMS/CT.RR /09/2013/0483	IRS 24,500	CT Surgery RR	NC	Syringe Pump	Organge	Flow Prima	13050578-Z	Organge Medical	2Y	03-09-13	02-09-15	SVIMS	Working
559	58	SVIMS/CT.RR /09/2013/0484	IRS 24,500	CT Surgery RR	NC	Syringe Pump	Organge	Flow Prima	13050579-Z	Organge Medical	2Y	03-09-13	02-09-15	SVIMS	Working
560	59	SVIMS/CT.RR /09/2013/0485	IRS 24,500	CT Surgery RR	NC	Syringe Pump	Organge	Flow Prima	13050580-Z	Organge Medical	2Y	03-09-13	02-09-15	SVIMS	Working
561	60	SVIMS/CT.RR /09/2013/0486	IRS 24,500	CT Surgery RR	NC	Syringe Pump	Organge	Flow Prima	13051374-Z	Organge Medical	2Y	03-09-13	02-09-15	SVIMS	Working
562	61	SVIMS/CT.RR /09/2013/0487	IRS 24,500	CT Surgery RR	NC	Syringe Pump	Organge	Flow Prima	13051375-Z	Organge Medical	2Y	03-09-13	02-09-15	SVIMS	Working
563	62	SVIMS/CT.RR /09/2013/0488	IRS 24,500	CT Surgery RR	NC	Syringe Pump	Organge	Flow Prima	13051376-Z	Organge Medical	2Y	03-09-13	02-09-15	SVIMS	Working
564	63	SVIMS/CT.RR /09/2013/0489	IRS 24,500	CT Surgery RR	NC	Syringe Pump	Organge	Flow Prima	13051377-Z	Organge Medical	2Y	03-09-13	02-09-15	SVIMS	Working
565	64	SVIMS/CT.RR /09/2013/0490	IRS 24,500	CT Surgery RR	NC	Syringe Pump	Organge	Flow Prima	13051378-Z	Organge Medical	2Y	03-09-13	02-09-15	SVIMS	Working
566	65	SVIMS/CT.RR /09/2013/0491	IRS 24,500	CT Surgery RR	NC	Syringe Pump	Organge	Flow Prima	13051379-Z	Organge Medical	2Y	03-09-13	02-09-15	SVIMS	Working
567	66	SVIMS/CT.RR /10/2015/0492	Euro 585	CT Surgery RR	C	Defibrillator	Mindray	BeneHeart D3	EL-5B023604	Green Apple	5Y	30/12/2015	29/12/2020	SVIMS	Working
568	67	SVIMS/CT.RR /04/2009/0493	Euro 585	CT Surgery RR	NC	Syringe Pump	Fresenius	Injectomat	20497424	Mitie	5Y	04-07-09	04-06-14	SVIMS	Working
569	68	SVIMS/CT.RR /04/2009/0494	Euro 585	CT Surgery RR	NC	Syringe Pump	Fresenius	Injectomat	20497440	Mitie	5Y	04-07-09	04-06-14	SVIMS	Working
570	69	SVIMS/CT.RR /04/2009/0495	Euro 585	CT Surgery RR	NC	Syringe Pump	Fresenius	Injectomat	20497442	Mitie	5Y	04-07-09	04-06-14	SVIMS	Working
571	70	SVIMS/CT.RR /04/2009/0496	Euro 585	CT Surgery RR	NC	Syringe Pump	Fresenius	Injectomat	20497423	Mitie	5Y	04-07-09	04-06-14	SVIMS	Working
572	71	SVIMS/CT.RR /04/2009/0497	Euro 585	CT Surgery RR	NC	Syringe Pump	Fresenius	Injectomat	20497355	Mitie	5Y	04-07-09	04-06-14	SVIMS	Working
573	72	SVIMS/CT.RR /04/2009/0498	Euro 585	CT Surgery RR	NC	Syringe Pump	Fresenius	Injectomat	20497420	Mitie	5Y	04-07-09	04-06-14	SVIMS	Working
574	73	SVIMS/CT.RR /04/2009/0499	Euro 585	CT Surgery RR	NC	Syringe Pump	Fresenius	Injectomat	20497356	Mitie	5Y	04-07-09	04-06-14	SVIMS	Working
575	74	SVIMS/CT.RR /04/2009/0500	Euro 585	CT Surgery RR	NC	Syringe Pump	Fresenius	Injectomat	20497458	Mitie	5Y	04-07-09	04-06-14	SVIMS	Working
576	75	SVIMS/CT.RR /04/2009/0501	Euro 585	CT Surgery RR	NC	Syringe Pump	Fresenius	Injectomat	20497456	Mitie	5Y	04-07-09	04-06-14	SVIMS	Working
577	76	SVIMS/CT.RR /04/2009/0502	Euro 585	CT Surgery RR	NC	Syringe Pump	Fresenius	Injectomat	20497451	Mitie	5Y	04-07-09	04-06-14	SVIMS	Working
578	77	SVIMS/CT.RR /04/2009/0503	Euro 585	CT Surgery RR	NC	Syringe Pump	Fresenius	Injectomat	20497438	Mitie	5Y	04-07-09	04-06-14	SVIMS	Working
579	78	SVIMS/CT.RR /04/2009/0504	Euro 585	CT Surgery RR	NC	Syringe Pump	Fresenius	Injectomat	20497460	Mitie	5Y	04-07-09	04-06-14	SVIMS	Working
580	79	SVIMS/M/CT.ICU/ 06/2016/0505	Reagent Rental	CT Surgery RR	C	Blood Gas Analyzer	RadioMeter	Abl 800	754R2246 N0007	JK Medical		28/06/2016		Reagent Rental	Working
581	80	SVIMS/CT.ICU/02/ 2010/0506	IRS 4,04,683	**CT ICU**	**C**	Multi Para Monitor	Mindray	Beneview T8	CF-99103973	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
582	81	SVIMS/CT.ICU/02/ 2010/0507	IRS 4,04,683	**CT ICU**	**C**	Multi Para Monitor	Mindray	Beneview T8	CF-99104006	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working

583	82	SVIMS/CT.ICU/02/ 2010/0508	IRS 4,04,683	**CT ICU**	**C**	Multi Para Monitor	Mindray	Beneview T8	CF-99104008	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
584	83	SVIMS/CT.ICU/02/ 2010/0509	IRS 4,04,683	**CT ICU**	**C**	Multi Para Monitor	Mindray	Beneview T8	CF-99103975	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
585	84	SVIMS/CT.POW/02 /2010/0510	IRS 4,04,683	**CT ICU**	**C**	Multi Para Monitor	Mindray	Beneview T8	CF-99103969	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
586	85	SVIMS/CT.POW/11 /2011/0511	IRS 11,18,929	CT post operative Ward	C	ICU Ventilator	Tecme	Graphnet	9101 123 1080	Meditronic	2Y	11-01-11	31/10/2013	PMSSY-HLL	Working
587	86	SVIMS/CT.POW/11 /2011/0512	IRS 11,18,929	CT post operative Ward	C	ICU Ventilator	Tecme	Graphnet	9101 133 1080	Meditronic	2Y	11-01-11	31/10/2013	PMSSY-HLL	Not Working
588	87	SVIMS/CT.POW/04 /2010/0513		CT post operative Ward	C	Defibrillator	Philips	MRX	US00537833	US00537833	2Y	28/04/10	27/04/12	PMSSY-HLL	Working
589	88	SVIMS/CT.POW/04 /2009/0515	Euro 585	CT post operative Ward	NC	Syringe Pump	Fresenius	Injectomat	20497435	Mitie	5Y	04-07-09	04-06-14	SVIMS	Working
590	89	SVIMS/CT.POW/04 /2009/0516	Euro 585	CT post operative Ward	NC	Syringe Pump	Fresenius	Injectomat	20497436	Mitie	5Y	04-07-09	04-06-14	SVIMS	Working
591	90	SVIMS/CT.POW/04 /2009/0518	Euro 585	CT post operative Ward	NC	Syringe Pump	Fresenius	Injectomat	20497453	Mitie	5Y	04-07-09	04-06-14	SVIMS	Working
592	91	SVIMS/CT.POW/07 /2009/0519	IRS 37,146	CT post operative Ward	NC	Pulse Oximeter	MediAid	900P	EGO9G00191	Micronic	2Y	23/01/2010	22/01/2012	PMSSY-HLL	Working
593	92	SVIMS/CT.POW/07 /2009/0520	IRS 37,146	CT post operative Ward	NC	Pulse Oximeter	MediAid	900p	EGO9G00192	Micronic	2Y	23/01/2010	22/01/2012	PMSSY-HLL	Working
594	93	SVIMS/CT.POW/04 /2010/0521		CT post operative Ward	NC	Syringe Pump	Baxter	Sep-105	6606					SVIMS	Working
595	94	SVIMS/CT.RR /01/2020/1301		CT Surgery RR	NC	Syringe Pump	Smiths Medical	Graseby C9	18320 2926	M M Medical	5 Y	06.01.2020	05.01.2025	SVIMS	Working
596	95	SVIMS/CT.RR /01/2020/1302		CT Surgery RR	NC	Syringe Pump	Smiths Medical	Graseby C9	18320 2903	M M Medical	5 Y	06.01.2020	05.01.2025	SVIMS	Working
597	96	SVIMS/CT.RR /01/2020/1303		CT Surgery RR	NC	Syringe Pump	Smiths Medical	Graseby C9	18320 2905	M M Medical	5 Y	06.01.2020	05.01.2025	SVIMS	Working
598	97	SVIMS/CT.RR /01/2020/1304		CT Surgery RR	NC	Syringe Pump	Smiths Medical	Graseby C9	18320 2928	M M Medical	5 Y	06.01.2020	05.01.2025	SVIMS	Working
599	98	SVIMS/CT.RR /01/2020/1305		CT Surgery RR	NC	Syringe Pump	Smiths Medical	Graseby C9	18320 2902	M M Medical	5 Y	06.01.2020	05.01.2025	SVIMS	Working
600	1	SVIMS/GEE.OT/09 /2012/0522		**GE Extn/Lung OT**	**NC**	OT Light	Martin	V16 + V 10	1665, 1666	Vishal	5Y	21/09/12	20/09/17	SVIMS	Working
601	2	SVIMS/GEE.OT/08 /2013/0523		**GE Extn/Lung OT**	**NC**	OT Table	Trident	7000SB-Dr.Mac	2A207-MS-0038	Bet Medical	2Y	27/08/13	26/08/15	PMSSY-HLL	Working
602	3	SVIMS/Uro.OT/07/ 2013/0524		**GE Extn/Lung OT**	**NC**	Surgical Diathermy	Erbe	vio 300D	11318694	Trivitron	3Y	07-01-13	31/6/2015	SVIMS	Working
603	1	SVIMS/Uro.OT/06/ 2009/0525		**UROLOGY OT**	**NC**	OT Light	Martin	V16 + V 10	1669, 1670	Vishal	3y	26/06/09	25/06/12	PMSSY-APHMHIDC	Working
604	2	SVIMS/Uro.OT/06/ 2009/0526		UROLOGY OT	**NC**	OT Light	Martin	V16 + V 10	1680, 1681	Vishal	3y	26/06/09	25/06/12	PMSSY-APHMHIDC	Working
605	3	SVIMS/Uro.ROT/0 9/2012/0527		UROLOGY OT	**NC**	OT Light	Martin	V16 + V 10	2090, 2091	Vishal	5Y	21/09/12	20/09/17	SVIMS	Working
606	4	SVIMS/Uro.OT/08/ 2013/0528		UROLOGY OT	**NC**	OT Table	Trident	7000SB-Dr.Mac	2A207-MS-0036	Bet Medical	2Y	27/08/13	26/08/15	PMSSY-HLL	Working
607	5	SVIMS/Uro.OT/08/ 2013/0529		UROLOGY OT	**NC**	OT Table	Trident	7000SB-Dr.Mac	2A207-MS-0032	Bet Medical	2Y	27/08/13	26/08/15	PMSSY-HLL	Working

608	6	SVIMS/Uro.OT/03/2017/0530		UROLOGY OT	**NC**	OT Table	Dr.Max	7000SKBD	2A347-PC-0001	Bet Medical	5Y	22/03/2017	21/03/2022	SVIMS	Working
609	7	SVIMS/Uro.OT/01/2009/0531		UROLOGY OT	**NC**	Surgical Diathermy	Alsa	Excel 350 MCD	3676	Advanced Medical	3Y	01-05-09	01-04-12	SVIMS	Working
610	8	SVIMS/Uro.OT/09/2013/0532		**UROLOGY OT**	**NC**	Surgical Diathermy	Aesculap/B.Braun	GN300	4097	Sisco	3Y				Working
611	9	SVIMS/Uro.OT/01/2009/0533		UROLOGY OT	**NC**	Surgical Diathermy	Martin	ME411	303082679	Visdhal	3y				Working
612	10	SVIMS/Uro.OT/08/2012/0534		UROLOGY OT	**NC**	Mobile C-ARM	Siemens	Compact II	L/30923	Siemens	1Y	31/08/12	30/08/13	SVIMS	Working
613	11	SVIMS/Uro.OT/02/2014/0535		UROLOGY OT	**NC**	3 Chip Camera system	Stykar			Indian Orthocare	3Y	02-11-14	02-10-17	SVIMS	Working
				12A	**NC**	3 Chip camera	Stykar		14GO28214						**Not Working**
				12.2	**NC**	Camera console	Stykar	1188 HD 3 Chip	14G028034						Working
				12.3	**NC**	Light Source	Stykar	X-8000	14G009444						Working
				123.4	**NC**	Monitor	Stykar	Vision Elect HDTV	VEH261EO511						Working
614	12	SVIMS/Uro.OT/04/2015/0536		UROLOGY OT	**NC**	3 Chip camera with light source,processor & Monitor	Karl Storz	Image-1 H3-Z	0V846713-4	Vishal	3Y	24/04/2015	23/04/2018	SVIMS	Working
				13.1	**NC**	3 Chip camera	Karl Storz		OU846713-H						Working
				13.2	**NC**	Camera Console	Karl Storz	22201020	OU729128-P						Working
				13.3	**NC**	Light Source	Karl Storz	LED Nova 150	OT 4437						Working
				13.4	**NC**	Monitor	StorZ	9627NB/KsS-27	A008VVD19						Working
615	13	SVIMS/Uro.OT/09/2013/0537		UROLOGY OT	**NC**	3 Chip camera with light source,processor & Monitor	Aesculap/B.Braun	PV460,PV462 & OP932	1,00,71,014	Global Life care	2Y	19/9/2013	18/9/2015	PMSSY-HLL	Working
				14.1	**NC**	3 Chip camera	Aesculap/B.Braun		1,210						Working
				14.2	**NC**	Camera console	Aesculap/B.Braun	Full HD	1,007						Working
				14.3	**NC**	Light Source	Aesculap/B.Braun	AXEL 300	3,428						Working
				14.4	**NC**	Insufflator , 20Litres	Aesculap/B.Braun	Flow 20	6,992						Working
				14.5	**NC**	Monitor		SC-WU26-A1511	12-202869						Working
				14.6	**NC**	Monitor	Aesculap/B.Braun		12-211511						Working
				14.7	**NC**	Multi Flow Plus		PG 145	1211CE338						Working
616	14	SVIMS/Uro.OT/09/2013/0538		UROLOGY OT	**NC**	single Chip camera with light source,processo	Karl Storz								Working

						r & Monitor									
				15.1	**NC**	single Chip camera	Karl Storz								Working
				15.2	**NC**	Camera console	Karl Storz		YU741139-P						Working
				15.3	**NC**	Light Source	Karl Storz	LED Nova 150	NU3255						Working
				15.4	**NC**	Insufflator , 20Litres	Karl Storz	26430520	NT34305						Working
				15.5	**NC**	Monitor	Sony	LMD-2110MD	32,06,141						Working
617	15	SVIMS/Uro.OT/01/2011/0539	Euro 35705	UROLOGY OT	**NC**	Lithocast Master	EMS Medical		BCO1573	Health Ware	5Y	01-12-11	01-11-16	SVIMS	Working
618	16	SVIMS/Uro.OT/02/1993/0540		UROLOGY OT	**NC**	Endo Cold Light	Karl Storz	4878		Vishal	3Y	26/02/93	25/02/96	SVIMS	Working
619	17	SVIMS/Uro.OT/01/2016/0541		UROLOGY OT	**NC**	Argon Plasma coagulation	ERBE	ERBE VIO300D	11405752	Colloq	5Y	29/01/2016	28/01/2021	SVIMS	Working
620	18	SVIMS/Uro.OT/06/2016/0542	RS 66,00,908/-	UROLOGY OT	**NC**	Ultra Sound Scanner	BK	Flex Focus 800	5008034	Healthware	5Y	29/06/16	28/06/21	SVIMS	Working
621	19	SVIMS/Uro.OT/08/2016/0543		UROLOGY OT	**NC**	Laser System	Sphinx	SPHNIX Junior	334	Healthware	5Y	08-04-16	08-03-21	SVIMS	Working
622	20	SVIMS/Uro.OT/02/2018/1099	Rs.39,58,910/-	UROLOGY OT	**NC**	Lower Track Endoscope Set Adult	Karl Storz, Germany		120D8M	Vishal Surgical	5 Y	23.02.2018	22.02.2019	SVIMS	Working
623	21	SVIMS/Uro.RR/09/2009/0544	IRS 4,04,683	Urology RR	**NC**	Multi Para Monitor	Mindray	Beneview T8	CF-9A104656	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
624	22	SVIMS/Uro.RR/09/2009/0545	IRS 4,04,683	Urology RR	**NC**	Multi Para Monitor	Mindray	Beneview T8	CF-9A104630	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
625	23	SVIMS/Uro.RR/09/2009/0546	IRS 4,04,683	Urology RR	**NC**	Multi Para Monitor	Mindray	Beneview T8	CF-99103992	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
626	24	SVIMS/Uro.RR/09/2009/0547	IRS 4,04,683	Urology RR	**NC**	Multi Para Monitor	Mindray	Beneview T8	CF-99104007	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
627	25	SVIMS/Uro.RR/09/2009/0548	IRS 4,04,683	Urology RR	**NC**	Multi Para Monitor	Mindray	Beneview T8	CF-99103980	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
628	26	SVIMS/Uro.RR/09/2009/0549	IRS 4,04,683	Urology RR	**NC**	Multi Para Monitor	Mindray	Beneview T8	CF-99103982	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
629	27	SVIMS/URO.RR/08/2011/0550/C	IRS 11,18,929	Urology RR	C	ICU Ventilator	Tecme	Graphnet	9101 128 1080	Meditronic	2Y	11-01-11	31/10/2013	PMSSY-HLL	Working
630	28	SVIMS/URO.RR/08/2011/0551/C	IRS 11,18,929	Urology RR	C	ICU Ventilator	Tecme	Graphnet	9101 112 1080	Meditronic	2Y	11-01-11	31/10/2013	PMSSY-HLL	Working
631	29	SVIMS/URO.RR/08/2011/0552/C	IRS 11,18,929	Urology RR	C	ICU Ventilator	Tecme	Graphnet	9101 111 1080	Meditronic	2Y	11-01-11	31/10/2013	PMSSY-HLL	Working
632	30	SVIMS/URO.RR/08/2011/0553	IRS 11,18,929	Urology RR	C	ICU Ventilator	Tecme	Graphnet	9101 140 1080	Meditronic	2Y	12-01-11	31/10/2013	PMSSY-HLL	Working
633	31	SVIMS/URO.RR/05/2012/0554	IRS 24,500	Urology RR	NC	Syringe Pump	Orange Medical	Prima	1112354Z	Orange Medical	2Y	18/05/2012	17/05/2014	SVIMS	Working
634	32	SVIMS/URO.RR/05/2012/0555	IRS 24,500	Urology RR	NC	Syringe Pump	Orange Medical	Prima	1112355Z	Orange Medical	2Y	18/05/2012	17/05/2014	SVIMS	Working
635	33	SVIMS/URO.RR/06/2016/0556		Urology RR	NC	Syringe Pump	Plenum Tech Pvt Ltd	Zion +	1384	Plenum Tech	3Y			SVIMS	Working

636	34	SVIMS/URO.RR/06/2016/0557		Urology RR	NC	Syringe Pump	Plenum Tech Pvt Ltd	Zion +	1395	Plenum Tech	3Y			SVIMS	Working
637	35	SVIMS/URO.RR/01/2010/0558	IRS 37,146	Urology RR	NC	Pulse Oximeter	MediAid	900P	EGO9G00173	Micronic	2Y	23/01/2010	22/01/2012	PMSSY-HLL	Working
638	36	SVIMS/URO.RR/02/2010/0560	IRS 37,146	Urology RR	NC	Pulse Oximeter	MediAid	900P	EGO9G00166	Micronic	2Y	23/01/2013	22/01/2015	PMSSY-HLL	Working
639	37	SVIMS/UrWard/02/1993/0561	IRS 37,146	Urology RR	NC	Pulse Oximeter	MediAid	900P	EGO9G00171	Micronic	2Y	23/01/2012	22/01/2014	PMSSY-HLL	Working
640	38	SVIMS/UrWard/11/2012/0562		UROLOGY ward	NC	Uro flowmetry-OPD	Status Medical		జనవరి-02	Status	1Y	16/08/2017	15/08/2018	SVIMS	Working
641	39	SVIMS/UrWard/11/2012/0563		UROLOGY ward	NC	Uro flowmetry - Ward	Dan	danflow 3000	271/47	Jai medics	2Y	23/05/2012	22/05/2014	SVIMS	Working
642	40	SVIMS/UrWard/02/2014/0564		UROLOGY ward	NC	Urodynamic System	Laborie, Canada	Doroto KT	rkt-1-13061569	kailesh	2Y	24/2/2014	23/2/2016	PMSSY-HLL	Working
643	41	SVIMS/UrWard/02/2010/0565	IRS 4,04,683	UROLOGY ward	NC	Multi Para Monitor	Mindray	Beneview T8	CF-99103993	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
644	42	SVIMS/UrWard/10/2006/0566	IRS 4,04,683	UROLOGY ward	NC	Multi Para Monitor	Mindray	Beneview T8	CF-99103974	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
645	43	SVIMS/UrWard/10/2006/0567		UROLOGY ward	NC	Syringe Pump	Baxter	SEP-105	27-08-65						Working
646	44	SVIMS/ ur.Ward/01/2012/0569		UROLOGY ward	NC	Pulse Oximeter	MediAid		EGO9G00184	Micronic	2Y	23/01/2012	22/01/2014	PMSSY-HLL	Working
647	45	SVIMS/ URO.RR./06/2018/1116	Irs 1,29,074/-	Urology	NC	Multi Para Monitor	Mindray	UMEC 12	KQ-84011710	Green apple	5Y	06-07-18	06-06-23	SVIMS	Working
648	46	**SVIMS/Uro.OT/08/2016/1170**		**Urology OT**	**NC**	**Ureteroscope**	**Olympus**	**N4502130**	**2513751**	**Olyumpus**	**5Y**	08-04-16	**08-03-21**	**SVIMS**	**Working**
		SVIMS/Uro.OT/08/2016/1170A		**Urology OT**	**NC**	**Leakage Tester for Flexible Olympus Endoscopes**	**Olympus**	**WA23080A**		**Olyumpus**	**5Y**	08-04-16	**08-03-21**	**SVIMS**	**Working**
		SVIMS/Uro.OT/08/2016/1170B		**Urology OT**	**NC**	**Lg-Adapter Olympus Telescopeto olympus Lg Cable**	**Olympus**	**A0460**		**Olyumpus**	**5Y**	08-04-16	**08-03-21**	**SVIMS**	**Working**
		SVIMS/Uro.OT/08/2016/1170C		**Urology OT**	**NC**	**Lg-Adapter Oes Telescope To Wolf Lg Cable**	**Olympus**	**332**		**Olyumpus**	**5Y**	08-04-16	**08-03-21**	**SVIMS**	**Working**
		SVIMS/Uro.OT/08/2016/1170D		**Urology OT**	**NC**	**Irp[ass AS 10/12Fr X 38 Cm**	**Olympus**	**610388X**		**Olyumpus**	**5Y**	08-04-16	**08-03-21**	**SVIMS**	**Working**
		SVIMS/Uro.OT/08/2016/1170E		**Urology OT**	**NC**	**Ultra-Catch NT (1.8 Fr X 115 cm) Stone**	**Olympus**	**NT4W18115**		**Olyumpus**	**5Y**	08-04-16	**08-03-21**	**SVIMS**	**Working**

						Retrieval Device									
		SVIMS/Uro.OT/08/2016/1170F		**Urology OT**	**NC**	**Clh-250 Halogen Light Source 220V Syymbol Version**	**Olympus**	**4604362**	**7657864**	**Olyumpus**	**5Y**	08-04-16	**08-03-21**	**SVIMS**	**Working**
		SVIMS/Uro.OT/08/2016/1170G		**Urology OT**	**NC**	**Light Guide Size M Plug Type 3 M Cf Type**	**Olympus**	**WA03310A**	**15ZW0002**	**Olyumpus**	**5Y**	08-04-16	**08-03-21**	**SVIMS**	**Working**
649	47	SVIMS/ URO.RR./01/2020/1300		Urology RR		Syringe Pump	Smiths Medical	Graseby C9	18320 2809	M M Medical	5 y	06.01.2020	05.01.2025	SVIMS	Working
650	1	SVIMS/NS. OT/06/2009/0570		**Neuro Surgery OT**	NC	OT Light	Martin	V16 + V 10	1676, 1676	Vishal	3Y	26/06/09	25/06/12	PMSSY-HLL	Working
651	2	SVIMS/NS. OT/06/2009/0571		Neuro Surgery OT	NC	OT Light	Martin	V16 + V 10	16631664	Vishal	3Y	26/06/09	25/06/12	PMSSY-HLL	Working
652	3	SVIMS/M/NS. OT/01/2000/0572		Neuro Surgery OT	NC	Surgical Diathermy	Alsa	Excel 350 MCD	4973	Advanced Medical	5Y	2000	2005	SVIMS	Working
653	4	SVIMS/NS. OT/05/2006/0573		Neuro Surgery OT	NC	Surgical Diathermy	Alsa	Excel 350 MCD	5200	Advanced Medical	5Y	17/05/06	16/05/11	SVIMS	Working
654	5	SVIMS/NS. OT/04/1993/0574		Neuro Surgery OT	NC	OT Table	Mizaho	EM 5501	90820520	Moola Tools	3Y	18/04/93	17/04/96	SVIMS	Working
655	6	SVIMS/NS. OT/01/2013/0575		Neuro Surgery OT	NC	OT Table	Berchtold	D850	3501110-T-10463	Venus	5Y	23/01/2013	22/01/2018	SVIMS	Working
656	7	SVIMS/NS. OT/08/2013/0576		Neuro Surgery OT	NC	OT Table	Trident	7000SB-Dr.Mac	2A207-MS-0034	Bet Medical	2Y	19/08/2013	18/08/2015	PMSSY-HLL	Working
657	8	SVIMS/NS. OT/08/2012/0577		Neuro Surgery OT	NC	Mobile C-ARM	Siemens	Compact II	L/30922	Siemens	1Y	31/08/2012	30/08/2013	SVIMS	Working
658	9	SVIMS/NS. OT/01/2010/0578		Neuro Surgery OT	NC	High Speed Drill	Stryker	Electrc Drill	924301513	Indian ortho	5Y	2010	2015	SVIMS	Working
659	10	SVIMS/NS. OT/02/1993/0579		Neuro Surgery OT	NC	Operating Microscope	Carl Zeiss	DXC 107AP	2244978	Toshnival	3Y	26/02/93	26/02/96	SVIMS	Working
660	11	SVIMS/NS. OT/05/2015/0580		Neuro Surgery OT	NC	Operating Microscope	Leica	M720, OH5	70514-OH5	Leica India	5Y	13/5/2015	05-12-20	SVIMS	Working
661	12	SVIMS/NS. OT/02/1993/0581		Neuro Surgery OT	NC	Fibre Optic Light Source	Cuda	M2150	129218	Sisco	3Y	26/02/93	25/02/96	SVIMS	Working
662	13	SVIMS/NS. OT/12/2000/0582		Neuro Surgery OT	NC	Neuro Endo System	Karl Storz			Vishal	3Y	12-01-00	31/11/2003	SVIMS	Working
				14.1	NC	Camera	Karl Storz	H3-Z	OU846636-H						
				14.2	NC	Camera console	Karl Storz	22201020	OU729116-P						
				14.3	NC	Light Source	Karl Storz	LED Nova 150	NU3224						
				14.4	NC	Monitor	Karl Storz	9627NB/KS27	A026ZV020						
663	14	SVIMS/N. OT/01/2016/0583		Neuro Surgery OT	NC	cusa System	Stryker	Cusa	5420-852-000	Strykar	3Y	01-11-16	01-10-19	SVIMS	Working
664	15	SVIMS/NS. OT/07/2012/0584		Neuro Surgery OT	NC	Power drill	medtronics	MidasRerx	56535	SS associate	1Y	28/07/2012	27/07/2013	SVIMS	Working
665	16	SVIMS/NS. OT/06/2016/0585	Rs 36, 22, 500/-	Neuro Surgery OT	NC	Ultra Sonic Bone Scapal	Misonic	Bone Scalpal	NY11735	Annulus	5Y	27/06/2016	26/06/2021	SVIMS	Working

666	17	SVIMS/NS. OT/12/2016/0586		Neuro Surgery OT	NC	Intra Operative Neuro Monitor	medtronics	NIM ECLIPSE	X06316110	SS associate	5Y	20/12/16	19-12-21	SVIMS	Working
667	18	SVIMS/NS. OT/02/2010/0587	IRS 4,04,683	Neuro Surgery RR	C	Multi Para Monitor	Miindray	Beneview T8	CF-99103968	Instromedic	2y	02-04-10	02-03-12	PMSS Y-HLL	Working
668	19	SVIMS/NS. OT/02/2010/0588	IRS 4,04,683	Neuro Surgery RR	C	Multi Para Monitor	Miindray	Beneview T8	CF-99104015	Instromedic	2y	02-04-10	02-03-12	PMSS Y-HLL	Working
669	20	SVIMS/NS. OT/02/2010/0589	IRS 4,04,683	Neuro Surgery RR	C	Multi Para Monitor	Miindray	Beneview T8	CF-99103994	Instromedic	2y	02-04-10	02-03-12	PMSS Y-HLL	Not Working
670	21	SVIMS/NS. OT/02/2010/0590	IRS 4,04,683	Neuro Surgery RR	C	Multi Para Monitor	Miindray	Beneview T8	CF-99104004	Instromedic	2y	02-04-10	02-03-12	PMSS Y-HLL	Not Working
671	22	SVIMS/NS. OT/02/2010/0591	IRS 4,04,683	Neuro Surgery RR	C	Multi Para Monitor	Miindray	Beneview T8	CF-99103995	Instromedic	2y	02-04-10	02-03-12	PMSS Y-HLL	Working
672	23	SVIMS/NS. OT/02/2010/0592	IRS 24,181	Neuro Surgery RR	C	Syringe Pump	Neuron BioMed	SP 102	609281	L & T	2Y	02-01-10	31/1/2012	PMSS Y-HLL	Working
673	24	SVIMS/NS. OT/02/2010/0593	IRS 24,181	Neuro Surgery RR	C	Syringe Pump	Neuron BioMed	SP 102	1109108	L & T	2Y	02-01-10	31/1/2012	PMSS Y-HLL	Working
674	25	SVIMS/NS. OT/11/2009/0595	IRS 11,18,928	Neuro Surgery RR	C	ICU Ventilator	GE Datex	Engstrom	CBCN 01000	GE Datex India	2y	30/11/2009	29/11/2011	PMSS Y-HLL	Working
675	26	SVIMS/NS. OT/09/2012/0596		Neuro Surgery RR	C	Debifrillator	Medtronics	LifePak	40173639	Instromedix	2Y	21/09/12	20/09/14	PMSS Y-HLL	Working
676	27	SVIMS/NS. OT/03/2009/0597	Euro 585	Neuro Surgery RR	NC	Syringe Pump	Fresenius	Injectomat/Agilia	20497444	Medi	5Y	19/03/09	18/03/14	SVIMS	Working
677	28	SVIMS/NS. OT/03/2009/0598	Euro 585	Neuro Surgery RR	NC	Syringe Pump	Fresenius	Injectomat/Agilia	20497425	Medi	5Y	19/03/09	18/03/14	SVIMS	Working
678	29	SVIMS/NS. OT/03/2009/0599/C	Euro 585	Neuro Surgery RR	NC	Syringe Pump	Fresenius	Injectomat/Agilia	20497437	Medi	5Y	19/03/09	18/03/14	SVIMS	Working
679	30	SVIMS/NS. OT/08/2011/0600/C	IRS 11,18,929	Neuro Surgery ward	C	ICU Ventilator	Tecme	Graphnet	091011311080 AIV	Meditronic	2Y	10-01-11	31/09/2013	PMSS Y-HLL	Working
680	31	SVIMS/NS. OT/08/2011/0601	IRS 11,18,929	Neuro Surgery ward	C	ICU Ventilator	Tecme	Graphnet	09 1011351080 AIV	Meditronic	2Y	10-01-11	31/09/2013	PMSS Y-HLL	Working
681	32	SVIMS/NS. OT/02/2010/0602	IRS 4,04,683	Neuro Surgery ward	NC	Multi Para Monitor	Mindray	Beneview T8	CF-99103990	Instromedic	2y	02-04-10	02-03-12	PMSS Y-HLL	Working
682	33	SVIMS/NS. OT/01/2010/0603	IRS 37,146	Neuro Surgery ward	NC	Pulse Oximeter	MediAid	900P	EGO9G00180	Micronic	2Y	23/01/2010	22/01/2012	PMSS Y-HLL	Working
683	34	SVIMS/NS. OT/10/2006/0606	IRS 37,146	Neuro Surgery ward	NC	Pulse Oximeter	MediAid	900P	EGO9G00200	Micronic	2Y	23/01/2010	22/01/2012	PMSS Y-HLL	Working
684	35	SVIMS/NS. OT/10/2006/0607		Neuro Surgery ward	NC	Syringe Pump	Baxter	Aitecs	71060		3Y	10-12-06	10-11-09	SVIMS	Working
685	36	SVIMS/NS. OT/10/2006/0608		Neuro Surgery ward	NC	Syringe Pump	Baxter	Aitecs	47406		3Y	10-12-06	10-11-09	SVIMS	Working
686	37	SVIMS/NS. OT/10/2006/0609		Neuro SurgeryOT	NC	C-Arm	Allenger	HF-49	2K1005190-C	Allenger	2Y	07-12-10	07-11-12	PMSS Y-HLL	Working
687	38	SVIMS/Neusur/06/2019/1172		Neurosurgery (NSRR)	NC	Syringe Pump	Smiths Medical	Grase by C9	18320 2914	M M Medical	5 y	17.06.2019	16.06.2024	SVIMS	Working
688	39	SVIMS/Neusur/06/2019/1173		Neurosurgery (NSRR)	NC	Syringe Pump	Smiths Medical	Grase by C9	18320 2895	M M Medical	5 y	17.06.2019	16.06.2024	SVIMS	Working
689	40	SVIMS/Neusur/06/2019/1174		Neurosurgery (NSRR)	NC	Syringe Pump	Smiths Medical	Grase by C9	18320 2804	M M Medical	5 y	17.06.2019	16.06.2024	SVIMS	Working
690	41	SVIMS/Neusur/06/2019/1175		Neurosurgery (NSRR)	NC	Syringe Pump	Smiths Medical	Grase by C9	18320 2923	M M Medical	5 y	17.06.2019	16.06.2024	SVIMS	Working
691	42	SVIMS/Neusur/07/2005/1228		Neurosurgery (NSRR)	NC	Patient Monitor	Philips	MP 20	DE50405086	Philips	3Y	14/07/05			
692	43	SVIMS/Neusur/01/2		Neurosurgery (NSRR)		Syringe Pump	Smiths	Graseby C9	18320 2961	M M	5 Y	06.01.20	05.01.2025	SVIMS	Working

		020/1296					Medical			Medical		20			
693	44	SVIMS/Neusur/01/2020/1297		Neurosurgery (NSRR)		Syringe Pump	Smiths Medical	Graseby C9	18320 2899	M M Medical	5 Y	06.01.2020	05.01.2025	SVIMS	Working
694	45	SVIMS/Neusur/01/2020/1298		Neurosurgery (NSRR)		Syringe Pump	Smiths Medical	Graseby C9	18320 2946	M M Medical	5 Y	06.01.2020	05.01.2025	SVIMS	Working
695	46	SVIMS/Neusur/01/2020/1299		Neurosurgery (NSRR)		Syringe Pump	Smiths Medical	Graseby C9	18320 2888	M M Medical	5 Y	06.01.2020	05.01.2025	SVIMS	Working
696	1	SVIMS/GE. OT/02/2017/0610	Rs 19,00,000/-	**Gastro Enterology OT**	NC	OT Light	BenQ	Trilite LS810-750	ZE38Z-P9-0001	Bet Medical	5Y	18/0/2017.	17/0/2022	SVIMS	Working
697	2	SVIMS/GE. OT/08/2013/0611		Gastro Enterology OT	NC	OT Table	Trident	7000SB-Dr.Mac	2A207-MS-0037	Bet Medical	2Y	27/08/13	256/08/15	PMSSY-HLL	Working
698	3	SVIMS/GE. OT/01/2009/0612		Gastro Enterology OT	NC	Surgical Diathermy	Alsa	Excel 350 MCDX	3677	Advanced	3Y	01-05-09	01-04-12	SVIMS	working
699	4	SVIMS/GE. OT/01/1992/0613		Gastro Enterology OT	NC	Endo Light Source	Karl Storz	Xenon 175		Vishal	3Y	1992	1995	SVIMS	Working
700	5	SVIMS/GE. OT/ 01/1992/614		Gastro Enterology OT	NC	Endoflator-Electronic	Karl Storz	264305 20	NT34314	Vishal	3Y	1993		SVIMS	Working
701	6	SVIMS/GE. OT/01/1992/0615		6	NC	Laprascope system									
		SVIMS/GE. OT/01/1992/0615A		6.1	NC	single Chip camera	Karl Storz		xu858384-h		3y				
		SVIMS/GE. OT/01/1992/0615B		6.2	NC	Camera console	Karl Storz	20223020	YU741135-P						
		SVIMS/GE. OT/01/1992/0615C		6.3	NC	Light Source	Karl Storz	20161220	OT441						
		SVIMS/GE. OT/01/1992/0615D		6.4	NC	Insufflator , 20Litres	Karl Storz	26430520	NT34314						
		SVIMS/GE. OT/01/1992/0615E		6.5	NC	Monitor	Sony	LMD-2110MD	3206133-S						
702	7	SVIMS/GE. OT/01/2009/0616	Rs 23,20,679/-	Gastro Enterology OT	NC	Laproscope SYSTEM	Strykar	Hi Di 3 Chip		Indian orthocare	5Y	27/01/2009	26/01/2014	SVIMS	Working
		SVIMS/GE. OT/01/2009/0616A		7A	NC	3 Chip camera	Strykar	1088iHD	08F027634						
		SVIMS/GE. OT/01/2009/0616B		7B	NC	Camera console	Strykar	1088iHD	08F032034						
		SVIMS/GE. OT/01/2009/0616C		7C	NC	Light Source	Strykar	X8000	71008484						
		SVIMS/GE. OT/01/2009/0616D		7D	NC	Insufflator	Strykar	40L	0901CE238						
		SVIMS/GE. OT/01/2009/0616E		7E	NC	Monitotr	Strykar	Vision Elect HDTV	SVE21910078						
703	8	SVIMS/GE. OT/04/2003/0617		Gastro Enterology OT	NC	Harmonic Scapel	J&J	Gen 3	Gn 4023566	J&J india	3Y	04-05-03	04-04-06	SVIMS	Working
704	9	SVIMS/GE. OT/01/2016/0618		Gastro Enterology OT	NC	Vessal Sealing System	ERBE	ERBE VIO 300D	11405826	Colloq	5Y	29/01/2016	28/01/2021	SVIMS	Working
705	10	SVIMS/GE. OT/07/2016/0619	RS 4,90,000/-	Gastro Enterology OT	NC	Argon Plasma Coagulation	EMED	ES 350	363097	Indian Orthiocare	5y	25/07/2016	24/07/2021	SVIMS	Working
706	11	SVIMS/GE. OT/07/2016/0620	RS 26, 85, 901/-	Gastro Enterology OT	NC	**Laproscope system**	Olympus			Healthware	5Y	15/07/2016	14/07/2021	SVIMS	Working
		SVIMS/GE. OT/07/2016/0620A			NC	Camera	Olympus	CH-S190E-XZ-E	7606353	Healthware					

		SVIMS/GE. OT/07/2016/0620B			NC	Video Processor	Olympus	OTV-S190	7680948	Healthware					
		SVIMS/GE. OT/07/2016/0620C			NC	Light Source-Xenon	Olympus	CLV-S190	7510832	Healthware					
		SVIMS/GE. OT/07/2016/0620D			NC	Insufflator	Olympus	N3493000	7620563	Healthware					
		SVIMS/GE. OT/07/2016/0620E			NC	Monitor	Olympus	OEV262H-E	7534723	Healthware					
707	12	SVIMS/GE. OT/02/2010/0621	IRS 4,04,683	Gastro Enterology RR	C	Multi Para Monitor	Mindray	Beneview T8	CF-99103978	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
708	13	SVIMS/GE. OT/02/2010/0622	IRS 4,04,683	Gastro Enterology RR	C	Multi Para Monitor	Mindray	Beneview T8	CF-9A1034635	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
709	14	SVIMS/GE. OT/02/2010/0623	US$6493	Gastro Enterology RR	C	Multi Para Monitor	Philips	MP 20	DE50405088	Philips	3Y				Working
710	15	SVIMS/GE. OT/02/2010/0624	US$6493	Gastro Enterology RR	C	Multi Para Monitor	Philips	MP 20	DE72838325	Philips	3Y				Working
711	16	SVIMS/GE. OT/02/2010/0625	US$6493	Gastro Enterology RR	C	Multi Para Monitor	Philips	MP 20	DE72838215	Philips	3Y				Working
712	17	SVIMS/GE. OT/02/2010/0626	IRS 4,04,683	Gastro Enterology ICU	C	Multi Para Monitor	Mindray	Beneview T8	CF-9A104645	Instromedic		02-04-10	02-03-12	PMSSY-HLL	Working
713	18	SVIMS/GE. OT/02/2010/0627	IRS 4,04,683	Gastro Enterology ICU	C	Multi Para Monitor	Mindray	Beneview T8	CF-9A104668	Instromedic		02-04-10	02-03-12	PMSSY-HLL	Working
714	19	SVIMS/GE. OT/02/2010/0628	IRS 4,04,683	Gastro Enterology ICU	C	Multi Para Monitor	Mindray	Beneview T8	CF-9A104650	Instromedic		02-04-10	02-03-12	PMSSY-HLL	Working
715	20	SVIMS/GE. OT/02/2010/0629	IRS 4,04,683	Gastro Enterology ICURR	C	Multi Para Monitor	Mindray	Beneview T8	CF-9A104639	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
716	21	SVIMS/GE. OT/02/2010/0630	IRS 4,04,683	Gastro Enterology ICU	C	Multi Para Monitor	Mindray	Beneview T8	CF-9A104003	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
717	22	SVIMS/GE. OT/02/2010/0631	IRS 4,04,683	Gastro Enterology Ward	C	Multi Para Monitor	Mindray	Beneview T8	CF-9A104643	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
718	23	SVIMS/GE. OT/02/2010/0632	IRS 4,04,683	Gastro Enterology Ward	C	Multi Para Monitor	Mindray	Beneview T8	CF-9A104654	Instromedic	2y	02-04-10	02-03-12	PMSSY-HLL	Working
719	24	SVIMS/GE. OT/02/2010/0633/C	IRS 4,04,683	Gastro Enterology Ward	C	Multi Para Monitor	Mindray	Beneview T8	CF-9A104632	Instromedic	2y	02-04-10	02-03-12		Working
720	25	SVIMS/GE. OT/11/2009/0634/C	IRS 11,18,932	Gastro Enterology RR	C	ICU Ventilator	GE Datex	Engstrom	CBCN 01476	GE Datex India	2y	30/11/2009	29/11/2011	PMSSY-HLL	Working
721	26	SVIMS/GE. OT/11/2009/0635/C	IRS 11,18,932	Gastro Enterology RR	C	ICU Ventilator	GE Datex	Engstrom	CBCN 01479	GE Datex India	2y	30/11/2009	29/11/2011	PMSSY-HLL	Working
722	27	SVIMS/GE. OT/11/2009/0636/C	IRS 11,18,932	Gastro Enterology RR	C	ICU Ventilator	GE Datex	Engstrom	CBCN 01500	GE Datex India	2y	30/11/2009	29/11/2011	PMSSY-HLL	Working
723	28	SVIMS/GE. OT/11/2009/0637/C	IRS 11,18,932	Gastro Enterology RR	C	ICU Ventilator	GE Datex	Engstrom	CBCN 01007	GE Datex India	2y	30/11/2009	29/11/2011	PMSSY-HLL	Working
724	29	SVIMS/GE. OT/11/2009/0638/C	IRS 11,18,932	Gastro Enterology RR	C	ICU Ventilator	GE Datex	Engstrom	CBCN 00994	GE Datex India	2y	30/11/2009	29/11/2011	PMSSY-HLL	Working
725	30	SVIMS/GE. OT/11/2009/0639	IRS 11,18,932	Gastro Enterology RR	C	ICU Ventilator	GE Datex	Engstrom	CBCN 01002	GE Datex India	2y	30/11/2009	29/11/2011	PMSSY-HLL	Working

726	31	SVIMS/GE. OT/05/2013/0640	IRS 24,500	Gastro Enterology RR	NC	Syringe Pump	Organge	Flow Prima	13050555-Z	Organge Medical	2y	23/05/13	22/05/15	SVIMS	Working
727	32	SVIMS/GE. OT/05/2013/0641	IRS 24,500	Gastro Enterology RR	NC	Syringe Pump	Organge	Flow Prima	13050556-Z	Organge Medical	2y	23/05/13	22/05/15	SVIMS	Working
728	33	SVIMS/GE. OT/05/2013/0642	IRS 24,500	Gastro Enterology RR	NC	Syringe Pump	Organge	Flow Prima	13050557-Z	Organge Medical	2y	23/05/13	22/05/15	SVIMS	Working
729	34	SVIMS/GE. OT/05/2013/0643	IRS 24,500	Gastro Enterology RR	NC	Syringe Pump	Organge	Flow Prima	13050558-Z	Organge Medical	2Y	23/05/13	22/05/15	SVIMS	Working
730	35	SVIMS/GE. OT/05/2013/0644	IRS 24,500	Gastro Enterology RR	NC	Syringe Pump	Organge	Flow Prima	13050559-Z	Organge Medical	2Y	23/05/13	22/05/15	SVIMS	Working
731	36	SVIMS/GE. OT/06/2016/0645	Rs 29,252.71	Gastro Enterology RR	NC	Syringe Pump	Plenum Tech Pvt Ltd	Zion +	1823	Plenum Tech	2Y	15/06/2016	14/06/2019	SVIMS	Working
732	37	SVIMS/GE. OT/06/2016/0646	Rs 29,252.71	Gastro Enterology RR	NC	Syringe Pump	Plenum Tech Pvt Ltd	Zion +	1833	Plenum Tech	2Y	15/06/2016	14/06/2019	SVIMS	Working
733	38	SVIMS/GE. OT/06/2016/0647	Rs 29,252.71	Gastro Enterology RR	NC	Syringe Pump	Plenum Tech Pvt Ltd	Zion +	1801	Plenum Tech	2Y	15/06/2016	14/06/2019	SVIMS	Working
734	39	SVIMS/GE. OT/06/2016/0648	Rs 29,252.71	Gastro Enterology RR	NC	Syringe Pump	Plenum Tech Pvt Ltd	Zion +	1819	Plenum Tech	3Y	15/06/2016	14/06/2019	SVIMS	Working
735	40	SVIMS/GE. OT/06/2016/0649	Rs 29,252.71	Gastro Enterology RR	NC	Syringe Pump	Plenum Tech Pvt Ltd	Zion +	1747	Plenum Tech	2Y	15/06/2016	14/06/2018	SVIMS	Working
736	41	SVIMS/GE. OT/07/2016/0650		Gastro Enterology RR	C	Defibrillator	Mindray	BeneHeart D3	EL-65027004	Green Apple	2Y	18/07/2016	17/07/2018	SVIMS	Working
737	42	SVIMS/GE. OT/03/2009/0651	Euro 585	Gastro Enterology RR	NC	Syringe Pump	Fresenius	Injectomat/Agilia	20497432	Midi	3Y	19/03/09	18/03/14	SVIMS	Working
738	43	SVIMS/GE. OT/03/2009/0653	Euro 585	Gastro Enterology RR	NC	Syringe Pump	Fresenius	Injectomat/Agilia	20497455	Medi	5Y	19/03/09	18/03/14	SVIMS	Working
739	44	SVIMS/GE. OT/03/2009/0654	Euro 585	Gastro Enterology RR	NC	Syringe Pump	Fresenius	Injectomat/Agilia	20497443	Medi	5Y	19/03/09	18/03/14	SVIMS	Working
740	45	SVIMS/GE. OT/10/2008/0655		GE RR Extention	C	Patient Monitor	Philips	MP 60	DE73113027	Philips	5Y	29/10/08	28/10/11	SVIMS	Working
741	46	SVIMS/GE. OT/10/2008/0656		GE RR Extention	C	Patient Monitor	Philips	MP 60	DE73113002	Philips	5Y	29/10/08	28/10/11	SVIMS	Working
742	47	SVIMS/GE. OT/10/2008/0657		GE RR Extention	C	Patient Monitor	Philips	MP 60	DE73113038	Philips	5Y	29/10/08	28/10/11	SVIMS	Working
743	48	SVIMS/GE. OT/10/2008/0658		GE RR Extention	C	Patient Monitor	Philips	MP60	DE73113032	Philips	3Y	29/10/08	28/10/11	SVIMS	Working
744	49	SVIMS/GE. OT/10/2008/0659		GE RR Extention	C	Patient Monitor	Philips	MP 60	DE73113045	Philips	3Y	29/10/08	28/10/11	SVIMS	Working
745	50	SVIMS/GE. OT/10/2008/0660		GE RR Extention	C	Patient Monitor	Philips	MP 60	DE73113033	Philips	3Y	29/10/08	28/10/11	SVIMS	Working
746	51	SVIMS/GE. OT/10/2008/0661		GE RR Extention	C	Patient Monitor	Philips	MP 60	DE73113046	Philips	3Y	29/10/08	28/10/11	SVIMS	Working
747	52	SVIMS/GE. OT/10/2008/0662		GE RR Extention	C	Patient Monitor	Philips	MP 60	DE73113036	Philips	3Y	29/10/08	28/10/11	SVIMS	Working
748	53	SVIMS/SO.OT/09/2016/1245		GE RR	c	Multi Para Monitor	Bionet	BM5	D8N0300090	Vijetha	1Y	28/09/16	27/09/17	SVIMS	Working
749	54	SVIMS/GE. OT/10/2008/0663		Gastro Enterology Endoscope	NC	Processer & Light Source	Fujinon			Wipro	2Y	01-05-01	01-04-03	svims	Working

		SVIMS/GE. OT/10/2008/0663/A			NC	Monitor	Sony	Trinitron	6012226						
		SVIMS/GE. OT/10/2008/0663/B			NC	Light Source	Fujinon	EPX 201	795191						
750	55	SVIMS/GE. OT/02/2011/0664		Gastro Enterology Endoscope	NC	Endoscopy System - (Endoscope-2 Nos, Light Source & Video Processor, Monitor-3 Nos, Imaging System, UPS and trolley)	Fujinon			RFCL	3y	02-10-11	02-09-14	PMSS Y-HLL	Working
		SVIMS/GE. OT/02/2011/0664				GastroSDcvope									
		SVIMS/GE. OT/02/2011/0664/A				Light Source	Fujinon								
		SVIMS/GE. OT/02/2011/0664/A				Video Processor	Fujinon	EPX 2500	3V564A13 8						
		SVIMS/GE. OT/02/2011/0664/C				Monitor	Sony	LMD 1530W	3001818						
		SVIMS/GE. OT/02/2011/0664/D				Monitor	Sony	LMD 1530W	3001819-S						
		SVIMS/GE. OT/02/2011/0664/E				Monitor	Dell	P190SVB	CNOWGM 4N-74261						
						Imaging System									
751	56	SVIMS/GE. OT/09/2015/0665		Gastro Enterology Endoscope	NC	Endoscopy System	Olympus			Rs 29,90,264	3Y	23/09/20 15	22/09/2018	SVIMS	Working
						Gastr oScope	Olympus	GIF-Q150	2519813						**Workin g**
						ColonoScope	Olympus	CF-Q150L	2504853						Working
						Duodenovideos cope	Olympus	TJF-150	2501655						Working
						Processer & Light Source	Olympus	CV-150	7549776						Working
						Color Monitor	Eizo	LCD	20350055						Working
						(Olympu Endoscope-3 Nos,(GIF-Q150,CF-Q150L,TJF-150), Light Source & Video Processor, Monitor, Imaging System & trolley									
752	57	SVIMS/GE. OT/06/2016/0666		Gastro Enterology Endoscope	NC	Paediatric Video GastroScope	Olympus	GIF-XP150N	2512524	Healthware	5Y	22/06/20 16	21/06/2021	SVIMS	Working
753	58	SVIMS/GE. OT/09/2016/0667		Gastro Enterology Endoscope	NC	Choledochosco pe	Olympus	CHF TYPE V	2651045	Healthware	5Y	09-01-16	31/8/2021	SVIMS	Working
754	59	SVIMS/GE. OT/00/0000/1244				Pulse Oximeter	MediAid	900P	EG09G001 88						

755	1	SVIMS/SO. OT/02/2010/0668	IRS 4,04,683	**Surgical Oncology** RR	C	Multi Para Monitor	Mindray	Beneview T8	CF-99103971	Instromedic	2y	02-04-10	02-03-12	PMSS Y-HLL	Working
756	2	SVIMS/SO. OT/02/2010/0669	IRS 4,04,683	Surgical Oncology RR	C	Multi Para Monitor	Mindray	Beneview T8	CF-99104005	Instromedic	2y	02-04-10	02-03-12	PMSS Y-HLL	Working
757	3	SVIMS/SO. OT/02/2010/0670	IRS 4,04,683	Surgical Oncology RR	C	Multi Para Monitor	Mindray	Beneview T8	CF-99104014	Instromedic	2y	02-04-10	02-03-12	PMSS Y-HLL	Working
758	4	SVIMS/SO. OT/02/2010/0671	IRS 4,04,683	Surgical Oncology RR	C	Multi Para Monitor	Mindray	Beneview T8	CF-99104009	Instromedic	2y	02-04-10	02-03-12	PMSS Y-HLL	Working
759	5	SVIMS/SO. OT/02/2010/0672	IRS 4,04,683	Surgical Oncology Ward	C	Multi Para Monitor	Mindray	Beneview T8	CF-9A104641	Instromedic	2y	02-04-10	02-03-12	PMSS Y-HLL	Working
760	6	SVIMS/SO. OT/02/2010/0673	IRS 4,04,683	Surgical Oncology ward	C	Multi Para Monitor	Mindray	Beneview T8	CF-9A104659	Instromedic	2y	02-04-10	02-03-12	PMSS Y-HLL	Working
761	7	SVIMS/SurOnc/08/ 2019/1224		Surgical Oncology RR	C	Multi Para Monitor	Schiller Healthcare	Ttruscope Ultra Q5	Q068E 017983	Schiller Healthcare	5 Y	07.08.2019	06.08.2024	SVIMS	Working
762	8	SVIMS/SurOnc/08/ 2019/1225		Surgical Oncology RR	C	Multi Para Monitor	Schiller Healthcare	Ttruscope Ultra Q5	Q068E 017984	Schiller Healthcare	5 Y	07.08.2019	06.08.2024	SVIMS	Working
763	9	SVIMS/SurOnc/08/ 2019/1226		Surgical Oncology RR	C	Multi Para Monitor	Schiller Healthcare	Ttruscope Ultra Q5	Q068E 017985	Schiller Healthcare	5 Y	07.08.2019	06.08.2024	SVIMS	Working
764	10	SVIMS/SurOnc/08/ 2019/1227		Surgical Oncology RR	C	Multi Para Monitor	Schiller Healthcare	Ttruscope Ultra Q5	Q068E 017986	Schiller Healthcare	5 Y	07.08.2019	06.08.2024	SVIMS	Working
765	11	SVIMS/SO. OT/11/2009/0674	IRS 11,18,932	Surgical Oncology RR	C	ICU Ventilator	GE Datex Ohmeda	Engstrom	CBCN01006	GE Datex Ohmeda	2Y	26/12/09	25/12/2011	PMSS Y-HLL	Working
766	12	SVIMS/SO. OT/08/2011/0675	IRS 11,18,929	Surgical Oncology RR	C	ICU Ventilator	Tecme	Graphnet	91011161080	Meditronic	2Y	11-01-11	31/10/2013	PMSS Y-HLL	Working
767	13	SVIMS/SO. OT/11/2011/0676	IRS 11,18,929	Surgical Oncology RR	C	ICU Ventilator	Tecme	Graphnet	91011421080	Meditronic	2Y	11-01-11	31/10/2013	PMSS Y-HLL	Working
768	14	SVIMS/SO. OT/05/2009/0677		Surgical Oncology RR	C	ICU Ventilator	Siemens	Servo 300	22440	maquet	5Y	27-05-09	27-04-14	SVIMS	working
769	15	SVIMS/SO. OT/07/2016/0678		Surgical Oncology RR	C	Defibrillator	Mindray	BeneHeart D3	EL-65027001	Green Apple	5Y	18/07/2016	17/07/2021	SVIMS	Working
770	16	SVIMS/SO. OT/03/2009/0679	Euro 585	Surgical Oncology RR	NC	Syringe Pump	Fresenius	Injectomat/Agilia	20497454	Midi	5Y	19/03/09	18/03/14	SVIMS	Working
771	17	SVIMS/SO. OT/03/2009/0680	Euro 585	Surgical Oncology RR	NC	Syringe Pump	Fresenius	Injectomat/Agilia	20497433	Medi	5Y	19/03/09	18/03/14	SVIMS	Working
772	18	SVIMS/SO. OT/08/2009/0681	Euro 585	Surgical Oncology RR	NC	Syringe Pump	Fresenius	Injectomat/Agilia	20497426	Medi	5Y	19/03/09	18/03/14	SVIMS	Working
773	19	SVIMS/SO. OT/00/0000/1246		Surgical Oncology RR	NC	Syringe Pump	B Braun	Perfusor Compact	53702		1Y				
774	20	SVIMS/SO. OT/08/2013/0682		Surgical Oncology OT	NC	OT Table	Trident	7000SB-Dr.Mac	2A207-MS-0033	Bet Medical	2Y	27/08/13	26/08/15	PMSS Y-HLL	Working
775	21	SVIMS/SO. OT/08/2013/0683		Surgical Oncology OT	NC	OT Table	Trident	7000SB-Dr.Mac	2A207-MS-0035	Bet Medical	2Y	27/08/13	26/08/15	PMSS Y-HLL	Working
776	22	SVIMS/SO. OT/08/2013/0684		Surgical Oncology OT	NC	OT Table		Mechnical			1Y				Working
777	23	SVIMS/SO. OT/09/2012/0685		Surgical Oncology OT	NC	OT Table		Mechnical			1Y				Working
778	24	SVIMS/SO. OT/09/2012/0686		Surgical Oncology OT	NC	OT Light	Martin	V10 + V16	2088 , 2087	Vishal	5Y	21/09/12	20/09/17	Svims	Working
779	25	SVIMS/SO. OT/03/1993/0687		Surgical Oncology OT	NC	OT Light with Camera Recording	BenQ Medical Technology Corp. Taiwan	Trilite LS810-750	2E443-R3-0001	BET Medical	5 Y	23.04.2018	22.04.2023	SVIMS	Working

780	26	SVIMS/SO. OT/03/2000/0688		Surgical Oncology OT	NC	OT Light with Camera Recording	BenQ Medical Technology Corp. Taiwan	Trilite LS810-750	2E443-R3-0002	BET Medical	5 Y	23.04.2018	22.04.2023	SVIMS	Working
781	27	SVIMS/SO. OT/10/2008/0689			NC	OT Light	Drager	Solo500+700	ARXH-1237,ARXH-0240	Drager					Working
782	28	SVIMS/SO. OT/10/2008/0690		Surgical Oncology OT	NC	Surgical diathermy	Alsa	Excel 350	3618	Advanced Medical	3Y	10-03-08	10-02-11	Svims	Working
783	29	SVIMS/SO. OT/10/2008/0691		Surgical Oncology OT	NC	Surgical diathermy	Alsa	Excel 350	3622	Advanced Medical	3Y	10-03-08	10-02-11	Svims	Working
784	30	SVIMS/SO. OT/12/2010/0692		Surgical Oncology OT	NC	Harmonic Scalpel	J& J	Gen 04	Gn4108255	SG Surgical	3Y	21/12/2010	20/12/2013	SVIMS	Working
785	31	SVIMS/SO. OT/11/2014/0693		Surgical Oncology OT	NC	NasolarnyoScope	Olympus	ENF-T3	2425315	Olympus	1Y	18/11/2014	17/11/2015	Svims	Working
786	32	SVIMS/SO. OT/01/2016/0694		Surgical Oncology OT	NC	Vessal Sealing System	ERBE	ERBE VIO 300D	11405746	Colloq	5Y	29/01/2016	28/01/2021	Svims	Working
787	33	SVIMS/SO. OT/09/2011/0695		Surgical Oncology OT	NC	Drill System	Strykar	core	1108400353	Indian Ortho	5Y	09-02-11	09-01-16	SVIMS	Working
					NC	(Core Console -1108400353, Micro Drill-1033600443, Sagital Saw-1032603233, Oscillating Saw-1025800913, Reciprococating saw-1036401443 & Core Universal Driver-1034000733)								Svims	
788	34	SVIMS/SO. OT/06/2016/0696	RS 47 , 50, 000/-	Surgical Oncology OT	NC	**Laparascope System**	Strykar			Indian Orthocare	5Y	22/06/2016	21/06/2021	SVIMS	Working
		SVIMS/SO. OT/06/2016/0696A			NC	Camera Console, Model: 1288, Sl No:15HO14714									
		SVIMS/SO. OT/06/2016/0696B			NC	Camera Head, Model:1288HD, Sl No: 16Bo11282									
		SVIMS/SO. OT/06/2016/0696C			NC	26" Monitor, Model : Sl No: VPD265l0915									
		SVIMS/SO. OT/06/2016/0696D			NC	26" Monitor, Model : Sl No: VPD265l0915									
		SVIMS/SO. OT/06/2016/0696E			NC	Xenon Light Source, Model:X8000, Sl No:141028024									
		SVIMS/SO. OT/06/2016/0696F			NC	Insufflator , 20Litres, Sl No : 1602CE0749									
789	35	SVIMS/SO.OT/02/2010/0697	Rs 14, 90, 265/-	Surgical Oncology OT	NC	Mandipular Reconstruction Instruments with Drill	KLS Martin		119	Vishal	5Y			SVIMS	Working
790	36	SVIMS/SO.OT/08/2018/1134	1,36,800	Surgical Oncology OT	NC	ECG Machine	Wipro GE	MAC 2000	SRR18300068PA	Wipro GE	1 Y	28.08.2018	27.08.2019	SVIMS	
791	37	SVIMS/Suronc/11/2018/1136		Surgical Oncology	NC	Mechanical Thrombo Prophylaxis Device	Starmed Health	DVT 2600	1700919	Starmed Helath	18 mon	23.11.2018	23.05.2020	SVIMS	Working
792	38	SVIMS/Suronc/11/2018/1137		Surgical Oncology	NC	Mechanical Thrombo Prophylaxis Device	Starmed Health	DVT 2600	1700920	Starmed Helath	18 mon	23.11.2018	23.05.2020	SVIMS	Working
793	39	SVIMS/SO. OT/02/2019/1144	IRS 11,18,929	Surgical Oncology RR	C	ICU Ventilator	Tecme	Graphnet	190740261083 AIV	Schiller	5Y	02-12-19	02-11-24	SVIMS	Working
794	40	SVIMS/SO. OT/02/2019/1145	IRS 11,18,929	Surgical Oncology RR	C	ICU Ventilator	Tecme	Graphnet	190740271083 AIV	Schiller	5Y	02-12-19	02-11-24	SVIMS	Working

795	41	SVIMS/SurOnc/08/ 2019/1204		Surgical Oncology	NC	Infusion Pump	Mindray	Benefusion	SK9060 5760	Green Apple	5 Y	20.08.20 19	19.08.2024	SVIMS	Working
796	42	SVIMS/SurOnc/08/ 2019/1205		Surgical Oncology	NC	Infusion Pump	Mindray	Benefusion	SK9060 5762	Green Apple	5 Y	20.08.20 19	19.08.2024	SVIMS	Working
797	43	SVIMS/SurOnc/08/ 2019/1206		Surgical Oncology	NC	Infusion Pump	Mindray	Benefusion	SK9060 5759	Green Apple	5 Y	20.08.20 19	19.08.2024	SVIMS	Working
798	44	SVIMS/SurOnc/08/ 2019/1207		Surgical Oncology	NC	Infusion Pump	Mindray	Benefusion	SK9060 5754	Green Apple	5 Y	20.08.20 19	19.08.2024	SVIMS	Working
799	45	SVIMS/SurOnc/08/ 2019/1208		Surgical Oncology	NC	Infusion Pump	Mindray	Benefusion	SK9060 5745	Green Apple	5 Y	20.08.20 19	19.08.2024	SVIMS	Working
800	46	SVIMS/SurOnc/08/ 2019/1209		Surgical Oncology	NC	Infusion Pump	Mindray	Benefusion	SK9060 5750	Green Apple	5 Y	20.08.20 19	19.08.2024	SVIMS	Working
801	47	SVIMS/SurOnc/08/ 2019/1210		Surgical Oncology	NC	Infusion Pump	Mindray	Benefusion	SK9060 5749	Green Apple	5 Y	20.08.20 19	19.08.2024	SVIMS	Working
802	48	SVIMS/SurOnc/08/ 2019/1211		Surgical Oncology	NC	Infusion Pump	Mindray	Benefusion	SK9060 5747	Green Apple	5 Y	20.08.20 19	19.08.2024	SVIMS	Working
803	49	SVIMS/SurOnc/08/ 2019/1212		Surgical Oncology	NC	Infusion Pump	Mindray	Benefusion	SK9060 5746	Green Apple	5 Y	20.08.20 19	19.08.2024	SVIMS	Working
804	50	SVIMS/SurOnc/08/ 2019/1213		Surgical Oncology	NC	Infusion Pump	Mindray	Benefusion	SK9060 5753	Green Apple	5 Y	20.08.20 19	19.08.2024	SVIMS	Working
805	51	SVIMS/SurOnc/00/ 0000/1247		Surgical Oncology	NC	Syringe Pump	L & T	SP 102	609280		2y				
806	52	SVIMS/SurOnc/00/ 0000/1248		Surgical Oncology	NC	Syringe Pump	L & T	SP 102	609237						
807	53	SVIMS/SurOnc/00/ 0000/1249		Surgical Oncology	NC	Pulse Oximeter	MediAid	900P	EG09G001 67						
808	54	SVIMS/SurOnc/00/ 0000/1250		Surgical Oncology	NC	Pulse Oximeter	MediAid	900P	EG09G001 69						
809	55	SVIMS/SurOnc/00/ 0000/1251		Surgical Oncology	NC	Pulse Oximeter	MediAid	900P	EG09G001 90						
810	56	SVIMS/SurOnc/00/ 0000/1252		Surgical Oncology	NC	Mobile OT Ligt	Martin	MARLED	20862087						
811	57	SVIMS/SurOnc/01/ 2020/1277		Surgical Oncology		Syringe Pump	Smiths Medical	Grase by C9	18320 2976	M M Medical	5 Y	06.01.20 20	05.01.2025	SVIMS	
812	58	SVIMS/SurOnc/01/ 2020/1278		Surgical Oncology		Syringe Pump	Smiths Medical	Grase by C10	18320 2952	M M Medical	5 Y	06.01.20 20	05.01.2025	SVIMS	
813	59	SVIMS/SurOnc/01/ 2020/1279		Surgical Oncology		Syringe Pump	Smiths Medical	Grase by C11	18320 2802	M M Medical	5 Y	06.01.20 20	05.01.2025	SVIMS	
814	60	SVIMS/SurOnc/01/ 2020/1280		Surgical Oncology		Syringe Pump	Smiths Medical	Grase by C12	18320 2898	M M Medical	5 Y	06.01.20 20	05.01.2025	SVIMS	
815	61	SVIMS/SurOnc/01/ 2020/1281		Surgical Oncology		Syringe Pump	Smiths Medical	Grase by C13	18320 2806	M M Medical	5 Y	06.01.20 20	05.01.2025	SVIMS	
816	62	SVIMS/SurOnc/01/ 2020/1282		Surgical Oncology		Syringe Pump	Smiths Medical	Grase by C14	18320 2972	M M Medical	5 Y	06.01.20 20	05.01.2025	SVIMS	
817	63	SVIMS/SurOnc/01/ 2020/1283		Surgical Oncology		Syringe Pump	Smiths Medical	Grase by C15	18320 2927	M M Medical	5 Y	06.01.20 20	05.01.2025	SVIMS	
818	64	SVIMS/SurOnc/01/ 2020/1284		Surgical Oncology		Syringe Pump	Smiths Medical	Grase by C16	18320 2920	M M Medical	5 Y	06.01.20 20	05.01.2025	SVIMS	
819	65	SVIMS/SurOnc/01/ 2020/1285		Surgical Oncology		Syringe Pump	Smiths Medical	Grase by C17	18320 2942	M M Medical	5 Y	06.01.20 20	05.01.2025	SVIMS	
820	66	SVIMS/SurOnc/01/ 2020/1286		Surgical Oncology		Syringe Pump	Smiths Medical	Grase by C18	18320 2943	M M Medical	5 Y	06.01.20 20	05.01.2025	SVIMS	
821	67	SVIMS/SurOnc/01/		Surgical Oncology		Syringe Pump	Smiths	Grase by C19	18320 2901	M M	5 Y	06.01.20	05.01.2025	SVIMS	

		2020/1287					Medical			Medical		20			
822	68	SVIMS/SurOnc/01/ 2020/1288		Surgical Oncology		Syringe Pump	Smiths Medical	Grase by C20	18320 2957	M M Medical	5 Y	06.01.20 20	05.01.2025	SVIMS	
823	69	SVIMS/SurOnc/01/ 2020/1289		Surgical Oncology		Syringe Pump	Smiths Medical	Grase by C21	18320 2934	M M Medical	5 Y	06.01.20 20	05.01.2025	SVIMS	
824	70	SVIMS/SurOnc/01/ 2020/1290		Surgical Oncology		Syringe Pump	Smiths Medical	Grase by C22	18320 2801	M M Medical	5 Y	06.01.20 20	05.01.2025	SVIMS	
825	71	SVIMS/SurOnc/01/ 2020/1291		Surgical Oncology		Syringe Pump	Smiths Medical	Grase by C22	18320 2803	M M Medical	5 Y	06.01.20 20	05.01.2025	SVIMS	
826	1	SVIMS/MedOnc/02 /2010/0698	IRS 4,04,683	**Medical Oncology**	C	Multi Para Monitor	Mindray	Beneview T8	CF 99104013	Instromedic	2y	02-04-10	02-03-12	PMSS Y-HLL	Working
827	2	SVIMS/MedOnc/02 /2010/0699	IRS 4,04,683	Medical Oncology	C	Multi Para Monitor	Mindray	Beneview T8	CF 99103981	Instromedic	2y	02-04-10	02-03-12	PMSS Y-HLL	Working
828	3	SVIMS/MedOnc/02 /2010/0700	IRS 4,04,683	Medical Oncology	C	Multi Para Monitor	Mindray	Beneview T8	CF 99104637	Instromedic	2y	02-04-10	02-03-12	PMSS Y-HLL	Working
829	4	SVIMS/MedOnc/05 /2016/0701	IRS 4,04,683	Medical Oncology	C	Multi Para Monitor	Mindray	Beneview T8	CF 99104640	Instromedic	2y	02-04-10	02-03-12	PMSS Y-HLL	Working
830	5	SVIMS/MedOnc/02 /2014/0702	RS 2,30,000/-	Medical Oncology	C	Defibrillator	Mindray	BeneHeart D3	EL-65027003	Green Apple	2Y	19/07/20 16	18/07/2018	SVIMS	Working
831	6	SVIMS/MEdOnc/02 /2016/0704		Medical Oncology	NC	Pulse Oximeter	Assapin DiagNotic		123164 600025					SVIMS	Working
832	7	SVIMS/MEdOnc/02 /2016/0705		Medical Oncology	NC	Laminar Air Flow	Clean Air	CAV 900	095/07/151 6					SVIMS	Working
833	8	SVIMS/MEdOnc/02 /2016/0706		Medical Oncology	NC	Laminar Air Flow	Technico	4*2*2		Indian Scientific	1Y	26/05/20 17			Working
834	9	SVIMS/MEdOnc/02 /2016/0707		Medical Oncology	NC	Laminar Air Flow	Technico	4*2*3		Indian Scientific	1Y				Working
835	10	SVIMS/RadOnc/02/ 2010/0708		Medical Oncology	NC	Weighting Scale	Tulaman	EFS	1448522	Tulaman					Working
836	11	SVIMS/MedOnc/08 /2011/1102	IRS 11,18,929	Medical Oncology	C	ICU Ventilator	Tecme	Graphnet	09101124 1080 AIV	Meditronic	2Y	10-08-11	31/09/2013	PMSS Y-HLL	Working
837	12	SVIMS/MedOnc/08 /2011/1103	IRS 11,18,929	Medical Oncology	C	ICU Ventilator	Tecme	Graphnet	0912 1028 1080 AIV	Meditronic	2Y	10-08-11	31/09/2013	PMSS Y-HLL	Working
838	1	SVIMS/RadOnc/02/ 2010/0709	IRS 4,04,683	**Radiation Oncology**	**C**	Multi Para Monitor	Mindray	Beneview T8	CF9A1046 57	Instromedic	2y	02-04-10	02-03-12	PMSS Y-HLL	Working
839	2	SVIMS/RadOnc/02/ 2010/0710	IRS 4,04,683	Radiation Oncology	**C**	Multi Para Monitor	Mindray	Beneview T8	CF9A1046 44	Instromedic	2y	02-04-10	02-03-12	PMSS Y-HLL	Working
840	3	SVIMS/RadOnc/02/ 2010/0711	IRS 4,04,683	Radiation Oncology	**C**	Multi Para Monitor	Mindray	Beneview T8	CF9A1046 69	Instromedic	2y	02-04-10	02-03-12	PMSS Y-HLL	Working
841	4	SVIMS/RadOnc/02/ 2010/0712	IRS 4,04,683	Radiation Oncology RT2	**C**	Multi Para Monitor	Mindray	Beneview T8	CF9A1039 86	Instromedic	2y	02-04-10	02-03-12	PMSS Y-HLL	Working
842	5	SVIMS/RadOnc/02/ 2010/0713	IRS 4,04,683	Radiation Oncology RT2	**C**	Multi Para Monitor	Mindray	Beneview T8	CF9A1039 66	Instromedic	2y	02-04-10	02-03-12	PMSS Y-HLL	Working
843	6	SVIMS/RadOnc/07/ 2008/0714	IRS 4,23,79,500 /-	Radiation Oncology	C	**Linear Accelarator**	Electa	Precise		Electa India	3Y	31/07/20 09	30/07/2012	SVIMS	Working
844	7	SVIMS/RadOnc/10/ 2008/0715	IRS 1,11,19,835 /-	Radiation Oncology	C	**BrachyTherap hy & TPS**	Varian	H-640340		Varian India	5Y	23/10/20 08	22/10/2011	SVIMS	Working
845	8	SVIMS/RadOnc/04/ 2015/0716	IRS 15,00,30,69 8/-	Radiation Oncology	C	**Linear Accelarator**	Electa	Synery		Electa India	5Y	04-01-15	31/3/2020	SVIMS	Working

846	9	SVIMS/RadOnc/06/ 2014/0717	IRS 4,62,28,000 /-	Radiation Oncology	C	**CT Simulator**	Siemens	As Definition 20		Siemens India	5Y	30/06/20 14	29/06/2019	PMSS Y-HLL	Working
847	10	SVIMS/RadOnc/07/ 2016/0718	RS 27, 25, 000/-	Radiation Oncology	NC	Ultra Sound Color Doppler	Esote	MYLAB		Healthware	5y	27/07/20 16	26/07/2021	SVIMS	Working
848	11	SVIMS/RadOnc/06/ 2016/0719		Radiation Oncology	NC	Syringe Pump	Plenum Tech Pvt Ltd	Zion +	1422	Plenum Tech	3Y	15/06/20 16	14/06/2019	SVIMS	Working
849	12	SVIMS/RadOnc/06/ 2016/0720		Radiation Oncology	NC	Syringe Pump	Plenum Tech Pvt Ltd	Zion +	1383	Plenum Tech	3Y	15/06/20 16	14/06/2019	SVIMS	Working
850	13	SVIMS/RadOnc/06/ 2016/0721		Radiation Oncology	NC	Syringe Pump	Plenum Tech Pvt Ltd	Zion +	1388	Plenum Tech	3Y	15/06/20 16	14/06/2019	SVIMS	Working
851	14	SVIMS/RadOnc/06/ 2016/0722		Radiation Oncology	NC	Syringe Pump	Plenum Tech Pvt Ltd	Zion +	1386	Plenum Tech	3Y	15/06/20 16	14/06/2019	SVIMS	Working
852	15	SVIMS/RadOnc/06/ 2016/0723		Radiation Oncology	NC	Syringe Pump	Plenum Tech Pvt Ltd	Zion +	1394	Plenum Tech	3Y	15/06/20 16	14/06/2019	SVIMS	Working
853	16	SVIMS/RadOnc/06/ 2016/0724		Radiation Oncology	NC	Syringe Pump	Plenum Tech Pvt Ltd	Zion +	1425	Plenum Tech	3Y	15/06/20 16	14/06/2019	SVIMS	Working
854	17	SVIMS/RadOnc/02/ 2015/0725		Radiation Oncology	NC	Digital Weighing Scale	Tulaman	EFD	154959	Tulaman	1Y	16/02/20 15	15/02/2016	SVIMS	Working
855	18	SVIMS/Radonc/02/ 2013/0726		Radiation Oncology	C	Defibrillator	Mindray	BeneHeart D3	EL-6B029765	Green Apple	5Y	01-01-17	31/12/2021	SVIMS	Working
856	19	SVIMS/Radonc/02/ 2013/0727	IRS 24,500	Radiation Oncology	NC	Syringe Pump	Organge	Flow Prima	13050551-Z	Organge Medical	2Y	23/05/13	22/05/15	SVIMS	Working
857	20	SVIMS/Radonc/09/ 2010/0728	IRS 24,500	Radiation Oncology	NC	Syringe Pump	Organge	Flow Prima	13050552-Z	Organge Medical	2Y	23/05/13	22/05/15	SVIMS	Working
858	21	SVIMS/Ranonc/07/ 2018/1113	IRS 83,220	Radiation Oncology	NC	Ot Light		4Wing/Cluster	2796	Vijetha	1Y	14.07.20 18	13.07.2019	SVIMS	Working
859	22	SVIMS/Radonc/02/ 2012/1253		Radiation Oncology	NC	Pulse Oximeter	Mediaid	900P	E49G00181	Adv. Micronic	2Y	02-06-10	02-05-12	PMSS Y-HLL	Working
860	23	SVIMS/Radonc/11/ 2019/1274		Radiation Oncology	NC	Gamma Zone Monitor	Pulsecho Systems	NZM Zone Monitor	OZ 378	Pulsecho Systems	1Y	11-06-19	11-05-19	SVIMS	Working
861	1	SVIMS/GenSur/07/ 2010/0729	IRS 35,87,022	**General Surgery**	NC	Laproscope Set	Strykar	3Chip Hi Di		Indian ortho	3Y	20/09/20 10	19/09/2013	SVIMS	Working
862	2	SVIMS/GenSur/08/ 2010/0730	IRS 14,31,560	General Surgery	NC	Surgical Diathermy with Vessal Sealing Machine	Erbe	Vio300S	11398195	Forward Surgical	3Y	07-02-10	07-01-13	SVIMS	Working
863	3	SVIMS/GenSur/01/ 2009/0731	IRS 23,50,000	General Surgery	NC	Harmonic Scalpal	J & J	Gen 4	GN4105947	J & J	3Y	08-12-10	08-11-13	SVIMS	working
864	4	SVIMS/GenSUR/02 /2017/0732		General Surgery	NC	Surgical Diathermy	Alsa	Excel 350 MCDX	3677	Advanced	3Y	01-05-09	01-05-12	SVIMS	working
865	5	SVIMS/GenSUR/04 /1999/0733		General Surgery	C	Defibrillator	Mindray	BeneHeart D3	EL-6B029766	Green Apple	5Y	02-04-17	02-03-22	SVIMS	Working
866	6	SVIMS/GenSUR/01 /2019/1146		General Surgery	Nc	**OT Light**	Manomey	4 Wings/Clusters	3862	Vijetha	1Y	23/01/20 19	22/01/2019	SVIMS	Working
867	7	SVIMS/GenSUR/01 /2020/1292		General Surgery		**Syringe Pump**	Smiths Medical	Grase by C9	18320 2807	M M Medical	5 Y	06.01.20 20	05.01.2025	SVIMS	Working

868	8	SVIMS/GenSUR/01/2020/1293		General Surgery		**Syringe Pump**	Smiths Medical	Grase by C9	18320 2921	M M Medical	5 Y	06.01.2020	05.01.2025	SVIMS	Working
869	9	SVIMS/GenSUR/01/2020/1294		General Surgery		**Syringe Pump**	Smiths Medical	Grase by C9	18320 0249	M M Medical	5 Y	06.01.2020	05.01.2025	SVIMS	Working
870	10	SVIMS/GenSUR/01/2020/1295		General Surgery		**Syringe Pump**	Smiths Medical	Grase by C9	18320 0247	M M Medical	5 Y	06.01.2020	05.01.2025	SVIMS	Working
						Labarotory									
871	1	SVIMS/TraMed/06/2012/0735		BLOOD BANK	NC	Blood Bank Chamber	terumo	BBR 300L		Magna	1Y	06-09-12	06-08-13	SVIMS	Working
872	2	SVIMS/TraMed/00/2010/0736		BLOOD BANK	NC	Blood Bank Chamber	Remi			Remi	1Y	2010	2011	SVIMS	Working
873	3	SVIMS/TraMed/03/2009/0737		BLOOD BANK	NC	Blood Bank Chamber	Wheecon	Haemo Guard	5110814	Wheecon	1Y	25/03/2009	24/03/2010	SVIMS	Working
874	4	SVIMS/TraMed/06/2010/0738		BLOOD BANK	NC	Blood Bank Chamber	Wheecon	Haemo Guard	3310610	Wheecon	1Y	21/06/2010	20/06/2011	SVIMS	Working
875	5	SVIMS/TraMed/06/2010/0739		BLOOD BANK	NC	Blood Bank Chamber	Wheecon	Haemo Guard	230109	Wheecon	1Y	22/06/2010	20/06/2011	SVIMS	Working
876	6	SVIMS/TraMed/06/2010/0740		BLOOD BANK	NC	Blood Bank Chamber	Wheecon	Haemo Guard	2590609	Wheecon	1Y	22/06/2010	21/06/2011	SVIMS	Working
877	7	SVIMS/TraMed/07/2012/0741		BLOOD BANK	NC	B.Bank Refrigerator	Terumo Penpol	300L	1206763	Terumo Penplo	5Y	07-12-12	07-11-17	SVIMS	Working
878	8	SVIMS/TraMed/04/1999/0742		BLOOD BANK	NC	Deep Freezer	Forma Scientific	minus 86		Jagkumar & Co	3Y	29/04/99	28/04/2002	SVIMS	Working
879	9	SVIMS/TraMed/00/0000/0743		BLOOD BANK	NC	Deep Freezer	Terumo	DF-40U	903103		3Y			SVIMS	Working
880	10	SVIMS/TraMed/09/2014/0744		BLOOD BANK	NC	Cryofuge	ThermoFisher	Cryofuge 6000i	41625100	Terumo Penplo	5Y	15/09/2014	14/09/2019	SVIMS	Working
881	11	SVIMS/TraMed/07/2014/0745		BLOOD BANK	NC	Plattlet agitator	Terumo Penpol	PI400	1002022	Terumo Penplo	5y	24/7/2014	23/7/2019	SVIMS	Working
882	12	SVIMS/TraMed/00/0000/0746		BLOOD BANK	NC	Plattlet agitator	Terumo Penpol	P1200	1309721					SVIMS	Working
883	13	SVIMS/TraMed/00/0000/0747		BLOOD BANK	NC	Cryobath	Terumo Penpol	CB100	1103151					SVIMS	Working
884	14	SVIMS/TraMed/00/0000/0748		BLOOD BANK	NC	Automatic Component Extractor	Terumo Penpol	T-ACE-II	6628					SVIMS	Working
885	15	SVIMS/TraMed/00/0000/0749		BLOOD BANK	NC	Automatic Component Extractor	Terumo Penpol	T-ACE-II	11082					SVIMS	Working
886	16	SVIMS/TraMed/04/2012/0750		BLOOD BANK	NC	Laminor Air Flow	Technico			Technico	1Y	20/04/2012	19/04/2013	SVIMS	Working
887	17	SVIMS/TraMed/00/0000/0751		BLOOD BANK	NC	Automated Chemiilluminance Analyzer	J & J			Reagent Rental				SVIMS	Working
888	18	SVIMS/TraMed/02/2008/0752		BLOOD BANK	NC	Elisa Reader	Bio Tek		211716		3Y	02-08-08	02-07-11	SVIMS	**Working**
889	19	SVIMS/TraMed/00/0000/0753		BLOOD BANK	NC	Elisa Washer	Bio-Rad	PW40	EC1B407614					SVIMS	Working
890	20	SVIMS/TraMed/08/2002/0754		BLOOD BANK	NC	Automated cell separator	Fresenius	7A2T	1020	Wheecon	3y	24/08/02	23/08/05	SVIMS	Working
891	21	SVIMS/TraMed/00/0000/0755		BLOOD BANK	NC	Donor Coatch	HLL		12188	HLL	1Y	02-డిసెంబర్	02-డిసెంబర్	SVIMS	Working

892	22	SVIMS/TraMed/09/2009/0756		BLOOD BANK	NC	Cell Counter 5Diff	Mindray	BC5300		Golden	5Y	18/09/2009	17/09/2014	SVIMS	Working
893	23	SVIMS/TraMed/04/2001/0757		BLOOD BANK	NC	QBC Reader,Light	QBC	QBC		Godraj	1Y	04-01-01	31/3/2002	SVIMS	Working
894	24	SVIMS/TraMed/00/0000/0758		BLOOD BANK	NC	Source,Pra Lens		Fibre optic Cable						SVIMS	Working
895	25	SVIMS/TraMed/08/2014/0759		BLOOD BANK	NC	Central Monitor Sys.	Terumo Penpol	24channel	1407171	Terumo Penplo	5Y	21/08/2014	20/08/2019	SVIMS	Working
896	26	SVIMS/TraMed/00/0000/0760		BLOOD BANK	NC	Incubator	Yorko	YSI-438	712381					SVIMS	Working
897	27	SVIMS/TraMed/05/2012/0761		BLOOD BANK	NC	Serilogical water bath	Guna		1026	Indian Scientific	1Y	21/05/12	20/05/13	SVIMS	Working
898	28	SVIMS/TraMed/00/0000/0762		BLOOD BANK	NC	VDRL Shaker	Kemi		2165					SVIMS	Working
899	29	SVIMS/TraMed/00/0000/0763		BLOOD BANK	NC	Cooling Centrifuge	Remi	MC 24BL	5042					SVIMS	Working
900	30	SVIMS/TraMed/02/1993/0764		BLOOD BANK	NC	Centrifuge	Remi	R8C	330	Remi	3Y	26/02/93	25/02/96	SVIMS	Working
901	31	SVIMS/TraMed/00/0000/0765		BLOOD BANK	NC	MicroScope	Olympus	CH-201	8J14751					SVIMS	Working
902	32	SVIMS/Tra Med/00/0000/0766		BLOOD BANK	NC	Tube Sealer	Terumo	X51010	10021224					SVIMS	Working
903	33	SVIMS/TraMed/00/0000/0767		BLOOD BANK	NC	Tube Sealer-Portable	Terumo	LM100E	1302283					SVIMS	Working
904	34	SVIMS/TraMed/00/0000/0768		BLOOD BANK	NC	Tube Sealer-Portable	Terumo	LM 100	1105622					SVIMS	Working
905	35	SVIMS/TraMed/00/0000/0769		BLOOD BANK	NC	Blood Collection Monitor	Terumo	D-601	13081517					SVIMS	Working
906	36	SVIMS/TraMed/00/0000/0770		BLOOD BANK	NC	Blood Collection Monitor	Terumo	D-601						SVIMS	Working
907	37	SVIMS/TraMed/00/0000/0771		BLOOD BANK	NC	Blood Collection Monitor	Terumo	D-601	13091538					SVIMS	Working
908	38	SVIMS/TraMed/00/0000/0772		BLOOD BANK	NC	Blood Collection Monitor	Terumo	D-601	12101280					SVIMS	Working
909	39	SVIMS/TraMed/00/0000/0773		BLOOD BANK	NC	Blood Collection Monitor	Terumo	D-601	811322					SVIMS	Working
910	40	SVIMS/TraMed/00/0000/0774		BLOOD BANK	NC	Blood Collection Monitor	Terumo	D-250	1085					SVIMS	Working
911	41	SVIMS/TraMed/00/00		BLOOD BANK	NC	Donor Cough								SVIMS	Working
912	42	SVIMS/TraMed/00/0000/1098		BLOOD BANK	NC	Donor Cough									Working
913	43	SVIMS/TraMed/00/0000/0776		BLOOD BANK	NC	Donor Cough									Working
914	44	SVIMS/TraMed/00/0000/0777		BLOOD BANK	NC	Weighing Scale-Electronic	ESSEA		10906566					SVIMS	Working

915	45	SVIMS/TraMed/00/0000/0778		BLOOD BANK	NC	Weighing Scale-Electronic	ESSEA		FB-20805362					SVIMS	Working
916	46	SVIMS/TraMed/00/0000/0779		BLOOD BANK	NC	Electrophoresis	Chromous biotech		16c20x150					SVIMS	Working
917	47	SVIMS/TraMed/00/0000/0780		BLOOD BANK	NC	AutoClave	Equitron	PAD-7431PAD	JH 120					SVIMS	Working
918	48	SVIMS/TraMed/00/0000/0781		BLOOD BANK	NC	Hot Air Oven	Hitech							SVIMS	Working
919	49	SVIMS/TraMed/00/0000/0782		BLOOD BANK	NC	HemoCUe		HB 201	627013068					SVIMS	Working
920	50	SVIMS/TraMed/00/0000/0783		BLOOD BANK	NC	HemoCUe		HB 301	1540821102					SVIMS	Working
921	51	SVIMS/TraMed/00/0000/0784		BLOOD BANK	NC	HemoCUe		HB 301	1540821103					SVIMS	Working
922	52	SVIMS/TraMed/06/2017/0785	Rs 4,93,500/-	BLOOD BANK	NC	Blood Collection Monitor	Terumo	Trac Ii	2016-0-4224		5Y	16/06/2017	15/06/2022	SVIMS	Working
923	53	SVIMS/TraMed/05/2013/0786		BLOOD BANK - HLA Lab	NC	Microscope	Olympus	CKX41	5501336		1y	28/05/2013	27/05/2014	SVIMS	Working
924	54	SVIMS/TraMed/04/2012/0787		BLOOD BANK - HLA Lab	NC	Inverted Microscope	Olympus				1Y	21/4/2012	20/4/2013	SVIMS	Working
925	55	SVIMS/TraMed/04/2012/0788		BLOOD BANK - HLA Lab	NC	Serological Water Bath			8940D		1Y	21/4/2012	20/4/2013	SVIMS	Working
926	56	SVIMS/TraMed/04/2005/0789		BLOOD BANK - HLA Lab	NC	Hot Air Oven					1y	04-07-05	04-06-06	SVIMS	Working
927	57	SVIMS/TraMed/04/2012/0790		BLOOD BANK - HLA Lab	NC	Deep Freezer Minus 80	Terumo Penplol	Df 80U	1393019		5Y	21/04/2012	20/04/2017	SVIMS	**Working**
928	58	SVIMS/TraMed/04/2012/0791		BLOOD BANK - HLA Lab	NC	Laminor Air Flow	Technico				1Y	21/04/2012	20/04/2013	SVIMS	Working
929	59	SVIMS/TraMed/07/2012/0792		BLOOD BANK - HLA Lab	NC	Centrifuge	Remi	412LAG	BCBF-1324		1Y	26/07/2012	25/07/2013	SVIMS	Working
930	60	SVIMS/ra Med/02/2013/0793		BLOOD BANK - HLA Lab	NC	B lood Bank Chamber	Terumo Penplol	BBR300G	1206417		1Y	21/4/2012	20/4/2013	SVIMS	Working
931	61	SVIMS/TraMed/02/2013/0794		BLOOD BANK - HLA Lab	NC	BOD Incubator	Technico				1Y	20/04/23012	19/04/23013	SVIMS	Working
932	62	SVIMS/TraMed/00/0000/0795		BLOOD BANK - HLA Lab	NC	Centrifuge-Micro	Thermo Scientific	Micro C2	41456777					SVIMS	Working
933	63	SVIMS/TraMed/11/2012/1142		BLOOD BANK - HLA Lab	NC	Sterile Connecting Device	Terumo	TSD -II	1203023		1Y	11-11-12	11-10-13	SVIMS	Working
934	64	SVIMS/TraMEd/09/2019/1219		Blood Bank	NC	Automatic Component Extactor	Terumo Penpol	TACE II +	2018 08017	JIVA TECH Surg	5 y Agreement	17.09.2019	16.09.2024	Reagent Rental	Working
935	65	SVIMS/TraMEd/09/2019/1220		Blood Bank	NC	Blood Collection Monitor	Terumo Penpol	D - 601	2019 06165	JIVA TECH Surg	5 y Agreement	17.09.2019	16.09.2024	Reagent Rental	Working
936	66	SVIMS/TraMEd/09/2019/1221		Blood Bank	NC	Blood Collection Monitor	Terumo Penpol	D - 601	2019 06171	JIVA TECH Surg	5 y Agreement	17.09.2019	16.09.2024	Reagent Rental	Working
937	67	SVIMS/TraMEd/09/2019/1222		Blood Bank	NC	TUBE SEALER	Terumo Penpol	XS 1010	2019 045084	JIVA TECH Surg	5 y Agre	17.09.2019	16.09.2024	Reagent	Working

											emen t			Rental	
938	68	SVIMS/TraMEd/09/ 2019/1223		Blood Bank	NC	TUBE SEALER	Terumo Penpol	XS 1010	2019 45085	JIVA TECH Surg	5 y Agre emen t	17.09.20 19	16.09.2024	Reagen t Rental	Working
939	1	SVIMS/BioChe/04/ 2012/0796		Bio-Chemistry	NC	Auto Analyzer With Ro System	Beckman	Au 480	201801170 1	Beckman	NA	04-04-12	Reagent rental	Reagen t Rental	Working
940	2	SVIMS/BioChe/01/ 2016/0797		Bio-Chemistry	NC	Auto Analyzer	Beckman	AU680	1071019	Beckman	NA	01-06-16	Reagent rental	SVIMS	Working
941	3	SVIMS/BioChe/11/ 2018/1143		Bio-Chemistry	C	Auto Analyzer	Beckman	AU480	201804192 1	Beckman	NA	30/11/20 18	Reagent rental	SVIMS	Working
942	4	SVIMS/BioChe/09/ 2008/0798		Bio-Chemistry	NC	Analyzer Bio,ISE	Awarness Tech	CHEMWELL	2910-2243	CPC	5Y	09-06-08	09-05-13	SVIMS	Working
943	5	SVIMS/BioChe/01/ 2010/0799		Bio-Chemistry	NC	PCR	Oxygen Scientific	TC9600		Sri Vijaya	3y	23/01/10	22/01/13	SVIMS	Working
944	6	SVIMS/BioChe/04/ 2015/0800		Bio-Chemistry	NC	PCR	Eppendorf	6331	6331EH409 156	Eppendorf india	1Y	07-04-15	07-03-16	SVIMS	Working
945	7	SVIMS/BioChe/07/ 2015/0801		Bio-Chemistry	NC	Gel Documentation		alpha imager	511275	BioScreen	3Y	22/7/201 5	21/7/2018	SVIMS	Working
946	8	SVIMS/BioChe/04/ 2013/0802		Bio-Chemistry	NC	Spectro PhotoMeter	Sytronic	118	1807	Vijetha	1Y	04-03-13	04-02-14	SVIMS	Working
947	9	SVIMS/BioChe/04/ 2013/0803		Bio-Chemistry	NC	Spectro PhotoMeter	Sytronic	118	1809	Vijetha	1Y	04-03-13	04-02-14	SVIMS	Working
948	10	SVIMS/BioChe/10/ 2010/0804		Bio-Chemistry	NC	Spectro PhotoMeter-UV	Perkin Elmer	Lamda 25	501S10030 206	Perkin Elmer	1Y	25/10/20 10	24/10/2011	SVIMS	Working
949	11	SVIMS/BioChe/06/ 2014/0805		Bio-Chemistry	NC	Spectro PhotoMeter	Thermo Fisher	Spectronic 200E	8A3S00800 6	Thermo fisher	1Y	18/06/20 14	17/06/2015	SVIMS	Working
950	12	SVIMS/BioChe/01/ 2007/0807		Bio-Chemistry	NC	Semi Auto Analyzer	stat Fax	SF3300	3422	CPC	3Y	12-01-07	31/12/2008	SVIMS	Working
951	13	SVIMS/BioChe/10/ 2007/0808		Bio-Chemistry	NC	Semi Auto Analyzer	stat Fax	SF3300	3468	CPC	3Y	12-01-07	31/12/2008	SVIMS	Working
952	14	SVIMS/BioChe/05/ 2013/0809		Bio-Chemistry	NC	OsmoMeter	Gonotec	Osmomat 30D	130413	Wheecon	3Y	20/05/20 13	19/05/2014	SVIMS	Working
953	15	SVIMS/BioChe/03/ 2010/0810		Bio-Chemistry	NC	HPLC System	Shimadzu	prominence		Spinco	1y	03-03-10	03-02-11	SVIMS	Working
954	16	SVIMS/BioChe/00/ 0000/0811		Bio-Chemistry	C	ABG Analyzer	Radiometer	ABL 80	754R2513 N0006	Jk Medical		Reagent rental	Reagent rental	SVIMS	Working
955	17	SVIMS/BioChe/11/ 2015/0812		Bio-Chemistry	NC	Electrolyte Machine	SM Diagnostic	EX D5	IEA170291 547	SM Diagnostic	2Y	నవంబర్- 15	నవంబర్-17	SVIMS	Working
956	18	SVIMS/BioChe/11/ 2015/0813		Bio-Chemistry	NC	Electrolyte Machine	SM Diagnostic	EX D5	IEA190707 75	SM Diagnostic	2Y	నవంబర్- 15	నవంబర్-17	SVIMS	Working
957	19	SVIMS/BioChe/08/ 2014/0814		Bio-Chemistry	NC	Elisa Reader	Transasia	Erba lisa Scan	120719	Tranasia	1Y	21/8/14	20/8/15	SVIMS	Working
958	20	SVIMS/BioChe/08/ 2014/0815		Bio-Chemistry	NC	Elisa Washer	Transasia	Erba Lisa Wash	130822	Tranasia	1Y	21/8/14	20/8/15	SVIMS	Working
959	21	SVIMS/BioChe/01/ 2000/0816		Bio-Chemistry	NC	Electrophoresis system	Genei		41111		1Y	01-01-00	31/12/2001	SVIMS	Working
960	22	SVIMS/BioChe/09/ 2009/0817		Bio-Chemistry	NC	Deep frezzer -86	Forma scintific	minus 86, 902	817306769	Pinnacle	1Y	09-08-09	09-07-10	SVIMS	Working
961	23	SVIMS/BioChe/02/		Bio-Chemistry	NC	Deep Frezer -86	Eppendorf	Premium	F410DQ51	Eppendorf	5Y	04-02-15	04-01-20	SVIMS	Working

		2015/0818						U410	467	india					
962	24	SVIMS/BioChe/06/2013/0819		Bio-Chemistry	NC	Deep Freezer -40	Terumo penpol	Df 40U	1304307	Terumo	5Y	26/06/2013	25/06/2018	SVIMS	Working
963	25	SVIMS/BioChe/06/2013/0820		Bio-Chemistry	NC	Deep Freezer -40	Terumo penpol	Df 40U	1304308	Terumo	5Y	26/06/2013	25/06/2018	SVIMS	Working
964	26	SVIMS/BioChe/00/0000/0821		Bio-Chemistry	NC	Double Distilled Water	Bhanu Scientific							SVIMS	Working
965	27	SVIMS/BioChe/00/0000/0822		Bio-Chemistry	NC	Double Distilled Water	Bhanu Scientific	AQBDXL	6210904034					SVIMS	Working
966	28	SVIMS/BioChe/00/0000/0824		Bio-Chemistry	NC	Water Bath	Equitron	JC 273	8414		1Y			SVIMS	Working
967	29	SVIMS/BioChe/00/0000/0825		Bio-Chemistry	NC	Water Bath	Equitron		JE 037		1Y			SVIMS	Working
968	30	SVIMS/BioChe/00/0000/0826		Bio-Chemistry	NC	Water Bath	Equitron		JE 036		1Y			SVIMS	Working
969	31	SVIMS/BioChe/00/0000/0827		Bio-Chemistry	NC	Water Bath	Equitron		8414-JC-272		1Y			SVIMS	Working
970	32	SVIMS/BioChe/00/0000/0828		Bio-Chemistry	NC	Water Bath with Shaker	Remi	M RSB-12	GBC M 1070					SVIMS	Working
971	33	SVIMS/BioChe/12/2001/0829		Bio-Chemistry	NC	Ultrasonic cleaner	Bros scientific	Tec 25H	20		1y	12-09-01	12-08-02	SVIMS	Working
972	34	SVIMS/BioChe/06/2005/0830		Bio-Chemistry	NC	ColoriMeter	Elico	CL-157	5147		1Y	15/06/2005	14/06/2005	SVIMS	Working
973	35	SVIMS/BioChe/11/2015/0831		Bio-Chemistry	NC	Refrigerated Centrifuge	Remi	CM-12-Plus	ZBJO-27378	Remi	1Y	26/11/2015	25/11/2016	SVIMS	Working
974	36	SVIMS/BioChe/00/0000/0832		Bio-Chemistry	NC	Refrigerated Centrifuge	Remi	M-C24BL	5677	Remi	1Y			SVIMS	Working
975	37	SVIMS/BioChe/02/2007/0833		Bio-Chemistry	NC	Centrifuge	Remi	R8C	3585	Remi	1y	26/02/07	25/02/08	SVIMS	Working
976	38	SVIMS/BioChe/02/2007/0834		Bio-Chemistry	NC	Centrifuge	Remi	R8C	4120	Remi	1Y	26/02/07	25/02/08	SVIMS	Working
977	39	SVIMS/BioChe/02/2007/0835		Bio-Chemistry	NC	Centrifuge	Remi	R8C	5215	Remi	1y	26/02/07	25/02/08	SVIMS	Working
978	40	SVIMS/BioChe/02/2007/0836		Bio-Chemistry	NC	Centrifuge	Remi	R8C	5229	Remi	1y	26/02/07	25/02/08	SVIMS	Working
979	41	SVIMS/BioChe/02/2007/0837		Bio-Chemistry	NC	Centrifuge	Remi	R8C	LMLC 9672	Remi	1Y	26/02/07	25/02/08	SVIMS	Working
980	42	SVIMS/BioChe/02/2007/0838		Bio-Chemistry	NC	Centrifuge	Remi	R8C	LJLC-8463	Remi	1y	26/02/07	25/02/08	SVIMS	Working
981	43	SVIMS/BioChe/02/2007/0839		Bio-Chemistry	NC	Centrifuge	Remi	R8C	CDLL 3588	Remi	1y	26/02/07	25/02/08	SVIMS	Working
982	44	SVIMS/BioChe/02/2007/0840		Bio-Chemistry	NC	Centrifuge	Remi	R8C	BPLC-2763	Remi	1y	26/02/07	25/02/08	SVIMS	Working
983	45	SVIMS/BioChe/01/2000/0841		Bio-Chemistry	NC	Cyclo Mixer	Remi	CM 101	1238		1Y	01-01-00	31/12/2000	SVIMS	Working
984	46	SVIMS/BioChe/01/2000/0842		Bio-Chemistry	NC	Cyclo Mixer	Remi	CM 101	1244		1Y	01-01-00	31/12/2000	SVIMS	Working
985	47	SVIMS/BioChe/01/2000/0843		Bio-Chemistry	NC	Cyclo Mixer	Remi	LM 121	1245		1Y	01-01-00	31/12/2000	SVIMS	Working
986	48	SVIMS/BioChe/00/2006/0844		Bio-Chemistry	NC	Hot Air Sterilizer	Heco			Bros	1Y	2006	2007	SVIMS	Working
987	49	SVIMS/BioChe/00/2006/0845		Bio-Chemistry	NC	Hot Air Sterilizer	Heco			Bros	1Y	2006	2007	SVIMS	Working

988	50	SVIMS/BioChe/01/2000/0846		Bio-Chemistry	NC	Cyclo Mixer	Remi	CM 101	1242		1Y	01-01-00	01-01-01	SVIMS	Working
989	51	SVIMS/BioChe/01/2000/0847		Bio-Chemistry	NC	PH Meter	Elico	LI 127	AE-109		1Y	01-01-00	31/12/2000	SVIMS	Working
990	52	SVIMS/BioChe/01/2000/0848		Bio-Chemistry	NC	Balance - Eletronic	Shimadzu	AUX 120	D449514001		1Y	01-01-00	31/12/2000	SVIMS	Working
991	53	SVIMS/BioChe/01/2000/0849		Bio-Chemistry	NC	Balance - Eletronic	Satorius	AC2105-00AC	30102467		1Y	01-01-00	31/12/2000	SVIMS	Working
992	54	SVIMS/BioChe/07/2005/0850		Bio-Chemistry	NC	Autoclave Vertical	Equitron	AEJ-351	STWLAEG356		1Y	07-07-05	07-06-06	SVIMS	Working
993	55	SVIMS/BioChe/12/2001/0851		Bio-Chemistry	NC	Magnetic Stirrer	Remi	2MCH	1675		1Y	12-01-01	31/11/2002	SVIMS	Working
994	56	SVIMS/BioChe/12/2001/0852		Bio-Chemistry	NC	Hot Plate	Kemi	KHPR 25	3438		1Y	12-01-01	31/11/2002	SVIMS	Working
995	57	SVIMS/BioChe/12/2001/0853		Bio-Chemistry	NC	Hot Plate	Guna		3437		1Y	12-01-01	31/11/2002	SVIMS	Working
996	58	SVIMS/BioChe/12/2001/0854		Bio-Chemistry	NC	Shaker-Rotary	Remi	RS 12	976		1Y	12-01-01	31/11/2002	SVIMS	Working
997	59	SVIMS/BioChe/12/2001/0855		Bio-Chemistry	NC	Homoginizer	Remi	RQ 127	4562		1Y	12-01-01	31/11/2002	SVIMS	Working
998	60	SVIMS/BioChe/10/2016/0856		Bio-Chemistry	NC	Laminor Air Flow	Technico Lab.Product	Floor Stand Model		Bhavani	1Y	20/10/16	19/10/17	SVIMS	Working
999	61	SVIMS/BioChe/11/2016/0857		Bio-Chemistry	NC	Elisa Reader	Transasia	Erba lisa Scan	161027	Tranasia	1Y	30/11/16	29/11/17	SVIMS	Working
1000	62	SVIMS/BioChe/11/2016/0858		Bio-Chemistry	NC	Elisa Washerer	Transasia	Erba Lisa Wash	131334	Tranasia	1Y	30/11/16	29/11/17	SVIMS	Working
1001	63	SVIMS/BioChe/05/2017/0859	Rs 40,68,750/-	Bio-Chemistry	NC	Automated Elisa System		Euroimmun Analyzer -1P	6238000310	CPC	5Y	26/05/2017	25/05/2022	SVIMS	Working
1002	64	SVIMS/BioChe/05/2017/0860	Free	Bio-Chemistry	NC	Semi Auto Analyzer	stat Fax	SF3300	33008395	CPC	5Y	26/05/2017	25/05/2022	SVIMS	Working
1003	65	SVIMS/BioChe/06/2017/0861	Rs 83,000/-	Bio-Chemistry	NC	Flame PhotoMeter	Elico	CL-378	198/2532	Vijetha	1Y	29/06/2017	28/06/2018	SVIMS	Working
1004	66	SVIMS/BioChe/06/2017/0862	Rs 83,000/-	Bio-Chemistry	NC	Flame PhotoMeter	Elico	CL-378	198/2531	Vijetha	1Y	29/06/2017	28/06/2018	SVIMS	Working
1005	67	SVIMS/BioChe/09/2017/0863	Rs 22,690/-	Bio-Chemistry	NC	Centrifuge	Remi	R8C	ZDGN19650	Medicoy	1y	26/09/2017	25/09/2018	SVIMS	Working
1006	68	SVIMS/BioChe/09/2017/0864	Rs 22,690/-	Bio-Chemistry	NC	Centrifuge	Remi	R8C	ZDGN19655	Medicoy	1Y	26/09/2017	25/09/2018	SVIMS	Working
1007	69	SVIMS/BioChe/06/2017/0865	RS 1,36,855/-	Bio-Chemistry	NC	Trans UV Illuminator	Labomate	Bench Top	111146	Medicoy	1Y	13.06.17			Working
1008	70	SVIMS/BioChe/05/2017/0866	Rs 7,69,583/-	Bio-Chemistry	NC	Nanodrop	Eppendorf	D30	6133FO201420		1Y				Working
1009	71	SVIMS/BioChe/01/2017/0867		Bio-Chemistry	NC	Balance - Eletronic	Citizen	MP-300	303		1Y	08-01-17	31/07/2018		Working
1010	72	SVIMS/BioChe/01/2017/0868		Bio-Chemistry	NC	Balance - Eletronic	Citizen	MP-300	303		1Y	08-01-17	31/07/2018		Working
1011	73	SVIMS/Bioche/03/2015/0869		Bio-Chemistry	NC	Hot Air Oven	Kemi	KOMS2TD	15076		1Y	30/03/2015	30/03/2015		Working
1012	74	SVIMS/Bioche/06/2018/1131		Bio-Chemistry	NC	Immuno Assay Analyzer	Beckman	Access-2	570682	beckman india		19/06/2018	Reagent Rental		Working
1013	75	SVIMS/Bioche/02/2019/1148		Bio-Chemistry	NC	Centrifuge	REMI	R8C	ZEJN - 34908	Indian Scientific	1 Y	23.02.2019	22.02.2020	SVIMS	Working

1014	76	SVIMS/Bioche/03/2019/1151		Bio-Chemistry	NC	Auto clave	KEMI	KAUC.S5	2619	Medicoy Life	2 Y	28.03.2019	27.03.2021	SVIMS	Working
1015	77	SVIMS/Bioche/06/2019/1193		Bio-Chemistry	NC	Hot Plate	GUNA Entriprizes	M S Top	5011	Indian Scientific	1Y	20.06.2019		SVIMS	Working
1016	78	SVIMS/Bioche/06/2019/1194		Bio-Chemistry	NC	Hot Plate	GUNA Entriprizes	M S Top	5012	Indian Scientific	1Y	20.06.2019		SVIMS	Working
1017	79	SVIMS/Bioche/06/2019/1195		Bio-Chemistry	NC	Hot Plate	GUNA Entriprizes	M S Top	5013	Indian Scientific	1Y	20.06.2019		SVIMS	Working
1018	80	SVIMS/Bioche/06/2019/1196		Bio-Chemistry	NC	Hot Plate	GUNA Entriprizes	S S Top	5014	Indian Scientific	1Y	20.06.2019		SVIMS	Working
1019	81	SVIMS/Bioche/06/2019/1197		Bio-Chemistry	NC	Hot Plate	GUNA Entriprizes	S S Top	5015	Indian Scientific	1Y	20.06.2019		SVIMS	Working
1020	82	SVIMS/Bioche/06/2019/1198		Bio-Chemistry	NC	Hot Plate	GUNA Entriprizes	S S Top	5016	Indian Scientific	1Y	20.06.2019		SVIMS	Working
1021	83	SVIMS/Bioche/08/2019/1202		Bio-Chemistry	NC	Incubator	Equitron	7247DT-091	AIE - 003840 A	Indian Scientific	1Y	13.08.2019		SVIMS	Working
1022	84	SVIMS/Bioche/08/2019/1203		Bio-Chemistry	NC	Incubator	Equitron	7247DT-091	AIE - 003841 A	Indian Scientific	1Y	13.08.2019		SVIMS	Working
1023	1	SVIMS/Pathol/00/0000/0870		**CLINICAL PATHOLOGY**	**NC**	QBC machine(with centrifuge,light source&microscope)	QBC			Goderaj	5y	16/03/09	15/03/14	SVIMS	Working
						Lighjt Source		5353006	3500-3330264						
						Reader	BD	4406	2870038						
						MicroScope	Carl Zeiss	Student	45071						
1024	2	SVIMS/Pathol/00/2000/0871		CLINICAL PATHOLOGY	**NC**	Digital centrifuge	Remi motors	8RC	HbLL7834	Remimotors	1y	2000	2001	SVIMS	Working
1025	3	SVIMS/Pathol/00/2000/0872		CLINICAL PATHOLOGY	**NC**	Centrifuge	Remi motors	8RC	IELL4464	Remi motors	1Y	2000	2001	SVIMS	Working
1026	4	SVIMS/Pathol/09/2009/0873		CLINICAL PATHOLOGY	**NC**	Cell Counter 5Diff	Mindray	BC5300	RD-7B101690	Golden	5Y	17/09/2009	16/09/2014	SVIMS	Working
1027	5	SVIMS/Pathol/06/2011/0874		CLINICAL PATHOLOGY	**NC**	Cell counter 5Diff	Mindray	BC5300	RD 73101503	Golden	5Y	22/06/2011	22/06/2016	Reagent Rental	Working
1028	6	SVIMS/Pathol/00/2015/0875		CLINICAL PATHOLOGY	**NC**	Cell counter 3 Diff	Mindray	BC2800	RP41112713	Golden	1y	2015	2016	PMSSY-HLL	Working
1029	7	SVIMS/Pathol/09/2009/0876		CLINICAL PATHOLOGY	**NC**	Semi Auto Analyzer-Coag	Diagnostica stago	start 4	BT 38117772	surog	1y	16/09/2009	15/09/2010	SVIMS	Working
1030	8	SVIMS/Pathol/07/1995/0877		CLINICAL PATHOLOGY	**NC**	Centrifuge	Remi	R8CBL	GHLC-10574	Indian scintific	1Y	08-07-05		SVIMS	Working
1031	9	SVIMS/Pathol/05/2016/0878	RS 2,04,750/-	CLINICAL PATHOLOGY	**NC**	Semi Auto Analyzer-Coag		CA2000-4	440000065	Golden	1y	31/05/2016	30/05/2017	SVIMS	Working
1032	10	SVIMS/Pathol/00/2000/0879		CLINICAL PATHOLOGY	**NC**	Centrifuge	Remi motors	8RC	IELC-4464	Remi motors	1Y	2000	2001	SVIMS	Working
1033	11	SVIMS/Pathol/09/2016/0880		CLINICAL PATHOLOGY	**NC**	Centrifuge	Remi motors	RM- 12C	ZGFN-17814		1Y	21/09/2016	20/09/2017	SVIMS	Working
1034	12	SVIMS/Pathol/09/2016/0881		CLINICAL PATHOLOGY	**NC**	Centrifuge	Remi motors	RM- 12C	ZGFN-17815		1Y				Working
1035	13	SVIMS/Pathol/09/2016/0882		CLINICAL PATHOLOGY	**NC**	Centrifuge	Remi motors	RM- 12C	424280		1Y				Working

1036	14	SVIMS/Pathol/06/1995/0883		CLINICAL PATHOLOGY	**NC**	Hot Air Oven	Technico					16-06-05			Working
1037	15	SVIMS/Pathol/06/1995/0884		CLINICAL PATHOLOGY	**NC**	Incubator	Yorco					15-06-05			Working
1038	16	SVIMS/Patol/02/2004/0885		CLINICAL PATHOLOGY	**NC**	Serological Water Bath	Yorco	YSI-413	9430-703			16-06-05			Working
1039	17	SVIMS/Pathol/02/20004/0886		PATHOLOGY	NC	Cryostart	LEICA	CM 1510	2889	Lab India	3y	19/02/2004	18/02/2007	SVIMS	Working
1040	18	SVIMS/Pathol/07/2010/0887		PATHOLOGY	NC	Tissue processor	Micron	STP 120	46370	labcom	5Y	26/07/2010	25/07/2015	SVIMS	Working
1041	19	SVIMS/Pathol/02/1993/0888		PATHOLOGY	NC	Ultra centrifuge	Shandon	Cytospin_3	MA3119095	Indchem	3y	18/02/93	17/02/94	SVIMS	Working
1042	20	SVIMS/Pathol/00/1993/0890		PATHOLOGY	NC	Rotory Microtome	Leica lab India	Jung Multicut	4291966-	lab India	3y	1993	1994	SVIMS	Working
1043	21	SVIMS/Pathol/07/2010/0891		PATHOLOGY	NC	Rotory Microtome	Micron	HM 340E	46785	Labcon	5Y	26/07/2010	25/07/2011	SVIMS	Working
1044	22	SVIMS/Pathol/02/1993/0892		PATHOLOGY	NC	Incubator	Yarco	ysi-438	95Ao889	Lazer Instrument	3y	18/02/93	17/02/94	SVIMS	Working
1045	23	SVIMS/Pathol/02/1993/0893		PATHOLOGY	NC	Water bath	Yarco	Ysi-133	OBH546	Lazer Instrument	3y	18/02/93	17/02/94	SVIMS	Working
1046	24	SVIMS/Pathol/08/2015/0894		PATHOLOGY	NC	Balance	shimadzu	BL-220H	D432908202	Yarco	1Y	08-10-15	08-09-16	SVIMS	Working
1047	25	SVIMS/Pathol/02/1993/0895		PATHOLOGY	NC	Microscope	Olympus	KIC 26631		Hospin surgical	3y	18/02/93	17/02/96	SVIMS	Working
1048	26	SVIMS/Pathol/12/1993/0896		PATHOLOGY	NC	Declcifier	Yarco			Laser	3y	18/02/93	17/02/96	SVIMS	Working
1049	27	SVIMS/Pathol/12/1994/0897		PATHOLOGY	NC	Immuno fluro.Microscope	Carl Zeiss	Axioscope	451485	Carl Zeiss toshniwal	3y	12-03-94	12-02-97	SVIMS	Working
1050	28	SVIMS/Pathol/12/1994/0898		PATHOLOGY	NC	Immuno fluro.Microscope	Carl Zeiss	Axioscope		Carl Zeiss toshniwal	3y	12-03-94	12-02-97	SVIMS	Working
1051	29	SVIMS/Pathol/04/1995/0899		PATHOLOGY	NC	Incubator	Yorco	Ysi-438	07C-4090	Yarco laser instument	3y	27/04/95	26/04/98	SVIMS	Working
1052	30	SVIMS/Pathol/00/1993/0900		PATHOLOGY	NC	Microscope	Nichon	UFX-DX			3y	1993	1994	SVIMS	Working
1053	31	SVIMS/Pathol/00/1993/0901		PATHOLOGY	NC	Microscope	Nichon	Labophot			3y	1993	1994	SVIMS	Working
1054	32	SVIMS/Pathol/11/2014/0902		PATHOLOGY	NC	Microscope	Nikon	E-200	610705	Towa Optics	1Y	14/11/2014	13/11/2015	SVIMS	Working
1055	33	SVIMS/Pathol/11/2014/0903		PATHOLOGY	NC	Microscope	Nikon	E-200	610716	Towa Optics	1Y	14/11/2014	13/11/2015	SVIMS	Working
1056	34	SVIMS/Pathol/02/2014/0904		PATHOLOGY	NC	Microscope	Nikon	E-200	209499	Towa Optics	1Y	13/02/2014	02-12-15	SVIMS	Working
1057	35	SVIMS/Pathol/02/2014/0905		PATHOLOGY	NC	Microscope	Nikon	E-200	209498	Towa Optics	1Y	13/02/2014	02-12-15	SVIMS	Working
1058	36	SVIMS/Pathol/02/2014/0906		PATHOLOGY	NC	Microscope	Nikon	E-201	209496	Towa Optics	1Y	13/02/2014	02-12-15	SVIMS	Working
1059	37	SVIMS/Pathol/12/2008/0907		PATHOLOGY	NC	Microscope	Olympus	CH20I	8L08931		1Y	12-09-08	12-08-09	SVIMS	Working
1060	38	SVIMS/Pathol/12/2008/0908		PATHOLOGY	NC	Microscope	Olympus	CH20I	8L08930		1Y	12-09-08	12-08-09	SVIMS	Working
1061	39	SVIMS/Pathol/12/2008/0909		PATHOLOGY	NC	Microscope	Olympus	CH20I	8L08924		1Y	12-09-08	12-08-09	SVIMS	Working

1062	40	SVIMS/Pathol/12/2008/0910		PATHOLOGY	NC	Microscope	Olympus	CH20I	8L08936		1Y	12-09-08	12-08-09	SVIMS	Working
1063	41	SVIMS/Pathol/12/2008/0911		PATHOLOGY	NC	Microscope	Olympus	CH20I	8K15613		1Y	12-09-08	12-08-09	SVIMS	Working
1064	42	SVIMS/Pathol/03/2009/0912		PATHOLOGY	NC	Microscope	Olympus	CH20I	9A02350		1Y	30/03/09	29/03/10	SVIMS	Working
1065	43	SVIMS/Pathol/03/2009/0913		PATHOLOGY	NC	Microscope	Olympus	CH20I	9A02349		1Y	30/03/09	29/03/10	SVIMS	Working
1066	44	SVIMS/Pathol/03/2009/0914		PATHOLOGY	NC	Microscope	Olympus	CH20I	9A02346		1Y	30/03/09	29/03/10	SVIMS	Working
1067	45	SVIMS/Pathol/03/2009/0915		PATHOLOGY	NC	Microscope	Olympus	CH20I	9B07580		1Y	30/03/09	29/03/10	SVIMS	Working
1068	46	SVIMS/Pathol/03/2009/0916		PATHOLOGY	NC	Microscope	Olympus	CH20I	9B07588		1Y	30/03/09	29/03/10	SVIMS	Working
1069	47	SVIMS/Pathol/03/2015/0918		PATHOLOGY	NC	PentaHead MicroScope	Olympus	BX-53F	4B43145	Dss Imagetech	5Y	16/09/2014	15/09/2019	SVIMS	Working
1070	48	SVIMS/Pathol/03/2015/0919		PATHOLOGY	NC	Microscope	Olympus	CH-20I	14E0604	Indian scintific	1Y	18/03/15	17/03/16	SVIMS	Working
1071	49	SVIMS/Pathol/03/2015/0920		PATHOLOGY	NC	Microscope	Olympus	CH-20I	14F0409	Indian scintific	1Y	18/03/15	17/03/16	SVIMS	Working
1072	50	SVIMS/Pathol/03/2015/0921		PATHOLOGY	NC	Microscope	Olympus	CH-20I	14F0397	Indian scintific	1Y	18/03/15	17/03/16	SVIMS	Working
1073	51	SVIMS/Pathol/03/2015/0922		PATHOLOGY	NC	Microscope	Olympus	CH-20I	15C0466	Indian scintific	1Y	18/03/15	17/03/16	SVIMS	Working
1074	52	SVIMS/Pathol/03/2015/0923		PATHOLOGY	NC	Microscope	Olympus	CH-20I	15C0470	Indian scintific	1Y	18/03/15	17/03/16	SVIMS	Working
1075	53	SVIMS/Pathol/03/2015/0924		PATHOLOGY	NC	Microscope	Olympus	CH-20I	15C0476	Indian scintific	1Y	18/03/15	17/03/16	SVIMS	Working
1076	54	SVIMS/Pathol/04/2016/0925		PATHOLOGY	NC	Flow cyto meter, Work station and UPS online	Beckman	FC500	AU30311	Beckman India	5Y	14.03.2013	13.03.2018	SVIMS	Working
1077	55	SVIMS/Pathol/04/2016/0926		PATHOLOGY	NC	Hot Air Oven	Navyog	NU-107	1895F			26/04/2016			Working
1078	56	SVIMS/Pathol/03/1995/0927		PATHOLOGY	NC	Hot Air Oven	Navyog	NU-107	1894F			26/04/2016			Working
1079	57	SVIMS/Pathol/05/2014/0928		PATHOLOGY	NC	Centrifuge	Remi	R8C	FKLL9320			1995			Working
1080	58	SVIMS/Pathol/04/1993/0929		PATHOLOGY	NC	Water Bath	Guna					14/05/2014			Working
1081	59	SVIMS/Pathol/10/2012/0930		PATHOLOGY	NC	Balance-Digital	ESSAe	D5-262	G25207131166						Working
1082	60	SVIMS/Pathol/04/2018/1105		PATHOLOGY	C	Cryostat with UV	Leica	Leica CM 1860	3290	Indian Scientific	5 Y	12.04.2018	11.04.2023	SVIMS	Working
1083	61	SVIMS/Pathol/02/2019/1149		PATHOLOGY	NC	Centrifuge	REMI	R8C	ZEKN - 37123	Indian Scientific	1 Y	27.02.2019	26.02.2020	SVIMS	Working
1084	62	SVIMS/Pathol/08/2020/1336		PATHOLOGY		Micro Tome	Leica India	Histo Core Multicut	00538/082019	Green Apple	3 y	24.08.2020	23.08.2023	SVIMS	Working
1085	1	SVIMS/MicBio/10/2012/0931		**Micro Biology**	NC	Analytical Balance	Wensar	PGB3000	18947	Indiab Scien	1Y	18.10.2012	17.10.2013	SVIMS	Working
1086	2	SVIMS/MicBio/06/2010/0932		Micro Biology	NC	Automated Blood Culture System 3D 30 Bac 'T'Alert	Biomerieux	Do ICR 3420	002IR 7786	Biomerieux India	2Y	14.06.2010	13.06.2012	SVIMS	Working

1087	3	SVIMS/MicBio/02/ 1993/0933		Micro Biology	NC	Balance Chemical	New Orintal	NOR/7			1Y	24.02.19 93	23.02.1994	SVIMS	Working
1088	4	SVIMS/MicBio/03/ 2001/0934		Micro Biology	NC	Balance Chemical	Keroy		22391		1Y	02.03.20 01	01.03.2002	SVIMS	Working
1089	5	SVIMS/MicBio/08/ 2009/0935		Micro Biology	NC	Bod Incubator	IN LABs	10 CFT			1Y	22.08.20 09	21.08.2010	SVIMS	Working
1090	6	SVIMS/MicBio/04/ 2007/0936		Micro Biology	NC	Bod Incubator with Stabilizer (875x570x570)	Kemi	105	KB 00-105378		1Y	21.04.20 07	20.04.2008	SVIMS	Working
1091	7	SVIMS/MicBio/00/ 1993/0937		Micro Biology	NC	Bio Safety Cabinet	Yarco		YSI 1490		1Y	1993	1994	SVIMS	Working
1092	8	SVIMS/MicBio/11/ 2011/0938		Micro Biology	NC	Bio Safety Cabinet 4x2x2 Class 11 B2				Technico	1Y	28.07.20 11	27.07.2012	SVIMS	Working
1093	9	SVIMS/MicBio/07/ 2011/0939		Micro Biology	NC	Bio Safety Cabinet 4x2x2 Class 11 B2				Technico	1Y	17.11.20 11	16.11.2012	SVIMS	Working
1094	10	SVIMS/MicBio/02/ 1993/0940		Micro Biology	NC	Centrifuge R 8C	Remi	R8C	ABLC 066		1Y	24.02.19 93	23.02.1994	SVIMS	Working
1095	11	SVIMS/MicBio/12/ 2004/0941		Micro Biology	NC	Centrifuge R 8C	Remi	R8C	JMCC 8306		1Y	22.12.20 04	2-1.12.2005	SVIMS	Working
1096	12	SVIMS/MicBio/12/ 2010/0942		Micro Biology	NC	Centrifuge RM 12C	Remi	RM12C	KDLC 12700		1Y	08.12.20 10	07.12.2011	SVIMS	Working
1097	13	SVIMS/MicBio/08/ 2012/0943		Micro Biology	NC	Centrifuge R 90 swing out head Glass Lid	Remi	R8CBL	FFLC-7202		1Y	31.08.20 12	30.08.2013	SVIMS	Working
1098	14	SVIMS/MicBio/03/ 2013/0944		Micro Biology	NC	Centrifuge RM 12 C (micro) RM 1215/1217	Remi	RM12 C	1029		1Y	30.03.20 13	29.03.2014	SVIMS	Working
1099	15	SVIMS/MicBio/05/ 2005/0945		Micro Biology	NC	Colony counter	Yarco		03K0552		1Y	31.05.20 05	30.05.2006	SVIMS	Working
1100	16	SVIMS/MicBio/01/ 2011/0946		Micro Biology	NC	Cyclomixer	Remi	CM101	BNCM-42		1Y			SVIMS	Working
1101	17	SVIMS/MicBio/01/ 2011/0947		Micro Biology	NC	Cyclomixer Vertex	Remi	CM101	CDCM 466		1Y	06.01.20 11	05.01.2012	SVIMS	Working
1102	18	SVIMS/MicBio/10/ 2012/0948		Micro Biology	NC	Distilled water plant + water level cutoff sys Steel	Kemi	KWS-3	3095		1Y	05.10.20 12	04.10.2013	SVIMS	Working
1103	19	SVIMS/MicBio/07/ 2013/0949		Micro Biology	NC	Deep freezer -40Ç	Thermo penpal	DF 40U	1304310	Rs 4,04,250	5Y	04.07.20 13	03.07.2018	SVIMS	Working
1104	20	SVIMS/MicBio/01/ 2014/0950		Micro Biology	NC	Double distilled water palnt	Bhanu Scientific	AQDD-20PDB/XL	WS-Q-20114		1Y	02.01.20 14	01.01.2015	SVIMS	Working
1105	21	SVIMS/MicBio/01/ 2014/0951		Micro Biology	NC	Water Stills dis.d water plant	Bhanu Scientific	Edu still single	AQDD201 14		1Y	02.01.20 14	01.01.2015	SVIMS	Working
1106	22	SVIMS/MicBio/03/ 2001/0952		Micro Biology	NC	Electronic Precision balance	Afcoset	FX300	2201007		1Y	31.03.20 01	30.03.2002	SVIMS	Working
1107	23	SVIMS/MicBio/12/ 2004/0953		Micro Biology	NC	Electronic Weighing balance digital	ESSAE	DS-252	G25204536 58		1Y	03.12.20 04	02.12.2005	SVIMS	Working
1108	24	SVIMS/MicBio/07/ 2009/0954		Micro Biology	NC	Electronic Analytical	Shimdzu		AUX 120		1Y	28.07.20 09	27.07.2010	SVIMS	Working

						balance									
1109	25	SVIMS/MicBio/05/2012/0955		Micro Biology	NC	Electronic Balance	Shimdzu	BL 2020H	D455007128		1Y	24.05.2012	23.05.2013	SVIMS	Working
1110	26	SVIMS/MicBio/02/2012/0956		Micro Biology	NC	Elisa Reader.Washer, PC., Printer and UPS	Tecan Sanrice	Sunraise, HydroFlex	1108003346, 1108003304		5Y	14.02.2012	13.02.2017	SVIMS	Working
1111	27	SVIMS/MicBio/00/1999/0957		Micro Biology	NC	Hot plate	Guna		1241		1Y	1999	2000	SVIMS	
1112	28	SVIMS/MicBio/06/2015/0958		Micro Biology	NC	Hot Plate (Rectangular)	Riviera	HPRE/14-7-141200	500211218			13.06.2015	12.06.2016	SVIMS	Working
1113	29	SVIMS/MicBio/04/2007/0959		Micro Biology	NC	Hot air Oven	Kemi		8776			21.04.2007	20.04.2008	SVIMS	Working
1114	30	SVIMS/MicBio/01/2011/0960		Micro Biology	NC	Hot Air oven Digital 600x600x900	Kemi	KDMS6PD	11624			18.01.2011	17.01.2012	SVIMS	Working
1115	31	SVIMS/MicBio/00/1995/0961		Micro Biology	NC	Incubator Portable	Yarco		83H0702YS1438			1995	1996	SVIMS	Working
1116	32	SVIMS/MicBio/00/1999/0962		Micro Biology	NC	Incubator Small	Yarco	YSI-438	94C794			1999	2000	SVIMS	Working
1117	33	SVIMS/MicBio/04/2007/0963		Micro Biology	NC	Incubator Digial 600x600x600	Kemi	S5FD	8777			21.04.2007	201.04.2008	SVIMS	Working
1118	34	SVIMS/MicBio/01/2011/0964		Micro Biology	NC	Incubator Bact.600x600x600	Kemi	KIS-5FD	11625			18.01.2011	17.01.2012	SVIMS	Working
1119	35	SVIMS/MicBio/07/2013/0965		Micro Biology	NC	Insipissator	Grant Germany	T-100IN	1240007			02.07.2013	01.07.2014	SVIMS	Working
1120	36	SVIMS/MicBio/00/1993/0966		Micro Biology	NC	Laminar Air Flow 2x4	Yorco					1993	1994	SVIMS	Working
1121	37	SVIMS/MicBio/00/1997/0967		Micro Biology	NC	Laminar Air Flow 2x2	Yorco	YSI-188	76K0999			1997	1998	SVIMS	Working
1122	38	SVIMS/MicBio/11/2011/0968		Micro Biology	NC	Laminar Air Flow 6x2x2 Chamber	Technico					17.11.2011	16.11.2012	SVIMS	Working
1123	39	SVIMS/MicBio/11/2004/0969		Micro Biology	NC	Magnetic Stirrer	Eltek		MS203			19.11.2004	19811.2005	SVIMS	Working
1124	40	SVIMS/MicBio/11/2012/0970		Micro Biology	NC	Microscope with phase contrast dark Field with camera	Carl Ziess	AxioScope 50	451485			21.11.2012	20.11.2013	SVIMS	Working
1125	41	SVIMS/MicBio/11/2012/0971		Micro Biology	NC	Microscope Research	Carl Ziess	AxioScope 50	451485			21.11.2012	20.11.2013	SVIMS	Working
1126	42	SVIMS/MicBio/00/1997/0972		Micro Biology	NC	Microscope Student	Carl Ziess	AxioScope 50	467085			1997	1998	SVIMS	Working
1127	43	SVIMS/MicBio/05/2004/0973		Micro Biology	NC	Microscope GB Monocular	Olympus					22.05.2004	21.05.2005	SVIMS	working
1128	44	SVIMS/MicBio/05/2004/0974		Micro Biology	NC	Microscope GB Monocular	Olympus					27.05.2004	26.05.2005	SVIMS	Working
1129	45	SVIMS/MicBio/00/0000/0975		Micro Biology	NC	Microscopes Primostar	Carl Zeiss	PRIMoSTAR	3116022383					SVIMS	Working

1130	46	SVIMS/MicBio/10/2012/0976		Micro Biology	NC	Microscopes Primostar	Carl Zeiss	PRIMoSTAR	3116022387					SVIMS	Working
1131	47	SVIMS/MicBio/06/2010/0977		Micro Biology	NC	Microscopes Primostar	Carl Zeiss	PRIMoSTAR	3116022388					SVIMS	Working
1132	48	SVIMS/MicBio/10/2012/0978		Micro Biology	NC	Microscopes Primostar	Carl Zeiss	PRIMoSTAR	3116022389					SVIMS	Working
1133	49	SVIMS/MicBio/06/2010/0979		Micro Biology	NC	Microscopes Primostar	Carl Zeiss	PRIMoSTAR	3116022391					SVIMS	Working
1134	50	SVIMS/MicBio/03/2013/0980		Micro Biology	NC	Micro MGIT Fluorescence reader		BDBBLMGIT				05.03.2013	04.03.2014	SVIMS	Working
1135	51	SVIMS/MicBio/06/2012/0981		Micro Biology	NC	Orbital shaker	Rivotek	50031003	2012012			18.06.2012	17.06.2013	SVIMS	Working
1136	52	SVIMS/MicBio/00/1993/0982		Micro Biology	NC	PH Meter-361	Systronics		423			1993	1994	SVIMS	Working
1137	53	SVIMS/MicBio/12/2004/0983		Micro Biology	NC	PH Meter Digital	Systronics		2686			03.12.2004	02.12.2005	SVIMS	Working
1138	54	SVIMS/MicBio/10/2012/0984		Micro Biology	NC	Real time PCR system	M/s. Indus	Rotor Gene Q 5Plex	R0911136			30.10.2012	29.10.2013	SVIMS	Working
1139	55	SVIMS/MicBio/01/2012/0985		Micro Biology	NC	PCR work station	Genei		10/2011/F/0185			11.01.2012	10.01.2013	SVIMS	Working
1140	56	SVIMS/MicBio/05/2005/0986		Micro Biology	NC	Serological Water both with Shaker	Yarco		450101			31.05.2005	30.05.2006	SVIMS	Working
1141	57	SVIMS/MicBio/01/2011/0987		Micro Biology	NC	Ultra Sonicator	Rivotek	2160	17000008			18.01.2011	17.01.2012	SVIMS	Working
1142	58	SVIMS/MicBio/07/2004/0988		Micro Biology	NC	VDRL Rotator	Remi	EYCM629	5704			23.07.2004	22.07.2005	SVIMS	Working
1143	59	SVIMS/MicBio/11/2012/0989		Micro Biology	NC	Vortex Mixer	Riviera		2013094			14.11.2012	13.11.2013	SVIMS	Working
1144	60	SVIMS/MicBio/02/2016/0990		Micro Biology	NC	Micro Centrifuge	Thermo Fisher	sorvall st16	41884263	genesis		18/02/2016	17/02/2017	SVIMS	Working
1145	61	SVIMS/MicBio/10/2016/0991		Micro Biology	NC	Laminor Air Flow	Technico Lab.Product	Floor Stand Model		Bhavani	1Y	20/10/16	19/10/17	SVIMS	Working
1146	62	SVIMS/MicBio/05/2017/0992	RS 3,16,547/-	Micro Biology	NC	Centrifuge	Thermo Fisher	Legend Micro 21R	42091355	genesis	5Y	17/05/2017	16/05/2022	SVIMS	Working
1147	63	SVIMS/MicBio/07/2014/0993		Micro Biology	NC	Serological Water Bath	Technico	2064-1	TLPPL109		1Y	23/07/2014	22/07/2015	SVIMS	Working
1148	64	SVIMS/MicBio/07/2014/0994		Micro Biology	NC	Serological Water Bath	Technico	2064-1	NA		1Y	23/07/2014	22/07/2015	SVIMS	Working
1149	65	SVIMS/MicBio/07/2014/0995		Micro Biology	NC	Centrifuge	Remi	R8CBL	9939		1Y			SVIMS	Working
1150	66	SVIMS/Virolo/03/2018/0996		Micro Biology	NC	Elisa Washer	BioRad	PW-40	EC7E716006			13-03-18		SVIMS	Working
1151	67	SVIMS/Micbio/08/2018/1150		Micro Biology	NC	Elisa Microplate Reader	Erba Trans Asia	Lisa Scan EM	80525	Sai Pavitra	2 Y	06.08.2018	05.08.2020	SVIMS	Working
1152	68	SVIMS/Micbio/04/2019/1152		Micro Biology	NC	Auto clave	Kadavil Electro	KAVC.S5.OP	2584	Medicoy Life	2 Y	09.04.2019	08.04.2021	SVIMS	Working
1153	69	SVIMS/Micbio/04/2019/1153		Micro Biology	NC	Auto clave	Kadavil Electro	KAVC.S5.OP	2585	Medicoy Life	2 Y	09.04.2019	08.04.2021		

1154	70	SVIMS/Micbio/01/2016/1166		Micro Biology	NC	Centrifuse Swing out heads (R-90)	REMI	R 8C - BL	ZBKN - 30586			20.01.2016			
1155	71	SVIMS/Micbio/07/2014/1167		Micro Biology	NC	Centrifuse Swing out heads (R-90)	REMI	R 8C - BL	30855			23.07.2014			
1156	72	SVIMS/Micbio/11/2017/1168		Micro Biology	NC	Heating block assay	Revotec	50031001	HB/385	Indian Scientific		02.11.2017			
1157	73	SVIMS/Micbio/05/2005/1169		Micro Biology	NC	Blot Shaket (Shaking tray for Dr. 100m)	Mitra Industrial		43284			31.05.2005			
1158	74	SVIMS/Micbio/04/2019/1199		Micro Biology	NC	40 deg C Freezer	LARK Innovative	DW-FL 531		LARK Innovative	5 Y	16.04.2019			
1159	1	SVIMS/Virolo/04/2015/0997		**Virology Lab**	NC	Semi Micro balance	Shindzu	AUW220D	D450022353	Shindzu	1 Y	24.03.2015	23.03.2016	SVIMS	Working
1160	2	SVIMS/Virolo/03/2015/0998		Virology Lab	NC	Refrigerated Centrifuge	Eppendrof	5424R	5404E6217380	Eppendrof	1 Y	01.04.2015	31.03.2016	SVIMS	Working
1161	3	SVIMS/Virolo/04/2015/0999		Virology Lab	NC	Laminar Air flow- Vertical	Technico Laborator			Technico Laborator	1 Y	20.04.2015	19.04.2016	SVIMS	Working
1162	4	SVIMS/Virolo/04/2015/1000		Virology Lab	NC	water bath	Equitron	6701 D1	TA01AIV-10822	Equitron	1 Y	21.04.2015	20.04.2016	SVIMS	Working
1163	5	SVIMS/Viro/05/2015/1001		Virology Lab	NC	Incubator	KEMI	KIS-5	15074	KEMI	1 Y	22.04.2015	21.04.2016	SVIMS	Working
1164	6	SVIMS/Virolo/05/20151002		Virology Lab	NC	Vertical Autoclave	Equitron	7440FA	NEIIGG-11028	Equitron	1 Y	04.05.2015	03.05.2016	SVIMS	Working
1165	7	SVIMS/Viroo/05/2015/1003		Virology Lab	NC	Deep Freezer - 20 C	Remi	RQV-600P	2bcd-06542	Bhavani Enterprizer	1 Y	04.05.2015	03.05.2016	SVIMS	**Not Working**
1166	8	SVIMS/Viroo/05/2015/1004		Virology Lab	NC	Micro Plate Reader	Bio Rad	PR 4100	1410007276	Bio Rad	1 Y	07.05.2015	06.05.2016	SVIMS	Working
1167	9	SVIMS/Viroo/05/2015/1005		Virology Lab	NC	Micro Plate Washer	Bio Rad	PW-40	48527912	Bio Rad	1 Y	07.05.2015	06.05.2016	SVIMS	Working
1168	10	SVIMS/Viroo/05/2015/1006		Virology Lab	NC	PCR Workstation	Genei		046015/Fo99	Vijetha	1 Y	07.05.2015	06.05.2016	SVIMS	Working
1169	11	SVIMS/Viroo/05/2015/1007		Virology Lab	NC	Water Purification system	Bio Agen	Dura Purification	CPDC-NB-1660	Bio Agen	1 Y	16.05.2015	15.05.2016	SVIMS	Working
1170	12	SVIMS/Virolo/06/2015/1008		Virology Lab	NC	Real time PCR	Agilant Technology	G8830-64001	MY16525297	Agilant Technology	2 Y	21.05.2015	20.05.2017	SVIMS	Working
1171	13	SVIMS/Virolo/06/2015/1009		Virology Lab	NC	Bio-Spectrometer	Eppendrof		6137CP001516	Eppendrof	2 Y	02.06.2015	01.06.2017	SVIMS	Working
1172	14	SVIMS/Virolo/06/2015/1010		Virology Lab	NC	IBCOTS System	Life Technology	Bo41AIB2	30941315	Life Technology	1 Y	02.06.2015	01.06.2016	SVIMS	Working
1173	15	SVIMS/Virolo/07/2015/1011		Virology Lab	NC	Bio Safety cabinet	Thermofisher	1336	153786-122	Thermofisher	3 Y	30.06.2015	29.06.2018	SVIMS	Working
1174	16	SVIMS/Virolo/07/2015/1012		Virology Lab	NC	Mastercycler nexus gradient	Eppendorf India Ltd	6331DQ008777	6331DQ008777	Eppendorf India Ltd	2 Y	04.07.2015	03.07.2017	SVIMS	Working
1175	17	SVIMS/Virolo/07/2015/1013		Virology Lab	NC	ICE Flaker Machine	Labman	LM-1F-30	l 4006	Labman	1 Y	21.07.2015	20.07.2016	SVIMS	Working
1176	18	SVIMS/Virolo/08/2015/1014		Virology Lab	NC	Gel Documentation	Bio Screen		511236	Bio Screen	3 Y	25.07.2015	24.07.2018	SVIMS	Working
1177	19	SVIMS/Virolo/05/2017/1015		Virology Lab	NC	Deep freezer - 80	Thermo	ULT 86	3000007011	Genisis	2Y	11.8.2015	10.8.2017	SVIMS	Working

1178	20	SVIMS/Virolo/02/2015/1016		Virology Lab	NC	BioSafety Cabinet	Thermo	1384M-1384	M317010401	Genesis	5Y	17.05.2017	16.05.2022	SVIMS	Working
1179	21	SVIMS/Virolo/02/2015/1017		Virology Lab	NC	CentriFuge	Remi	R8CBL	ZBEN-17236	Indian Scientific	1Y	08-02-15	07-01-16	SVIMS	Working
1180	22	SVIMS/Virolo/02/2015/1018		Virology Lab	NC	Magnetic Stirrer-Digital	Remi	4050	1401110	Indian Scientific	1Y	08-02-15	07-02-16	SVIMS	Working
1181	23	SVIMS/Virolo/02/2015/1019		Virology Lab	NC	DryBath	Revira	5003-00/1	HP-13-06-16/103	Indian Scientific	1Y	06-02-16	06-01-17	SVIMS	Working
1182	24	SVIMS/Virolo/02/2015/1020		Virology Lab	NC	Hot Air Oven	Equitron	7051/150	AEK096		1Y	12-02-15		SVIMS	Working
1183	25	SVIMS/Virolo/02/2015/1021		Virology Lab	NC	Orbital shaker	Tarson	3060	1401019		1Y			SVIMS	Working
1184	26	SVIMS/Virolo/02/2015/1022		Virology Lab	NC	PH Meter	Eutech	ECPC-700433	2368080	Verandra Surgical	1Y			SVIMS	Working
1185	27	SVIMS/Virolo/02/2015/1023		Virology Lab	NC	Rocking Shaker	Tarson	4082	1401005		1Y			SVIMS	Working
1186	28	SVIMS/Virolo/02/2015/1024		Virology Lab	NC	Test Tube Rotator	Tarson	3070	1501RR007		1Y			SVIMS	Working
1187	29	SVIMS/Virolo/02/2015/1025		Virology Lab	NC	Vertex Shaker	Tarson	3020	1401807		1Y			SVIMS	Working
1188	30	SVIMS/Virolo/01/2001/1026		Virology Lab	NC	DRYBATH-Digital	Tarson	6040	1008		1Y			SVIMS	Working
1189	31	SVIMS/Virolo/07/2018/1124	IRS 3,70,000	Virology Lab	NC	Laminor Air Flow	ESCO	LVG-4CG-F8	2018-128735	ESCO	2Y	29/07/2018	28/07/2020	SVIMS	Working
1190	32	SVIMS/Virolo/05/2018/1200		Virology Lab	NC	Micro Plate Reader	Bio Rad Laboratories	PE40	EC718108	Poja Medical	1Y	24.05.2018	23.05.2019	SVIMS	Working
1191	33	SVIMS/Virolog/09/2018/1200		Virology Lab	NC	Mircoplate Washer	Bio Rad	PW 40	EC7G718108	Pooja Medicals	1 Y	24.05.2018	23.05.2019	SVIMS	Working
1192	34	SVIMS/Virolog/05/2019/1201		Virology Lab	NC	CO2 Incubator	Ependorf	CO - 170 R	CO17GM904333	Medicoy Life	5 Y	02.05.2019	01.05.2024	SVIMS	Working
1193	35	SVIMS/Virolog/09/2019/1171		Virology Lab-CFAR	NC	Inverted Microscope	Olympus	CKX53	8K45808	Indian Scientific	5 Y	23.09.2019	22.09.2024	SVIMS	Working
1194	36	SVIMS/Micbio/04/2019/1199		Virology Lab-CFAR	NC	40 deg C Freezer	LARK Innovative	DW-FL 531		LARK Innovative	5 Y	16.04.2019	15.04.2024	SVIMS	Working
1195	37	SVIMS/Virolog/09/2019/1215		Virology Lab-CFAR	NC	CO2 Shaker Incubator	Ependorf	S41i	S41IIK900877	Medicoy Life	5 Y	12.09.2019	11.09.2024	SVIMS	Working
1196	38	SVIMS/Virolog/09/2019/1216		Virology Lab-CFAR	NC	Real Time PCR	Thermo Scientific	QS50.2ML QPCR	272522755	Indian Scientific	5 Y	23.09.2019	22.09.2024	SVIMS	Working
1197	39			Virology Lab-CFAR	NC	Automated nucleic Acid Extraction/12 sample	Qiagen	QIA Cube	SN 49460					Covid-19	
1198	40			Virology Lab-CFAR	NC	Automated nucleic Acid Extraction/12 sample	Qiagen	QIA Cube	SN 48730					Covid-19	
1199	41			Virology Lab-CFAR	NC	Bio Safety Cabinet Class II A2	Heal Force	HF SaFE 1200 LC	SN 091912LCJ4901E					Covid-19	
1200	42			Virology Lab-CFAR	NC	Real Time PCR	Thermo Scientific	Quant Studio 5	SN 272523527					Covid-19	
1201	43			Virology Lab-CFAR	NC	Refrigerated Centrifuge	Eppendrof	5430R	SN 5428JH630					Covid-19	

									261						
1202	44			Virology Lab-CFAR	NC	Automated nucleic Acid Extraction/96 well	Qiagen	QIA Cube HT	SN015012					Covid-19	
1203	45			Virology Lab-CFAR	NC	Liquid Handling flatform	QIAGEN	QIAgility	SN015868					Covid-19	
1204	46			Virology Lab-CFAR	NC	Deep Freezer minus 86	Eppendrof	U410-86	F410IN213634					Covid-19	
1205	47			Virology Lab-CFAR	NC	Autoclave - Horizontal	Alapatt Medica	Horzontal	S.No.006					Covid-19	
1206	48			Virology Lab-CFAR	NC	Incubator Shaker	Thermo	MTH-100	E02-91090					Covid-19	
1207	49			Virology Lab-CFAR	NC	Deep Freezer minus 20	Remi	RQV-600 Plus	ZGFD-10827	Sri Vijaya Scientic	3Y	30.06.2020	29.06.2023	Covid-19	
1208	50			Virology Lab-CFAR	NC	Deep Freezer minus 80	Remi	ULT-650	200590091	Sri Vijaya Scientic	3Y	30.06.2020	29.06.2023	Covid-19	
1209	51			Virology Lab-CFAR	NC	Centrifuge	thermo/sorvall	ST 16R	42566029			30.06.2020		Covid-19	
1210	52			Virology Lab-CFAR	NC	Bio Safety Cabinet	THERMO	1384M	1384M 320011618					Covid-19	
1211	53			Virology Lab-CFAR	NC	Bio Safety Cabinet	THERMO	1374	1374M 320011618					Covid-19	
1212	1	SVIMS/PhyThe/07/2011/1027		**Physio Therapy**	NC	Laser Therapy	Electro care	EC Laser 306		Electrocare	3Y	01-01-01	31/12/2004	SVIMS	Working
1213	2	SVIMS/PhyThe/07/2010/1028		Physio Therapy	NC	**IsoKinetic System**	biodex	system 4pro		Hospimedica	3Y	21/07/2011	20/07/2014	SVIMS	Working
1214	3	SVIMS/PhyThe/09/2017/1029		Physio Therapy	NC	Traction Machine	Autotrac 100		12708		**1Y**	01-09-17	01-08-18	SVIMS	Working
1215	4	SVIMS/PhyThe/00/0000/1030		Physio Therapy	NC	Traction Machine	Autotrac		5593-A		1 Y			SVIMS	Working
1216	5	SVIMS/PhyThe/00/0000/1031		Physio Therapy	NC	Muscle Stimulators	Bharat Medical Sys	Physiotim - 7	5960		1Y			SVIMS	Working
1217	6	SVIMS/PhyThe/00/0000/1032		Physio Therapy	NC	Muscle Stimulators	Bharat Medical Sys	Physiotim - 8	5956		1 Y			SVIMS	Working
1218	7	SVIMS/PhyThe/00/0000/1033		Physio Therapy	NC	Muscle Stimulators	Bharat Medical Sys	Physiotim - 9	5057		1Y			SVIMS	Working
1219	8	SVIMS/PhyThe/00/0000/1034		Physio Therapy	NC	Muscle Stimulators	Bharat Medical Sys	Physiotim - 10	5958		1Y			SVIMS	Working
1220	9	SVIMS/PhyThe/00/0000/1035		Physio Therapy	NC	Muscle Stimulators	Bharat Medical Sys	Physiotim - 11	5959		1Y			SVIMS	Working
1221	10	SVIMS/PhyThe/00/0000/1036		Physio Therapy	NC	Muscle Stimulators	HMS		5958		1 Y			SVIMS	Working
1222	11	SVIMS/PhyThe/00/0000/1037		Physio Therapy	NC	Muscle Stimulators	HMS		10514310212		1Y			SVIMS	Working
1223	12	SVIMS/PhyThe/00/0000/1038		Physio Therapy	NC	IFT	Kody Medical	Kodytron Plus	IT 174		1 Y			SVIMS	Working

							Electronic								
1224	13	SVIMS/PhyThe/00/0000/1039		Physio Therapy	NC	IFT	Kody Medical Electronic	Kodytron Plus			1Y			SVIMS	Working
1225	14	SVIMS/PhyThe/00/0000/1040		Physio Therapy	NC	IFT	Kody Medical Electronic	Kodytron Plus			1Y			SVIMS	Working
1226	15	SVIMS/PhyThe/00/0000/1041		Physio Therapy	NC	IFT	HMS	INDOMED 601	10112360415		1Y			SVIMS	Working
1227	16	SVIMS/PhyThe/00/0000/1042		Physio Therapy	NC	WAX Therapy	HMS		110		8 Y			SVIMS	Working
1228	17	SVIMS/PhyThe/00/0000/1043		Physio Therapy	NC	WAX Therapy			1255490415		1Y			SVIMS	Working
1229	18	SVIMS/PhyThe/00/0000/1044		Physio Therapy	NC	Ultrasound	Techomed Electronics	Electroson - 709	TU -1656		9 Y			SVIMS	Working
1230	19	SVIMS/PhyThe/00/0000/1045		Physio Therapy	NC	Ultrasound	Techomed Electronics	Electroson - 710	TU -7856		1Y			SVIMS	Working
1231	20	SVIMS/PhyThe/00/0000/1046		Physio Therapy	NC	Ultrasound		Electrostim-T	TTH - 793		10 Y			SVIMS	Working
1232	21	SVIMS/PhyThe/00/0000/1047		Physio Therapy	NC	Ultrasound	HMS	INDOSONIC 102	10281660415		1Y			SVIMS	Working
1233	22	SVIMS/PhyThe/12/2014/1048		Physio Therapy	NC	Ultrasound	HMS	INDOSONIC 103	10281670415		11 Y			SVIMS	Working
1234	23	SVIMS/PhyThe/12/2014/1049		Physio Therapy	NC	Body Composition Analyzer		N 20	N20 - 2351JJH	Rs 6,54,100	5Y	12-05-14	12-04-19	SVIMS	Working
1235	24	SVIMS/PhyThe/00/0000/1050		Physio Therapy	NC	Portable Laser	Techomed Electronic		275		1 Y			SVIMS	Working
1236	25	SVIMS/PhyThe/00/0000/1051		Physio Therapy	NC	Portable Laser	Techomed Electronic		272		1Y			SVIMS	Working
1237	26	SVIMS/PhyThe/00/0000/1052		Physio Therapy	NC	Threadmill	Stayfit	CTX3	X120898013	Rs 2,09,738	1 Y			SVIMS	Working
1238	27	SVIMS/PhyThe/00/0000/1053		Physio Therapy	NC	Threadmill	Aerofit	HK300	90622789		1Y			SVIMS	Working
1239	28	SVIMS/PhyThe/00/0000/1054		Physio Therapy	NC	Short wave Diathermy	HMS	Indotherm 500	107351021	HMS	1Y			SVIMS	Working
1240	29	SVIMS/PhyThe/01/2016/1055		Physio Therapy	NC	Short wave Diathermy	IBMT				1Y			SVIMS	Working
1241	30	SVIMS/PhyThe/01/2004/1056		Physio Therapy	NC	ENMG BioFeedBack System	Enraf	Myomed 632X	15473	Rs 4,12,072	1Y	29/01/2016	28/01/2017	SVIMS	Working
1242	31	SVIMS/PhyThe/04/2018/1106		Physio Therapy	NC	Lipotone	Johari Digital	Flex-E-Tone EME 123	1708FTE420	Vijetha	1 Y	27.04.2018	26.04.2019	SVIMS	Working
1243	32	SVIMS/PhyThe/04/2018/1107		Physio Therapy	NC	Lipotone	Johari Digital	Flex-E-Tone EME 124	1708FTE455	Vijetha	1 Y	27.04.2018	26.04.2019	SVIMS	Working
1244	33	SVIMS/PhyThe/04/2018/1108		Physio Therapy	NC	Lipotone	Johari Digital	Flex-E-Tone EME 125	1708FTE465	Vijetha	1 Y	27.04.2018	26.04.2019	SVIMS	Working
1245	34	SVIMS/PhyThe/04/2018/1109		Physio Therapy	NC	Lipotone	Johari Digital	Flex-E-Tone EME 126	1708FTE469	Vijetha	1 Y	27.04.2018	26.04.2019	SVIMS	Working
1246	35	SVIMS/PhyThe/04/2019/1154		Physio Therapy	NC	Laser Therapy	Techno Med	SS - 1000	113	Pain Care	1 Y	13.04.2019	12.04.2020	SVIMS	Working

1247	36	SVIMS/PhyThe/04/ 2019/1135		Physio Therapy	NC	Waxbath	HMS Medicals		125 9100 319	HMS Medicals	1 Y	22.04.20 19	21.04.2020	SVIMS	Working
1248	37	SVIMS/PhyThe/04/ 2019/1155		Physio Therapy	NC	Waxbath	HMS Medicals		125 9090 319	HMS Medicals	1 Y	22.04.20 19	21.04.2020	SVIMS	Working
1249	38	SVIMS/PhyThe/04/ 2019/1156		Physio Therapy	NC	Ultrasound Unit	HMS Medicals	Indosonic 102	10211 2370 319	HMS Medicals	1 Y	22.04.20 19	21.04.2020	SVIMS	Working
1250	39	SVIMS/PhyThe/04/ 2019/1157		Physio Therapy	NC	Ultrasound Unit	HMS Medicals	Indosonic 102	10211 2380 319	HMS Medicals	1 Y	22.04.20 19	21.04.2020	SVIMS	Working
1251	40	SVIMS/PhyThe/04/ 2019/1158		Physio Therapy	NC	IFT	HMS Medicals	Indomed D	130 5860 319	HMS Medicals	1 Y	22.04.20 19	21.04.2020	SVIMS	Working
1252	41	SVIMS/PhyThe/04/ 2019/1159		Physio Therapy	NC	IFT	HMS Medicals	Indomed D	130 5870 319	HMS Medicals	1 Y	22.04.20 19	21.04.2020	SVIMS	Working
1253	42	SVIMS/PhyThe/04/ 2019/1160		Physio Therapy	NC	IFT	HMS Medicals	Indomed D	130 5880 319	HMS Medicals	1 Y	22.04.20 19	21.04.2020	SVIMS	Working
1254	43	SVIMS/PhyThe/04/ 2019/1161		Physio Therapy	NC	IFT	HMS Medicals	Indomed D	130 5890 319	HMS Medicals	1 Y	22.04.20 19	21.04.2020	SVIMS	Working
1255	44	SVIMS/PhyThe/04/ 2019/1162		Physio Therapy	NC	Indo TENS	HMS Medicals	Indo TENS	1101 6400 319	HMS Medicals	1 Y	22.04.20 19	21.04.2020	SVIMS	Working
1256	45	SVIMS/PhyThe/04/ 2019/1163		Physio Therapy	NC	Indo TENS	HMS Medicals	Indo TENS	1101 6410 319	HMS Medicals	1 Y	22.04.20 19	21.04.2020	SVIMS	Working
1257	46	SVIMS/PhyThe/11/ 2019/1254		Physio Therapy	NC	Muscle Stimulators-Diag	Techno Med	Electrostim DT	5463	Pain care	1Y	11-11-19	11-10-20	SVIMS	Working
1258	47	SVIMS/PhyThe/11/ 2019/1255		Physio Therapy	NC	Muscle Stimulators-Diag	Techno Med	Electrostim DT	5464	Pain care	1Y	11-11-19	11-10-20	SVIMS	Working
1259	48	SVIMS/PhyThe/11/ 2019/1256		Physio Therapy	NC	Muscle Stimulators-Diag	Techno Med	Electrostim DT	5465	Pain care	1Y	11-11-19	11-10-20	SVIMS	Working
1260	49	SVIMS/PhyThe/11/ 2019/1257		Physio Therapy	NC	Muscle Stimulators-Diag	Techno Med	Electrostim DT	5466	Pain care	1Y	11-11-19	11-10-20	SVIMS	Working
1261	50	SVIMS/PhyThe/11/ 2019/1258		Physio Therapy	NC	Muscle Stimulators-Theraputic	Techno Med	Computerised Therapy	3806	Pain care	1Y	11-11-19	11-10-20	SVIMS	Working
1262	51	SVIMS/PhyThe/11/ 2019/1259		Physio Therapy	NC	Muscle Stimulators-Theraputic	Techno Med	Computerised Therapy	3807	Pain care	1Y	11-11-19	11-10-20	SVIMS	Working
1263	52	SVIMS/PhyThe/11/ 2019/1260		Physio Therapy	NC	Muscle Stimulators-Theraputic	Techno Med	Computerised Therapy	3808	Pain care	1Y	11-11-19	11-10-20	SVIMS	Working
1264	53	SVIMS/PhyThe/11/ 2019/1261		Physio Therapy	NC	Muscle Stimulators-Theraputic	Techno Med	Computerised Therapy	3809	Pain care	1Y	11-11-19	11-10-20	SVIMS	Working
1265	54	SVIMS/PhyThe/11/ 2019/1262		Physio Therapy	NC	Muscle Stimulators-Theraputic	Techno Med	Computerised Therapy	3810	Pain care	1Y	11-11-19	11-10-20	SVIMS	Working
1266	55	SVIMS/PhyThe/11/ 2019/1263		Physio Therapy	NC	Muscle Stimulators-Theraputic	Techno Med	Computerised Therapy	3811	Pain care	1Y	11-11-19	11-10-20	SVIMS	Working
1267	56	SVIMS/PhyThe/11/ 2019/1264		Physio Therapy	NC	Muscle Stimulators-Theraputic	Techno Med	Computerised Therapy	3812	Pain care	1Y	11-11-19	11-10-20	SVIMS	Working

1268	57	SVIMS/PhyThe/11/2019/1265		Physio Therapy	NC	Muscle Stimulators-Theraputic	Techno Med	Computerised Therapy	3813	Pain care	1Y	11-11-19	11-10-20	SVIMS	Working
1269	58	SVIMS/PhyThe/11/2019/1266		Physio Therapy	NC	ViBrator	Thrive Co Ltd	717	NA	Pain care	1Y	15/11/2019	11-10-20	SVIMS	Working
1270	59	SVIMS/PhyThe/11/2019/1267		Physio Therapy	NC	ViBrator	Thrive Co Ltd	717	NA	Pain care	1Y	15/11/2019	11-10-20	SVIMS	Working
1271	60	SVIMS/PhyThe/11/2019/1268		Physio Therapy	NC	ViBrator	Thrive Co Ltd	717	NA	Pain care	1Y	15/11/2019	11-10-20	SVIMS	Working
1272	61	SVIMS/PhyThe/11/2019/1269		Physio Therapy	NC	ViBrator	Thrive Co Ltd	717	NA	Pain care	1Y	15/11/2019	11-10-20	SVIMS	Working
1273	62	SVIMS/PhyThe/11/2019/1270		Physio Therapy	NC	IR Lamp		NA	NA	Pain care	1Y	15/11/2019	11-10-20	SVIMS	Working
1274	63	SVIMS/PhyThe/11/2019/1271		Physio Therapy	NC	IR Lamp		NA	NA	Pain care	1Y	15/11/2019	11-10-20	SVIMS	Working
1275	64	SVIMS/PhyThe/11/2019/1272		Physio Therapy	NC	IR Lamp		NA	NA	Pain care	1Y	15/11/2019	11-10-20	SVIMS	Working
1276	65	SVIMS/PhyThe/11/2019/1273		Physio Therapy	NC	IR Lamp		NA	NA	Pain care	1Y	15/11/2019	11-10-20	SVIMS	Working
1277	1	SVIMS/BioT/08/2008/1059		Bio-Technology	NC	Double Distilled Water plant	BHANU	AQDD-20P-DB	160606058	Infusil India Pvt	1Y	05.01.2005	04.01.2006	SVIMS	Working
1278	2	SVIMS/BioT/08/2008/1060		Bio-Technology	NC	Deep Freezer -20C		Vestfrost	1245	Vijetha medical Systems	1Y	20.08.2008	19.08.2009	SVIMS	Working
1279	3	SVIMS/BioTec/10/2008/1062		Bio-Technology	NC	Cooling Centrifuge	Remi	C-24	BY01-7941	Vijetha medical Systems	1Y	28.10.2008	27.10.2009	SVIMS	Working
1280	4	SVIMS/BioTec/10/2006/1063		Bio-Technology	NC	Laminar Air Flow (2x2)	Air Tech			Bross Sci	1Y	27.10.2006	26.10.2007	SVIMS	Working
1281	5	SVIMS/BioTec/05/2004/1064		Bio-Technology	NC	UV trans Illuminator	Lab india			Bross Sci	1Y	13.05.2004	12.05.2005	SVIMS	Working
1282	6	SVIMS/BioTec/07/2009/1065		Bio-Technology	NC	Sonicator	Revotek	STD Sonicator	1999	Indian Scientific	1Y	31.07.2009	30.07.2010	SVIMS	Working
1283	7	SVIMS/BioTec/05/2009/1066		Bio-Technology	NC	Colony Counter	HIMEDIA		LA660/167/0923	Bross Sci	1Y	04.05.2009	03.05.2010	SVIMS	Working
1284	8	SVIMS/BioTec/09/2004/1067		Bio-Technology	NC	Dry Bath	GENEI	DB900	409696	Bross Sci	1Y	17.09.2004	16.09.2005	SVIMS	Working
1285	9	SVIMS/BioTec/09/2005/1068		Bio-Technology	NC	Cyclo Mixer	Remi	CM-101	1KXCM1624	Indian Scientific	1Y	08.09.2005	07.09.2006	SVIMS	Working
1286	10	SVIMS/BioTec/11/2008/1069		Bio-Technology	NC	DNA Sequencer	GENEI			L.V.products	1Y	26.11.2008	25.11.2009	SVIMS	Working
1287	11	SVIMS/BioTec/12/2003/1070		Bio-Technology	NC	Laminar Air Flow (4x2x2)	Clean Air	CAH1200		Indian Scientific	1Y	06.12.2003	05.12.2004	SVIMS	Working
1288	12	SVIMS/BioTec/04/2005/1071		Bio-Technology	NC	Inverted Microscope	Motic AE-31	50212001	Motic	Lab AID	1Y	29.04.2005	28.04.2006	SVIMS	Working
1289	13	SVIMS/BioTec/09/2005/1072		Bio-Technology	NC	Multiporator	Ependrof		430830479	Ependrof	1Y	01.09.2005	31.08.2006	SVIMS	Working
1290	14	SVIMS/BioTec/07/2016/1073	RS 4,62,000/-	Bio-Technology	NC	PCR	Ependrof		6331FH311350	Ependrof	1Y	19/07/16	18/07/17	SVIMS	Working
1291	15	SVIMS/BioTec/06/2004/1074		Bio-Technology	NC	UV trans Illuminator	Lab india		514245	Bross Sci	1Y	13.06.2004	12.06.2005	SVIMS	Working
1292	16	SVIMS/BioTec/05/2005/1075		Bio-Technology	NC	Gel Documenter	Vilber Lourmet		515258	Labmate	1Y	20.05.2005	18.05.2007	SVIMS	Working

1293	17	SVIMS/BioTec/08/2009/1076		Bio-Technology	NC	PH Meter	Eutech		1470569	Bross Sci	1Y	28.08.2009	27.08.2010	SVIMS	Working
1294	18	SVIMS/BioTec/01/2009/1077		Bio-Technology	NC	UV Spectrophotometer	Cyber Lab	CYBER UV-1	2C4630-07A008-00	Indian Scientific	1Y	06.01.2009	05.01.2010	SVIMS	Working
1295	19	SVIMS/BioTec/02/2017/1079		Bio-Technology	NC	CO2 Incubator	Thermofisher	Stericycle i160	42057396	Genesis	5Y	16/02/2017	**15/02/2022**	SVIMS	Working
1296	20	SVIMS/BioTec/12/2002/1080		Bio-Technology	NC	PH Meter	Systronics	361	2425	Systronics	1Y	06.12.2002	05.12.2003	SVIMS	Working
1297	21	SVIMS/BioTec/09/2005/1081		Bio-Technology	NC	Homogenizer	Remi	RQ127A	AML252	Inaian Scie	1Y	06.12.2003	05.12.2004	SVIMS	Working
1298	22	SVIMS/BioTec/09/2005/1082		Bio-Technology	NC	Water Bath	Remi	KWB.190	4192	Indian Scientific	1Y	08.09.2005	07.09.2006	SVIMS	Working
1299	23	SVIMS/BioTec/03/2005/1084		Bio-Technology	NC	Electrophoresis Horizantel	GENEI			Indian Scientific	1Y	23.03.2005	22.03.2006	SVIMS	Working
1300	24	SVIMS/BioTec/03/2005/1085		Bio-Technology	NC	Electrophoresis Verticle	GENEI			Indian Scientific	1Y	23.03.2005	22.03.2006	SVIMS	Working
1301	25	SVIMS/BioTec/03/2005/1086		Bio-Technology	NC	GEL Rocker	GENEI	GR020	504332	Indian Scientific	1Y	23.03.2005	22.03.2006	SVIMS	Working
1302	26	SVIMS/BioTec/03/2005/1087		Bio-Technology	NC	Incubator 37C	Yarco	YSI-438	04B2446	Lszer Instru	1Y	14.03.2005	13.03.2006	SVIMS	Working
1303	27	SVIMS/BioTec/01/2004/1088		Bio-Technology	NC	GEL Dryer	GENEI	2535/3545	104081	Indian Scientific	1Y	06.01.2004	05.01.2005	SVIMS	Working
1304	28	SVIMS/BioTec/10/2008/1089		Bio-Technology	NC	Cooling Centrifuge	Remi	RBC	JDLC-4448	Indian Scientific	1Y	20.10.2008	21.10.2009	SVIMS	Working
1305	29	SVIMS/BioTec/12/2003/1090		Bio-Technology	NC	Centrifuge	Remi	RBC	AMLC-398	Indian Scientific	1Y	10.12.2003	09.12.2004	SVIMS	Working
1306	30	SVIMS/BioTec/10/2004/1091		Bio-Technology	NC	BOD Incubator	HECO	216		Bross Sci	1Y	06.10.2004	05.10.2005	SVIMS	Working
1307	31	SVIMS/BioTec/01/2009/1092		Bio-Technology	NC	Real Time PCR	Applied Bio	7300	273003646	Lab India	1Y	04-01-09	31/4/2010	SVIMS	Working
1308	32	SVIMS/BioTec/12/2003/1093		Bio-Technology	NC	Microscope	Olympus	CX21i	12F-429		1Y	10.12.2003	09.12.2004	SVIMS	Working
1309	33	SVIMS/BioTec/12/2003/1094		Bio-Technology	NC	Microscope (Monocular)	Olympus	MLM	13-F1315		1Y	10.12.2003	09.12.2004	SVIMS	Working
1310	34	SVIMS/BioTec/12/2003/1095		Bio-Technology	NC	Microscope (Monocular)	Olympus	MLM	13F-1320		1Y	10.12.2003	09.12.2004	SVIMS	Working
1311	35	SVIMS/BioTec/12/2003/1096		Bio-Technology	NC	Microscope (Monocular)	Olympus	MLM	13F-1349		1Y	10.12.2003	09.12.2004	SVIMS	Working
1312	36	SVIMS/BioTec/10/2019/1218		Bio-Technology	NC	Analytical Weighing Balance	SHIMADZU	AUW320	D449326056	SSR Enterprises	1Y	11.10.2019	10.10.2020	SVIMS	Working

Equipment status Report on 31st JANUARY, 2021– SVIMS, SPMCW-Hospital

Total Number of Equipment = 145

Number of functional Equipment=144

Number of Non functional Equipment = 1

Action Report

Sl No	Equipment	Manufacturer	Days of Disrepair	Value	Remarks
1	Ventilator	Air Liquide	11/01/2021	6,50,000	Needs parts. Under process

Equipment List - SPMCW – Hospital

	Index Number	Equipment	Department	Manufacturer	Supplier	Model	serial number	W	Ins.date	Purchase done by	Status	Unit cost in IRs
1	SPMCH/GenSur/05/2015/ 0001	OT Lights Dual Dome	Septic OT	Magna Tek	Magna Tek	Magnapax	G2002	3 Y	11.05.2015	APMSIDC	Working	3,47,000
2	SPMCH/ophtha/04/2015/ 0002	OT Lights Dual Dome	Emergency OT	Magna Tek	Magna Tek	Magnapax	G1960	3 Y	30.04.2015	APMSIDC	Working	3,47,000
3	SPMCH/OB&GYN/04/2015/ 0003	OT Lights Dual Dome	O B G	Magna Tek	Magna Tek	Magnapax	G1961	3 Y	30.04.2015	APMSIDC	Working	3,47,000
4	SPMCH/OB&GYN/04/2015/ 0004	OT Lights Dual Dome	O B G	Magna Tek	Magna Tek	Magnapax	G1962	3 Y	30.04.2015	APMSIDC	Working	3,47,000
5	SPMCH/ E N T /04/2015/ 0005	OT Lights Dual Dome	E N T	Magna Tek	Magna Tek	Magnapax	G1963	3 Y	30.04.2015	APMSIDC	Working	3,47,000
6	SPMCH/GenSur/04/2015/ 0006	OT Lights Dual Dome	G S O T	Magna Tek	Magna Tek	Magnapax	G1964	3 Y	30.04.2015	APMSIDC	Working	3,47,000
7	SPMCH/Anaest/05/2015/ 0007	Multi para Monitor	Anaesthesia	General Meditech	Trans Health Care	G 3 G	G3GM30013	3 Y	05.05.2015	APMSIDC	Working	1,41,750
8	SPMCH/Anaest/05/2015/ 0008	Multi para Monitor	Anaesthesia	General Meditech	Trans Health Care	G 3 G	G3GM30003	3 Y	05.05.2015	APMSIDC	Working	1,41,750
9	SPMCH/Anaest/05/2015/ 0009	Multi para Monitor	OBG ICU - 2	General Meditech	Trans Health Care	G 3 G	G3GM30029	3 Y	05.05.2015	APMSIDC	Working	1,41,750
10	SPMCH/Anaest/05/2015/ 0010	Multi para Monitor	Anaesthesia	General Meditech	Trans Health Care	G 3 G	G3GM30017	3 Y	05.05.2015	APMSIDC	Working	1,41,750

11	SPMCH/Anaest/05/2015/ 0011	Multi para Monitor	Anaesthesia	General Meditech	Trans Health Care	G 3 G	G3GM30005	3 Y	05.05.2015	APMSIDC	Working	1,41,750
12	SPMCH/Anaest/05/2015/ 0012	Multi para Monitor	O B G	General Meditech	Trans Health Care	G 3 G	G3GM30008	3 Y	05.05.2015	APMSIDC	Working	1,41,750
13	SPMCH/Anaest/05/2015/ 0013	Multi para Monitor	Anaesthesia	General Meditech	Trans Health Care	G 3 G	G3GM30021	3 Y	05.05.2015	APMSIDC	Working	1,41,750
14	SPMCH/Anaest/05/2015/ 0014	Multi para Monitor	Anaesthesia	General Meditech	Trans Health Care	G 3 G	G3GM30030	3 Y	05.05.2015	APMSIDC	**Not Working**	1,41,750
15	SPMCH/Anaest/05/2015/ 0015	Multi para Monitor	G S O T	General Meditech	Trans Health Care	G 3 G	G3GM30010	3 Y	05.05.2015	APMSIDC	Working	1,41,750
16	SPMCH/ Anaest/05/2015/ 0016	Multi para Monitor	E N T	General Meditech	Trans Health Care	G 3 G	G3GM30028	3 Y	05.05.2015	APMSIDC	Working	1,41,750
17	SPMCH/Anaest/05/2015/ 0017	Multi para Monitor	O B G	General Meditech	Trans Health Care	G 3 G	G3GM30022	3 Y	05.05.2015	APMSIDC	Working	1,41,750
18	SPMCH/Anaest/05/2015/ 0018	Multi para Monitor	O B G	General Meditech	Trans Health Care	G 3 G	G3GM30023	3 Y	05.05.2015	APMSIDC	Working	1,41,750
18	SPMCH/Anaest/09/2015/ 0019	Multichannel Monitor	Anaesthesia	General Meditech	Trans Health Care	G3G	434M50059	3 Y	30.09.2015	APMSIDC	Working	1,32,300
19	SPMCH/Anaest/09/2015/ 0020	Multichannel Monitor	Anaesthesia	General Meditech	Trans Health Care	G3G	434M50007	3 Y	30.09.2015	APMSIDC	Working	1,32,300
20	SPMCH/Anaest/09/2015/ 0021	Multichannel Monitor	Anaesthesia	General Meditech	Trans Health Care	G3G	434M50044	3 Y	30.09.2015	APMSIDC	Working	1,32,300
21	SPMCH/Anaest/09/2015/ 0022	Multichannel Monitor	Anaesthesia	General Meditech	Trans Health Care	G3G	434M50006	3 Y	30.09.2015	APMSIDC	Working	1,32,300
22	SPMCH/Anaest/09/2015/ 0023	Multichannel Monitor	OBG ICU - 1	General Meditech	Trans Health Care	G3G	434M50003	3 Y	30.09.2015	APMSIDC	Working	1,32,300
23	SPMCH/Anaest/09/2015/ 0024	Multichannel Monitor	Anaesthesia	General Meditech	Trans Health Care	G3G	434M50010	3 Y	30.09.2015	APMSIDC	Working	1,32,300
25	SPMCH/Anaest/05/2015/ 0025	ICU Ventilator	Anaesthesia	Air Liquide	Air Liquide Medical	Monnal 175	MT 75-04315	3 Y	26.05.2015	APMSIDC	**Working**	6,50,000
26	SPMCH/Anaest/05/2015/ 0026	ICU Ventilator	Anaesthesia	Air Liquide	Air Liquide Medical	Monnal 175	MT 75-04316	3 Y	26.05.2015	APMSIDC	Working	6,50,000
27	SPMCH/Anaest/05/2015/ 0027	ICU Ventilator	Anaesthesia	Air Liquide	Air Liquide Medical	Monnal 175	MT 75-04317	3 Y	26.05.2015	APMSIDC	Working	6,50,000
28	SPMCH/Anaest/05/2015/ 0028	ICU Ventilator	Anaesthesia	Air Liquide	Air Liquide Medical	Monnal 175	MT 75-04318	3 Y	26.05.2015	APMSIDC	NotWork ing	6,50,000
29	SPMCH/Anaest/05/2015/ 0029	ICU Ventilator	Anaesthesia	Air Liquide	Air Liquide Medical	Monnal 175	MT 75-04319	3 Y	26.05.2015	APMSIDC	Working	6,50,000

30	SPMCH/Anaest/05/2015/ 0030	ICU Ventilator	Anaesthesia	Air Liquide	Air Liquide Medical	Monnal 175	MT 75-04320	3 Y	26.05.2015	APMSIDC	**Not Working**	6,50,000
31	SPMCH/ Ophtha/06/2015/ 0031	Potec Auto Ref.Keratometer	Ophthalmology	Appasamy Associates	Appasamy Associates	PRK 6000	K6DL18F	1 Y	01.06.2015	SVIMS	Working	
32	SPMCH/ ENT/06/2015/ 0032	Impedenec Audiometer stem with accessories	E N T	Alliance Biomedica	Alliance Biomedica	G3139 Velsion3	G50059259	3 Y	08.06.2015	SVIMS	Working	4,72,557
33	SPMCH/GenSur/08/2015/ 0033	Bipolar Cautery	G S O T	ERBE, Germany	ERBE, Germany	VIO 300S Version I	11394575	3y	14.08.2015	SVIMS	Working	3,93,750
34	SPMCH/GenSur/08/2015/ 0034	Bipolar Cautery	Emergency OT	ERBE, Germany	ERBE, Germany	VIO 300S Version I	11394574	3 Y	14.08.2015	SVIMS	Working	3,93,750
35	SPMCH/ENT/08/2015/ 0035	Bipolar Cautery	E N T	ERBE, Germany	ERBE, Germany	VIO 300S Version I	11395339	3 Y	14.08.2015	SVIMS	Working	3,93,750
36	SPMCH/OB&Gyn/08/2015/ 0036	Bipolar Cautery	O B G	ERBE, Germany	ERBE, Germany	VIO 300S Version I	11398195	3 Y	14.08.2015	SVIMS	Working	3,93,750
37	SPMCH/OB&Gyn/08/2015/ 0037	Cryosurgery Unit	Gynaecalogy	ERBE, Germany	ERBE, Germany	ERBO KRYO CA	11397972	3 Y	14.08.2015	SVIMS	Working	5,98,500
38	SPMCH/OB&Gyn/08/2015/ 0038	Cryosurgery Unit	Gynaecalogy	ERBE, Germany	ERBE, Germany	ERBO KRYO CA	11397971	3 Y	14.08.2015	SVIMS	Working	5,98,500
39	SPMCH/Anaest/09/2015/ 0039	Infusion Pump	Anaesthesia	GUANGZHOU WIT	Trans Health Care	WIT 601A	60100 1506047	3 Y	30.09.2015	APMSIDC	Working	34,963
40	SPMCH/Anaest/09/2015/ 0040	Infusion Pump	Anaesthesia	GUANGZHOU WIT	Trans Health Care	WIT 601A	601001 503059	3 Y	30.09.2015	APMSIDC	Working	34,963
41	SPMCH/Anaest/09/2015/ 0041	Infusion Pump	Anaesthesia	GUANGZHOU WIT	Trans Health Care	WIT 601A	60102 1506001	3 Y	30.09.2015	APMSIDC	Working	34,963
42	SPMCH/Anaest/09/2015/ 0042	Infusion Pump	Anaesthesia	GUANGZHOU WIT	Trans Health Care	WIT 601A	60103 1506041	3 Y	30.09.2015	APMSIDC	Working	34,963
43	SPWMC/Anaest/09/2015/ 0043	Infusion Pump	Anaesthesia	GUANGZHOU WIT	Trans Health Care	WIT 601A	60104 1506040	3 Y	30.09.2015	APMSIDC	Working	34,963
44	SPMCH/Anaest/09/2015/ 0044	Infusion Pump	Anaesthesia	GUANGZHOU WIT	Trans Health Care	WIT 601A	60105 1506042	3 Y	30.09.2015	APMSIDC	Working	34,963
45	SPMCH/Anaest/09/2015/ 0045	Infusion Pump	Anaesthesia	GUANGZHOU WIT	Trans Health Care	WIT 601A	60106 1506043	3 Y	30.09.2015	APMSIDC	Working	34,963
46	SPMCH/Anaest/09/2015/ 0046	Infusion Pump	Anaesthesia	GUANGZHOU WIT	Trans Health Care	WIT 601A	60107 1506044	3 Y	30.09.2015	APMSIDC	Working	34,963
47	SPMCH/Anaest/09/2015/ 0047	Infusion Pump	Anaesthesia	GUANGZHOU WIT	Trans Health Care	WIT 601A	60108 1506002	3 Y	30.09.2015	APMSIDC	Working	34,963
48	SPMCH/Anaest/09/2015/ 0048	Infusion Pump	Anaesthesia	GUANGZHOU WIT	Trans Health Care	WIT 601A	60109 1503058	3 Y	30.09.2015	APMSIDC	Working	34,963

49	SPMCH/Anaest/10/2015/ 0049	Anaesthesia Workstation	Anaesthesia	Allied Medical	Allied Medical Ltd	Jupiter Plus	1503JP111	3 Y	16.10.2015	APMSIDC	Working	5,76,535
50	SPMCH/Anaest/10/2015/ 0050	Anaesthesia Workstation	O B G	Allied Medical	Allied Medical Ltd	Jupiter Plus	1503JP112	3 Y	16.10.2015	APMSIDC	Working	5,76,535
51	SPMCH/Anaest/10/2015/ 0051	Anaesthesia Workstation	Anaesthesia	Allied Medical	Allied Medical Ltd	Jupiter Plus	1503JP113	3 Y	16.10.2015	APMSIDC	Working	5,76,535
52	SPMCH/Anaest/10/2015/ 0052	Anaesthesia Workstation	Anaesthesia	Allied Medical	Allied Medical Ltd	Jupiter Plus	1503JP114	3 Y	16.10.2015	APMSIDC	Working	5,76,535
53	SPMCH/Anaest/10/2015/ 0053	Anaesthesia Workstation	Emergency OT	Allied Medical	Allied Medical Ltd	Jupiter Plus	1503JP115	3 Y	16.10.2015	APMSIDC	Working	5,76,535
54	SPMCH/Anaest/10/2015/ 0054	Anaesthesia Workstation	Septic OT	Allied Medical	Allied Medical Ltd	Jupiter Plus	1503JP116	3 Y	16.10.2015	APMSIDC	Working	5,76,535
55	SPMCH/OB&Gyn/06/2015/ 0055	Suction Apparatus	OBG	Supreme Enterprises		INSTAVAC	15F26-001	3 Y	24.06.2015	APMSIDC	Working	18,750
56	SPMCH/GenSur/06/2015/ 0056	Suction Apparatus	General Surgery	Supreme Enterprises		INSTAVAC	15F26-002	3 Y	24.06.2015	APMSIDC	Working	18,750
57	SPMCH/OB&Gyn/06/2015/ 0057	Suction Apparatus	OBG	Supreme Enterprises		INSTAVAC	15F26-003	3 Y	24.06.2015	APMSIDC	Working	18,750
58	SPMCH/OB&Gyn/06/2015/ 0058	Suction Apparatus	OBG	Supreme Enterprises		INSTAVAC	15F26-004	3 Y	24.06.2015	APMSIDC	Working	18,750
59	SPMCH/ENT/06/2015/ 0059	Suction Apparatus	ENT	Supreme Enterprises		INSTAVAC	15F26-005	3 Y	24.06.2015	APMSIDC	Working	18,750
60	SPMCH/OB&Gyn/06/2015/ 0060	Suction Apparatus	Obg	Supreme Enterprises		INSTAVAC	15F26-006	3 Y	24.06.2015	APMSIDC	Working	18,750
61	SPMCH/E N T /06/2015/ 0061	Suction Apparatus	ENT	Supreme Enterprises		INSTAVAC	15F26-007	3 Y	24.06.2015	APMSIDC	Working	18,750
62	SPMCH/OB&Gyn/06/2015/ 0062	Suction Apparatus	OBG	Supreme Enterprises		INSTAVAC	15F26-008	3 Y	24.06.2015	APMSIDC	Working	18,750
63	SPMCH/GenSur/06/2015/ 0063	Suction Apparatus	General Surgery	Supreme Enterprises		INSTAVAC	15F26-009	3 Y	24.06.2015	APMSIDC	Working	18,750
64	SPMCH/GenSur/06/2015/ 0064	Suction Apparatus	General Surgery	Supreme Enterprises		INSTAVAC	15F26-010	3 Y	24.06.2015	APMSIDC	Working	18,750
65	SPMCH/Nuroom/06/2015/ 0065	Suction Apparatus	Nurses Room	Supreme Enterprises		INSTAVAC	15F26-011	3 Y	24.06.2015	APMSIDC	Working	18,750
66	SPMCH/OB&Gyn/06/2015/ 0066	Suction Apparatus	OBG Ward	Supreme Enterprises		INSTAVAC	15F26-012	3 Y	24.06.2015	APMSIDC	Working	18,750
67	SPMCH/NI C U/06/2015/ 0067	Suction Apparatus	NICU	Supreme Enterprises		INSTAVAC	15F26-013	3 Y	24.06.2015	APMSIDC	Working	18,750

68	SPMCH/GenSur/06/2015/ 0068	Suction Apparatus	General Surgery	Supreme Enterprises		INSTAVAC	15F26-014	3 Y	24.06.2015	APMSIDC	Working	18,750
69	SPMCH/N I C U/06/2015/ 0069	Suction Apparatus	NICU	Supreme Enterprises		INSTAVAC	15F26-015	3 Y	24.06.2015	APMSIDC	Working	18,750
70	SPMCH/N I C U/06/2015/ 0070	Suction Apparatus	NICU	Supreme Enterprises		INSTAVAC	15F26-016	3 Y	24.06.2015	APMSIDC	Working	18,750
71	SPMCH/OB&Gyn/06/2015/ 0071	Suction Apparatus	OBG OT	Supreme Enterprises		INSTAVAC	15F26-017	3 Y	24.06.2015	APMSIDC	Working	18,750
72	SPMCH/OB&Gyn/06/2015/ 0072	Suction Apparatus	Nurses Room	Supreme Enterprises		INSTAVAC	15F26-018	3 Y	24.06.2015	APMSIDC	Working	18,750
73	SPMCH/OB&Gyn/06/2015/ 0073	Suction Apparatus	OBG OT	Supreme Enterprises		INSTAVAC	15F26-019	3 Y	24.06.2015	APMSIDC	Working	18,750
74	SPMCH/OB&Gyn/06/2015/ 0074	Suction Apparatus	OBG OT	Supreme Enterprises		INSTAVAC	15F26-020	3 Y	24.06.2015	APMSIDC	Working	18,750
75	SPMCH/OB&Gyn/06/2015/ 0075	Suction Apparatus	OBG	Supreme Enterprises		INSTAVAC	15F04-001	3 Y	24.06.2015	APMSIDC	Working	18,750
76	SPMCH/OB&Gyn/06/2015/ 0076	Suction Apparatus	OBG	Supreme Enterprises		INSTAVAC	15F04-002	3 Y	24.06.2015	APMSIDC	Working	18,750
77	SPMCH/OB&Gyn/06/2015/ 0077	Suction Apparatus	OBG	Supreme Enterprises		INSTAVAC	15F04-003	3 Y	24.06.2015	APMSIDC	Working	18,750
78	SPMCH/OB&Gyn/06/2015/ 0078	Suction Apparatus	OBG	Supreme Enterprises		INSTAVAC	15F04-004	3 Y	24.06.2015	APMSIDC	Working	18,750
79	SPMCH/GenSur/06/2015/ 0079	Suction Apparatus	SICU	Supreme Enterprises		INSTAVAC	15F04-005	3 Y	24.06.2015	APMSIDC	Working	18,750
80	SPMCH/GenSur/06/2015/ 0080	Suction Apparatus	General Surgery	Supreme Enterprises		INSTAVAC	15F04-006	3 Y	24.06.2015	APMSIDC	Working	18,750
81	SPMCH/OB&Gyn/06/2015/ 0081	Suction Apparatus	OBG	Supreme Enterprises		INSTAVAC	15F04-007	3 Y	24.06.2015	APMSIDC	Working	18,750
82	SPMCH/GenSur/06/2015/ 0082	Suction Apparatus	G S Ward	Supreme Enterprises		INSTAVAC	15F04-008	3 Y	24.06.2015	APMSIDC	Working	18,750
83	SPMCH/OB&Gyn/11/2015/ 0083	Fetal Monitor (CTG)/Cardiotocogram Machine	OBG & Gynic	B P L		FM9852T	EPTB5F 1465	3 Y	28.11.2015	APMSIDC	Working	87,150
84	SPMCH/OB&Gyn/11/2015/ 0084	Fetal Monitor (CTG)/Cardiotocogram Machine	Gynic	B P L		FM9852T	EPTB5F 1463	3 Y	28.11.2015	APMSIDC	Working	87,150

85	SPMCH/E N T /12/2015/ 0085	1. Endoscopy Set with Fess Instrument with Light Source and Camera	E N T	Carl Storze	Vishal Surgical			3 Y	01.12.2015	APMSIDC	Working	81,94,091
	SPMCH/E N T /12/2015/ 0085A	2. Esophagoscopy Set(LIGHT SOURCE)				XENON NOVA 300	PU0702240					3,78,000
	SPMCH/E N T /12/2015/ 0085B	3. Light Source with Cable and Head Band				XENON NOVA 300	PU0702097					10,20,275
	SPMCH/E N T /12/2015/ 0085C	4. Rhino-Pharyngo-Laryngo-Fiberscope										5,71,253
	SPMCH/E N T /12/2015/ 0085D	TH100 Image 1 H3-ZSPIES Sl.No.RZW829256-H,									Working	
	SPMCH/E N T /12/2015/ 0085E	26'FULL HD Monitor		STORZ HD	VISHAL	EJ-MLA26EKIA	L41D10267					
	SPMCH/E N T /12/2015/ 0085F	IMAGE 1 CONNECT CONSOLE		KARL STORZ	VISHAL	TC200	YU741030-P					
	SPMCH/E N T /12/2015/ 0085G	IMAGE 1 H3-LINK				TC300	RU731600-P				Working	
	SPMCH/E N T /12/2015/ 0085H	PEDSTAL FOR DEBRADOR					SU4498					
	SPMCH/E N T /12/2015/ 0085**I**	Debrador				Unidrive SIII ECO	PU2479					
	SPMCH/E N T /12/2015/ 0085J	Light source				XENON NOVA175	OUO701225				Working	
	SPMCH/E N T /12/2015/ 0085K	Ceramax Xenon Lamp 175W Sl.No.4HJB2694										
	SPMCH/E N T /12/2015/ 0085L	Fiber Optic Cable, Hopkins II Telescope O"4mm Sl.No.120IQV, 1201RB, Hopkins II Telescope 30"4mm									Working	

		Sl.No.1202SH										
	SPMCH/E N T /12/2015/ 0085M	Hopking II Telescope 45"4mm Sl.No.12008B, Hopkins II Telescope 70"4mm 12012X,									Working	
	SPMCH/E N T /12/2015/ 0085N	HOPKINS II TELESCOPE 0"2.7mm SlNo.1201LP, Hopkins II Telescope 30"2.7Mm Sl.No.1201A3									Working	
86	SPMCH/ Ophtha/12/2015/ 0086	1. Wireless Indirect Ophthalmoscope with 20 D Lens 2. 78 D Volk Lens 3. Near Vision Chart	Ophthalmology	Appasamy	Appasamy	AAIO Wireles	1802150237	1 Y	07.12.2015	SVIMS	Working	1. 58,000/- 2. 16,000/- 3. 450/-
87	SPMCH/ Ophtha/01/2016/ 0087	Slit Lamp-5 step	Ophthalmology	Appaswamy	Appaswamy	A1A 125S	1504160002	1 Y	11.01.16	SVIMS	Working	1,10,000
88	SPMCh/ GenSur/01/2016/ 0088	O T Table	G S O T	Hospi Tech		Hospitak	105SS		11.01.16		Working	
89	SPMCH/ OB&Gyn/01/2016/ 0089	O T Table	OBG	Hospi Tech		Hospitak	105SS		11.01.16		Working	
90	SPMCH/ E N T /01/2016/ 0090	O T Table	ENT	Hospi Tech		Hospitak	105SS		11.01.16		Working	
91	SPMCH/ Ob&Gyn/01/2016/ 0091	O T Table	OBG	Hospi Tech		Hospitak	105SS		11.01.16		Working	
92	SPMCH/GenSur/01/2016/ 0092	O T Table	Emergency OT	Hospi Tech		Hospitak	105SS		11.01.16		Working	
93	SPMCH/ Ob&Gyn/02/2016/ 0093	**Double Punch Laproscope Set**	**O B G**	**Carl Storz**	**Vishal**			3 Y	15.02.2016	APMSIDC	Working	8,90,000
	SPMCH/ Ob&Gyn/02/2016/ 0093A	CAMERA CONSOLE		KARL STORZ	VISHAL	Telecam Dx II CCU	SU731764-P				Working	
	SPMCH/ Ob&Gyn/02/2016/ 0093B	Camera Head		KARL STORZ	VISHAL	Telecam Camera Head	RU849685-H				Working	

	SPMCH/ Ob&Gyn/02/2016/ 0093C	C-Mount Lens									Working	
	SPMCH/ Ob&Gyn/02/2016/ 0093D	Light Source		KARL STORZ	VISHAL	Led Nova 150W	RU3517,				Working	
	SPMCH/ Ob&Gyn/02/2016/ 0093E	Fiber Opetic Cable									Working	
	SPMCH/ Ob&Gyn/02/2016/ 0093F	Telescope 30'6.5mm					4004694				Working	
	SPMCH/ Ob&Gyn/02/2016/ 0093G	LED Monitor		SAMSUNG	VISHAL	UA23H400 3ARLXL	H00M3PAG60 7312T				Working	
94	SPMCH/ Ob&Gyn/02/2016/ 0094	**Operating Laparoscope Set**	**O B G**	**Carl Storz**	**Vishal**			3 Y	15.02.2016	APMSIDC	Working	
	SPMCH/ Ob&Gyn/02/2016/ 0094A	CAMERA CONSOLE				Tricam SL II	RU730933-P				Working	
	SPMCH/ Ob&Gyn/02/2016/ 0094B	Camera Head				Tricam Camera Head	RU848536-H				Working	
	SPMCH/ Ob&Gyn/02/2016/ 0094C	15,Color LCD Monitor		SONY	VISHAL	LMD-1510W	3005697				Working	
	SPMCH/ Ob&Gyn/02/2016/ 0094D	Electronic CO2 Endoflator		KARL STORZ	VISHAL	26430520	SU33042				Working	
	SPMCH/ Ob&Gyn/02/2016/ 0094E	Light Source		KARL STORZ	VISHAL	Led Nova Light 150W	SU3591				Working	
	SPMCH/ Ob&Gyn/02/2016/ 0094F	Fiber Optic Cable 4.8mm									Working	
	SPMCH/ Ob&Gyn/02/2016/ 0094G	Hopkins II Telescope 30'10mm					121BLO				Working	
95	SPMCH/ Ob&Gyn/02/2016/ 0095	**Operating Laparoscope Set**	**O B G**	**Carl Storz**	**Vishal**			3 Y	15.02.2016	APMSIDC	Working	
	SPMCH/ Ob&Gyn/02/2016/ 0095A	Camera CONSOLE		KARL STORZ	VISHAL	Tricam SL II	RU730926-P				Working	
	SPMCH/ Ob&Gyn/02/2016/ 0095B	Camera Head				Tricam Camera Head	PU848358-H				Working	
	SPMCH/ Ob&Gyn/02/2016/ 0095C	15,Color LCD Monitor		SONY	VISHAL	LMD-2110MD	3206129				Working	
	SPMCH/ Ob&Gyn/02/2016/ 0095D	Electronic CO2 Endoflator		KARL STORZ	VISHAL	26430520	SU33053				Working	
	SPMCH/ Ob&Gyn/02/2016/ 0095E	Light Source		KARL STORZ	VISHAL	Led Nova Light 150W	SU3597				Working	

						Light Source						
	SPMCH/ Ob&Gyn/02/2016/ 0095F	Fiber Optic Cable 4.8mm									Working	
	SPMCH/ Ob&Gyn/02/2016/ 0095G	Hopkins II Telescope 30'10mm					121AAF				Working	
96	SPMCH/ Ob&Gyn/02/2016/ 0096	**Coloposcope Set**	**O B G**		**Vishal**	**Video Colopscope**	**15-070013**	3 Y	15.02.2016	APMSIDC	Working	9,08,250
	SPMCH/ Ob&Gyn/02/2016/ 0096A	Coloposcope SeT	O B G		Vishal	Video Colopscope	15-070013	3 Y	15.02.2016	APMSIDC	Working	
	SPMCH/ Ob&Gyn/02/2016/ 0096B	Stand for Coloposcope										
	SPMCH/ Ob&Gyn/02/2016/ 0096C	Laptop with Medi-Scope Oem lite edition Software, Data Recording System										
97	SPMCH/ N I C U /03/2016/ 0097	Baby Weighing Machine	Pediatrics	nice Neotech Medical	nice Neotech Medical		15160 300 2089	1 Y	29.03.2016	APMSIDC	Working	v
98	SPMCH/ N I C U /03/2016/ 0098	Baby Weighing Machine	Pediatrics	nice Neotech Medical	nice Neotech Medical		15160 300 2092	1 Y	29.03.2016	APMSIDC	Working	14,175
99	SPMCH/ N I C U /03/2016/ 0099	Infant meter	Pediatrics	nice Neotech Medical	nice Neotech Medical			1 Y	29.03.2016	APMSIDC	Working	13,356
100	SPMCH/ Ob&Gyn /04/2016/ 0100	**Diagnostic Laparoscopy set**	**Gynaec OT**	**Karl Storz Germany**	**Vishal**			3 Y	05.04.2016	APMSIDC	Working	28,84,350
	SPMCH/ Ob&Gyn /04/2016/ 0100A	HOPKINS Telescope 30' 10mm, 31cm					121J4E				Working	
	SPMCH/ Ob&Gyn /04/2016/ 0100B	Electronic CO2 Endoflator SCB Set		KARL STORZ	VISHAL	26430520	NT34312				Working	
	SPMCH/ Ob&Gyn /04/2016/ 0100C	Light Source		KARL STORZ	VISHAL	LED Nova 150	OT4383				Working	
	SPMCH/ Ob&Gyn /04/2016/ 0100D	CAMERA CONSOLE		KARL STORZ	VISHAL	TRICAM SL II	YU741134-P				Working	
	SPMCH/ Ob&Gyn /04/2016/ 0100E	Camera Head		KARL STORZ	VISHAL	TRICAM 2 Chip	XU857546-H				Working	
	SPMCH/ Ob&Gyn /04/2016/ 0100F	Monitor		SONY	VISHAL	LMD-1510W	3005690				Working	
101	SPMCH/OB&Gyn/04/2016/0101	**Diagnostic Laparoscopy set**	**Gynaec OT**	**Karl Storz Germany**	**Vishal**			3 Y	05.04.2016	APMSIDC	Working	28,84,350

	SPMCH/OB&Gyn/04/2016/0101A	HOPKINS Telescope 30' 10mm, 31cm					121FDX				Working	
	SPMCH/OB&Gyn/04/2016/0101B	Electronic CO2 Endoflator SCB Set		KARL STORZ	VISHAL	26430520	NT34323				Working	
	SPMCH/OB&Gyn/04/2016/0101C	Light SOURCE		KARL STORZ	VISHAL	LED Nova 150	OT4389				Working	
	SPMCH/OB&Gyn/04/2016/0101D	CAMERA CONSOLE		KARL STORZ	VISHAL	TRICAM (R) II CCU SCB	YU741138-P				Working	
	SPMCH/OB&Gyn/04/2016/0101E	Camera Head		KARL STORZ	VISHAL	TRICAM 2 Chip	XU858378-H				Working	
	SPMCH/OB&Gyn/04/2016/0101F	Monitor		SONY	VISHAL	LMD-2110MD	3206140				Working	
102	SPWMC/ Ob&Gyn /04/2016/ 0102	**Diagnostic Laparoscopy set**	**Gynaec OT**	**Karl Storz Germany**	**Vishal**			3 Y	05.04.2016	APMSIDC	Working	28,84,350
	SPWMC/ Ob&Gyn /04/2016/ 0102A	HOPKINS Telescope 30' 10mm, 31cm					121FR6				Working	
	SPWMC/ Ob&Gyn /04/2016/ 0102B	Electronic CO2 Endoflator SCB Set		KARL STORZ	VISHAL	26430520	NT34313				Working	
	SPWMC/ Ob&Gyn /04/2016/ 0102C	Light Source		KARL STORZ	VISHAL	LED Nova 150	OT4440				Working	
	SPWMC/ Ob&Gyn /04/2016/ 0102D	CAMERA CONSOLE		KARL STORZ	VISHAL	TRICAM SL II	YU741141-P				Working	
	SPWMC/ Ob&Gyn /04/2016/ 0102E	Camera Head		KARL STORZ	VISHAL	TRICAM 2 Chip	XU858379-H				Working	
		Monitor		SONY	VISHAL	LMD 2110MD	3206142				Working	
103	SPMCH/ Ob&Gyn /04/2016/ 0103	**Diagnostic Laparoscopy set**	**Gynaec OT**	**Karl Storz Germany**	**Vishal**			3 Y	05.04.2016	APMSIDC	Working	28,84,350
	SPMCH/ Ob&Gyn /04/2016/ 0103A	HOPKINS Telescope 30' 10mm, 31cm					121FRB				Working	
	SPMCH/ Ob&Gyn /04/2016/ 0103B	Electronic CO2 Endoflator SCB Set		KARL STORZ	VISHAL	26430520	NT34306				Working	
	SPMCH/ Ob&Gyn /04/2016/ 0103C	Light Source		KARL STORZ	VISHAL	LED NOVA 150	OT4431				Working	
	SPMCH/ Ob&Gyn /04/2016/ 0103D	Camera console		KARL STORZ	VISHAL	TRICAM SLII	YU741137-P				Working	
	SPMCH/ Ob&Gyn /04/2016/ 0103E	Camera Head		KARL STORZ	VISHAL	TRICAM 2 Chip	XU858808-H				Working	

104	SPMCH/ Ob&Gyn /04/2016/ 0104	Hystroscope set - 1 No.	Gynaec OT	Karl Storz Germany	Vishal			3 Y	05.04.2016	APMSIDC	Working	17,48,250
	SPMCH/ Ob&Gyn /04/2016/ 0104A	HOPKINS II TELESCOPE 30 4mm Sl.No.1205Z3									Working	
	SPMCH/ Ob&Gyn /04/2016/ 0104B	HAMOU ENDOMAT SCB Sl.No. NT14214									Working	
	SPMCH/ Ob&Gyn /04/2016/ 0104C	One Pedal Footswitch, One Stage Sl.No. A01G2S									Working	
	SPMCH/ Ob&Gyn /04/2016/ 0104D	Electronic CO2 Endoflator SCB Sl.No.NT34307									Working	
105	SPMCH/ Ob&Gyn /04/2016/ 0105	Defibrillator	Maternity	Nihon Kohden	Biomed Healthcare	TEC-5521	10259	3 Y	21.04.2016	APMSIDC	Working	
106	SPMCH/ Ob&Gyn /05/2016/ 0106A	Ultrasound Color Doppler System	Obstetrics (Gynaecology)	Esaote India	Esaote India	**Mylab 40**	40-13587	3 Y	03.05.2016	SVIMS	Working	15,49,400
	SPMCH/ Ob&Gyn /05/2016/ 0106B	a. 19"LCD Monitor		Esaote India	Esaote India		21799095					
	SPMCH/ Ob&Gyn /05/2016/ 0106C	b. B/B Convex Probe (2-7 MHz)		Esaote India	Esaote India	CA 541	7280					
	SPMCH/ Ob&Gyn /05/2016/ 0106D	c. B/B Endocavity Probe (3-9 MHz)		Esaote India	Esaote India	EC1123	16045005					
	SPMCH/ Ob&Gyn /05/2016/ 0106E	d. B/W Thermal Printer		SONY	Esaote India	UP898MD						
	SPMCH/ Ob&Gyn /05/2016/ 0106F	e. 1 KVA Online UPS		BPE	Esaote India							
	SPMCH/ Ob&Gyn /05/2016/ 0106G	f. B/W Laser Printer		CANON	Esaote India	LBP2900						
	SPMCH/ Ob&Gyn /05/2016/ 0106H	g. 100 CDS & 100 DVDS										
	SPMCH/ Ob&Gyn /05/2016/ 0106I	h. Standard Accessories										
107	SPMCH/ Ob&Gyn /05/2016/ 0107A	Portable Premium Color Doppler System	Obstetrics (Gynaecology)	Esaote India	Esaote India	**Mylab 25 GOLD**	8536	5 Y	13.06.2016	SVIMS	Working	19,00,000

	SPMCH/ Ob&Gyn /05/2016/ 0107B	a. Convex Probe		Esaote India	Esaote India	CA431	15590					
	SPMCH/ Ob&Gyn /05/2016/ 0107C	b. Endocavity Probe		Esaote India	Esaote India	EC1123	16085060					
	SPMCH/ Ob&Gyn /05/2016/ 0107D	c. Biopsy Attachment for Convex probe		Civico								
	SPMCH/ Ob&Gyn /05/2016/ 0107E	d. Biopsy attachement for Endocavity probe		Civico								
	SPMCH/ Ob&Gyn /05/2016/ 0107F	e. Trolley		Esaote India		145930108						
	SPMCH/ Ob&Gyn /05/2016/ 0107G	f. Battery Set										
	SPMCH/ Ob&Gyn /05/2016/ 0107H	g. B/W Thermal Printer		SONY		UPX898 MD	7034236					
	SPMCH/ Ob&Gyn /05/2016/ 0107I	h. 1 KVA Online UPS		DELTA								
	SPMCH/ Ob&Gyn /05/2016/ 0107J	i. Computer with colour laser printer		HP		HP disktop						
	SPMCH/ Ob&Gyn /05/2016/ 0107K	j. Image management software standard Accessories		SONO								
108	SPMCH/NICU /06/2016/ 0108	Infant Warmers with bassinets	Paediatrics	Phoenix Medical	Phoenix Medical	NWS 102	2,213	1 Y	18.06.2016	SVIMS	Working	55,000
109	SPMCH/NICU /06/2016/ 0109	Infant Warmers with bassinets	Paediatrics	Phoenix Medical	Phoenix Medical	NWS 102	2214	1 Y	18.06.2016	SVIMS	**Working**	55,000
110	SPMCH/NICU /06/2016/ 0110	Infant Warmers with bassinets	Paediatrics	Phoenix Medical	Phoenix Medical	NWS 102	2215	1 Y	18.06.2016	SVIMS	**Working**	55,000
111	SPMCH/NICU /06/2016/ 0111	Phototherapy Unit	Paediatrics	Phoenix Medical	Phoenix Medical	Brilliance	3034	1 Y	18.06.2016	SVIMS	Working	64,000
112	SPMCH/NICU /06/2016/ 0112	Phototherapy Unit	Paediatrics	Phoenix Medical	Phoenix Medical	Brilliance	3035	1 Y	18.06.2016	SVIMS	Working	64,000
113	SPMCH/NICU /06/2016/ 0113	Phototherapy Unit	Paediatrics	Phoenix Medical	Phoenix Medical	Brilliance	3036	1 Y	18.06.2016	SVIMS	Working	64,000
		TB & Respiratory										

114	SPMCH/TB & CD /10/2016/ 0114	Spirometer	TB & CD	NDD	JK Medical	Easy on PC	227258	1Y	13/10/2016	SVIMS	Working	**Rs1,88,372**
115	SPMCH/Ophtha/01/2018/ 0115	Coagulator	Ophthalmology	Appa samy	Appa samy	AAOM Advent FS9		2Y	20.01.2018	SVIMS	Working	**Rs 5,60,000/-**
116	SPMCH/Ophtha/05/2017/ 0116	A Scan	Ophthalmology	Appa samy	Appa samy						Working	
117	SPMCH/Ophtha/05/2017/ 0117	OT Table	Ophthalmology	Appa samy	Appa samy		3101170133				Working	
118	SPMCH/Ophtha/05/2017/ 0118	Operating Microscope	ENT	Carl Zeiss		S100/OPMI 1-FC	6627501964		26.09.2016	SVIMS	Working	
119	SPMCH/ Ob&Gyn /00/0000/ 0119	OT Lights Dual Dome	OBG	Martin	Na	Na					Working	
120	SPMCH/ Ob&Gyn /00/0000/ 0120	Surgical diathermy	OBG	Martin	Vishal	Maximum	ME402M				Working	
121	SPMCH/ E N T /00/0000/ 0121	Suction Apparatus	ENT OP	Sisco	Sisco	Venky	15231				Working	
122	SPMCH/ Ob&Gyn /00/0000/ 0122	Suction Apparatus	OBG	Dolpin		Dolpin	145				Working	
123	SPMCH/ Ob&Gyn /00/0000/ 0123	Suction Apparatus	OBG				141				Working	
124	SPMCH/ Ob&Gyn /00/0000/ 0124	Suction Apparatus	OBG				139				Working	
125	SPMCH/ Ob&Gyn /00/0000/ 0125	Suction Apparatus	OBG				143				Working	
126	SPMCH/ Ob&Gyn /00/0000/ 0126	Suction Apparatus	OBG				142				Working	
127	SPMCH/ Ob&Gyn /00/0000/ 0127	Suction Apparatus	OBG				140				Working	
128	SPMCH/Dermat/00/0000/0128	Radio surgery Unit	Dermatology op	Mega Surg Gold			4190				Working	
129	SPMCH/PaeOPD/00/0000/0129	Weighing machine	Paediatrics opd	DS-415N	Essae		G41516545756				Working	
130	SPMCH/Physci/03/2015/0130	ECT Machine	NC	physcitry	Niviqure meditech	Niviqure meditech	VR-ECT,B3-EEG		31.032015	SVIMS	Working	
131	SPMCH/dental /08/2014/0131	Dental Unit	NC	Dental	confident dental	Mookambika Dental Unit			26.06.2014		Working	
132	SPMCH/ Ob&Gyn /00/0000/ 0132	surgical diathermy	OBG	Dolpin	Dolphin	Smart plus4					Working	

133	SPMCH/ Ob&Gyn /00/0000/ 0133	surgical diathermy	OBG	Dolpin	Dolphin	Smart plus4					Working	
134	SPMCH/ Ob&Gyn /00/0000/ 0134	surgical diathermy	OBG	Dolpin	Dolphin	Smart plus 4					Working	
135	SPMCH/ Ob&Gyn /00/0000/ 0135	surgical diathermy	OBG	Dolpin	Dolphin	Smart plus4					Working	
136	SPMCH/ Ob&Gyn /00/0000/ 0136	surgical diathermy	OBG	Dolpin	Dolphin	Smart plus4					Working	
137	SPMCH/ Ob&Gyn /00/0000/ 0137	surgical diathermy	OBG	Dolpin	Dolphin	Smart plus 4					Working	
138	SPMCH/ E N T /00/0000/ 0138	Micro motor drill	ENT	Saeyang		Marathon 3	1836715					
139	SPMCH/ Ob&Gyn /11/2019/ 0139	ECG Machine	GE	Wipro GE		MAC 2000	STD 19440040 PA	1Y	21/11/2019	SVIMS	Working	
140	SPMCH/ N I C U /01/2020/ 0140	Syringe Pump	NICU	Smith Medical	M M Medical	Grase By C9	18320 2900	5 Y	06.01.2020	SVIMS	Working	
141	SPMCH/ N I C U /01/2020/ 0141	Syringe Pump	NICU	Smith Medical	M M Medical	Grase By C9	18320 2945	5 Y	06.01.2020	SVIMS	Working	
142	SPMCH/ N I C U /01/2020/ 0142	Syringe Pump	NICU	Smith Medical	M M Medical	Grase By C9	18320 2915	5 Y	06.01.2020	SVIMS	Working	
143	SPMCH/ N I C U /01/2020/ 0143	Syringe Pump	NICU	Smith Medical	M M Medical	Grase By C9	18320 2905	5 Y	06.01.2020	SVIMS	Working	
144	SPMCH/ N I C U /01/2020/ 0144	Syringe Pump	NICU	Smith Medical	M M Medical	Grase By C9	18320 2916	5 Y	06.01.2020	SVIMS	Working	
145	SPMCH/ N I C U /02/2020/ 0145	Infusion Pump	NICU	Mindray	Green Apple	Benevion VPI	SK-90605752	5 Y	12.02.2020	SVIMS	Working	

PATIENT MOBILITY SERVICES –SVIMSOPD & SVIMS Clinic
Wheel chairs and Trolley status as on 31-01-2021

SRI VENKATESWARA INSTITUTE OF MEDICAL SCIENCES;; TIRUPATI
PATIENT MOBILITY SERVICE- SVIMS OPD, SVIMS CLINICS & COLLEGE OF PHYSIOTHERAPY

1	Total Number of **Wheel chairs**	**15**
2	Number of Functioning Wheel chairs	**6**
3	Number of non Functioning Wheel chairs	**9**
4	Percentage of Functioning wheel chairs	**40**

1	Total Number of **Patient Trolleys**	**11**
2	Number of Functioning Patient Trolleys	**7**
3	Number of non Functioning Patient Trolleys	**4**
4	Percentage of Functioning Patient Trolleys	**63**

PATIENT MOBILITY SERVICE- SVIMS SPECIALITY WARDS &
GENERAL WARDS,

1	Total Number of **Wheel chairs**	**54**
2	Number of Functioning Wheel chairs	**35**
3	Number of non Functioning Wheel chairs	**19**
4	Percentage of Functioning wheel chairs	**64**

1	Total Number of **Patient Trolleys**	**70**
2	Number of Functioning Patient Trolleys	**55**
3	Number of non Functioning Patient Trolleys	**15**
4	Percentage of Functioning Patient Trolleys	**78**

PATIENT MOBILITY SERVICE- SVIMS OT COMPLEX

1	Total Number of **Wheel chairs**	**8**
2	Number of Functioning Wheel chairs	**6**
3	Number of non Functioning Wheel chairs	**2**
4	Percentage of Functioning wheel chairs	**75**

1	Total Number of **Patient Trolleys**	**26**
2	Number of Functioning Patient Trolleys	**19**
3	Number of non Functioning Patient Trolleys	**7**
4	Percentage of Functioning Patient Trolleys	**73**

PATIENT MOBILITY SERVICE- SVIMS STORES, SANITORY, LAUNDRY

1	Total Number of **SHIFTING TROLLEYS**	**12**
2	Number of Functioning **SHIFTING TROLLEYS**	**8**
3	Number of non Functioning **SHIFTING TROLLEYS**	**4**
4	Percentage of Functioning **SHIFTING TROLLEYS**	**66**

PATIENT MOBILITY SERVICE- SPMCW OP & OT

1	Total Number of **Wheel chairs**	**4**
2	Number of Functioning Wheel chairs	**2**
3	Number of non Functioning Wheel chairs	**2**
4	Percentage of Functioning wheel chairs	**50**

1	Total Number of **Patient Trolleys**	**4**
2	Number of Functioning Patient Trolleys	**2**
3	Number of non Functioning Patient Trolleys	**2**
4	Percentage of Functioning Patient Trolleys	**50**

Healthcare Associated Infections (HAI)

About 5% - 10% of patients admitted to hospitals acquire one or more infections, as per the data reported from developed countries. In the USA, it is reported that 1 out of every 136 hospital patients becomes seriously ill as a result of acquiring an infection in the hospital. It is estimated that in developing countries (including India) the risk of Healthcare Associated Infections (HAI) is 2 to 20 times higher than in developed countries. In India, indiscriminate use of antibiotics both in community settings and in hospital settings contributes to development of antibiotic resistance. Further there is need for robust reporting of HAI in India. This ‘double-edged-sword’ of indiscriminate antibiotic use and lack of reporting of healthcare associated infections needs to be addressed. The Director-cum-Vice Chancellor of SVIMS **Dr. B. Vengamma** announced that SVIMS is taking a step forward to contribute in containing HAI in India. Adapting international guidelines (eg WHO, CDC) SVIMS is invoking a ten pronged strategy. One key component is ‘Antimicrobial Stewardship’, which aims to optimize antibiotic use among patients in order to reduce antibiotic resistance, improve patient outcomes and safety and ensure cost effective therapy. Hon’ble Health Minister of Andhra Pradesh, released the first edition of “SVIMS Antimicrobial Stewardship pocket guide” on 12.07.2016. This is revised 6 monthly and new editions are released every January and July to inform all health care personnel (doctors, nurses, and allied health staff) of pathogen surveillance, antimicrobial use, infection control measures and outcomes. This programme is jointly monitored by Hospital Infection Control Committee and SVIMS Quality Council.

CONTENTS

1. Ten Pronged Strategy

2. Hospital Infection Control (HIC) Committees

3. HIC Terms of Reference

4. Hand Hygiene

5. Outcomes & KPIs for Infection

   i) VAP
   ii) CLABSI
   iii) CAUTI
   iv) SSI
   v) Standardized infection ratio (SIR)
   vi) Hand Hygiene Compliance
   vii) Needle Stick Injury Incidence

6. Antimicrobial Stewardship Hand Pocket Guide 10th Edition

1) Healthcare Associated Infections (HAI): SVIMS Ten Pronged Strategy

	Strategy	Implementation
1	• Reducing Inappropriate Device usage	Education by SQC
2	• Hand hygiene and Barrier precaution	HICC, SQC group
2	• Antimicrobial stewardship	Release pocket guide on 12.07.2016
4	• Leadership support at highest level	Director involvement Engineering AP Heath Ministry
5	• Implementing culture of safety	SQC launch
6	• Financial incentives & regulatory oversight	Consideration by AP Health Ministry
7	• System based appropriate protocol and checklist	Ongoing development
8	• Better care of technology	BME monitoring
9	• Public reporting of credible data	Launch 12.07.2016
10	• Partnership	Explore with CDC, WHO

SQC = SVIMS Quality Council

HICC = Hospital Infection Control Committee

BME = Biomedical Engineering

CDC = Center for Disease Control and Prevention

WHO = World Health Organization

2) Hospital Infection Control (HIC) Committees

HIC Committee Members:

- HICC Chairman – Dr B. Vengamma, Director cum Vice Chancellor
  HICC Co-Chairman
- Dr. Ram, Medical Superintendent
- Member Secretary- Dr K.V. Sreedhar Babu, HOD i/c of Microbiology
- Hospital Infection Control Officers-Dr.R.Jayaprada, Dr.N.Ramakrishna, Dr S. Yamini
- Senior Consultant- Dr A. Mohan, Senior professor& HOD of Medicine-
  Member All the heads of the departments- Members
- Nursing AD- Mrs T. Prabhavathi
- Nursing Superintendent Grade I- Mrs.C.Sunitha-Member
- Infection Control Nurses- V.Karpugam, D.Redemma, A.Shobharani & all 47 Head nurses-Members
- Infection Control technicians: Mr P.Yashodhar, Mr V. Venkatesh
- Operating theatre Incharge- Mrs Munilakshmi- Member
- In-charge of Central Sterile Supplies Department- Mrs. T. Prabhavathi-Member
- Health inspector – Mrs. A.Umamaheswari-Member
- In-charge of pharmacy- Dr. P.Subramanyam-Member In-charge of
  hospital linen- Mrs. C.Sunitha-Member
- In-charge of hospital laundry- D.Indiramma-Member
- In-charge of hospital kitchen- Mrs M.Sunitha, Mrs Geetha-Member
- Epidemiologist- Dr V. Chandrasekhar, Assistant professor, Social &
  Preventive medicine-Member

3) HIC Terms of Reference

1. **Health care associated infections**

   i) Ventilator Associate Pneumonia (VAP)
   ii) Central Line Associated Blood Stream Infections (CLABSI)
   iii) Catheter Associated Urinary Tract Infections (CAUTI)
   iv) Surgical Site Infections (SSI)
   v) Standardized infection ratio (SIR)
   vi) Needle stick injury incidence
   vii) Hand hygiene compliance

2. Bed sore analysis
3. O.T. surveillance (Monthly)
4. Blood bank surveillance
5. Environmental surveillance (water& air) (Monthly)
6. Hand hygiene
7. Dialysate fluid testing
8. Needle-stick injuries incidence
9. Multi drug-resistant organisms (MDRO's) Surveillance
10. Outbreak investigation
11. Biomedical waste management
12. High end antibiotic monitoring
13. AMR surveillance
14. HBs Ag antibody titre testing
15. Endotoxin (LAL) assay for Dialysate fluid & water
16. Disinfectant testing-new and in-house
17. Stool for *Clostridium difficile* toxin A&B testing
18. Blood contamination rate
19. *Legionella* spp screening in humidifier water from ACs.
20. Audits: Bundle care audits for VAP, CLABSI, CAUTI and SSI, Hand hygiene audit, PPE audit, Biomedical waste audits

4) Hand Hygiene

- The organization adheres to standard precautions at all times regarding the use of PPE, prevention of sharp injury etc.

- Hand Hygiene guidelines are followed in all areas of the hospital-Posters regarding Hand Hygiene are available.

- Specific precautions are being followed when required. Safe Injection and Infusion practices are followed.

- Cleaning, disinfection and sterilization practices being followed

Steps of Procedure Hand Hygiene – Hand Rub (20-30 secs)

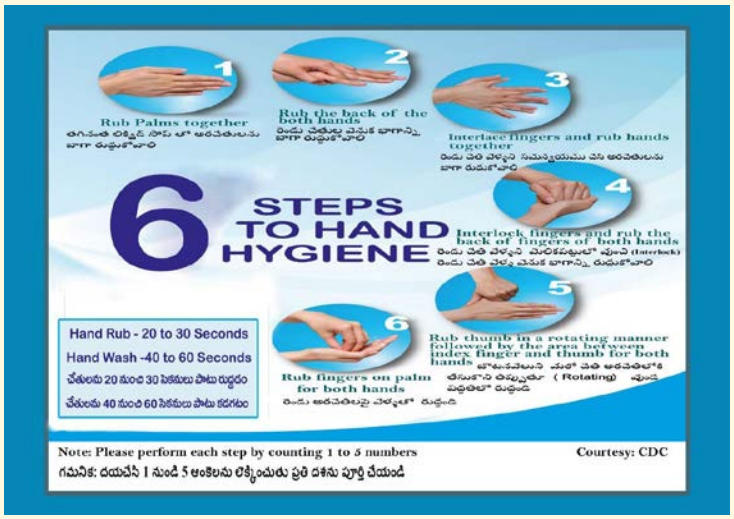

Surgical Hand Wash (3-5mts)

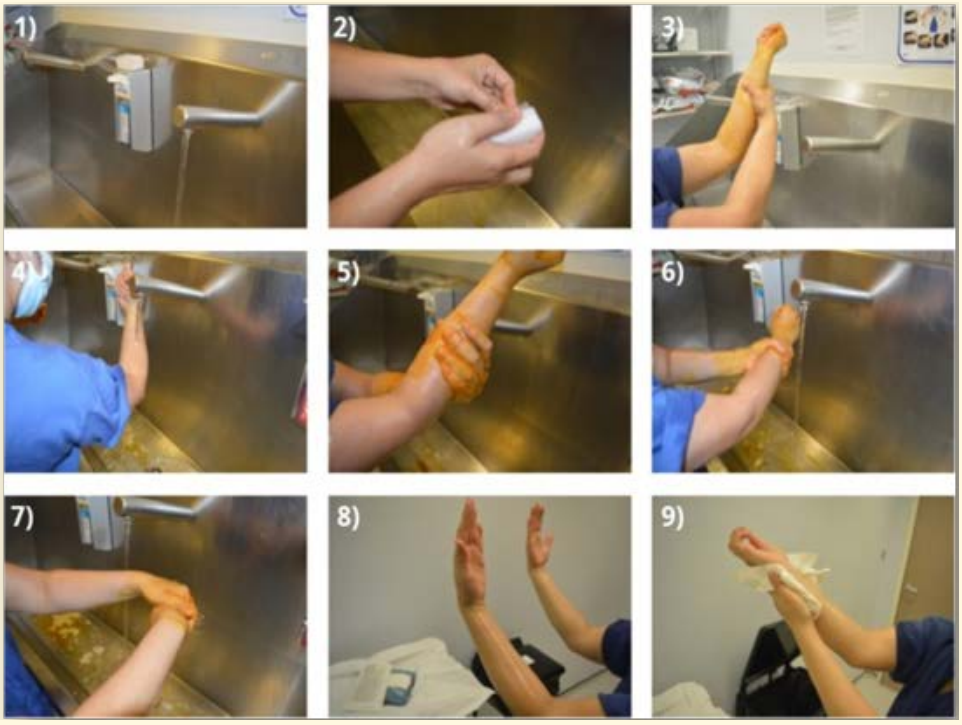

Greeting each other in Health care

Another dimension
in Hand Hygiene!

Spread Goodwill, not Germs

Prevent droplet spread
when coughing, sneezing

Director cum Vice-Chancellor

Sri Venkateswara Institute of
Medical Sciences, Tirupati.

5) Outcomes & KPIs for Infections

i) Control chart for VAP from Jan to Dec 2020

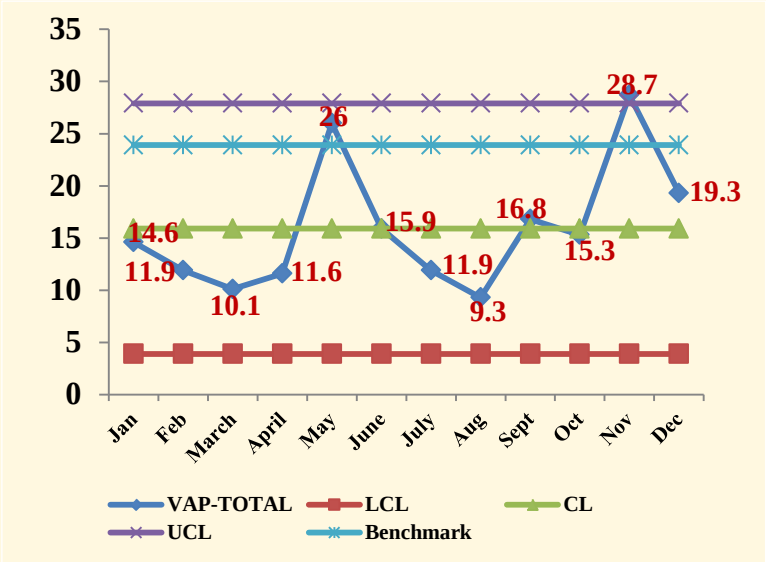

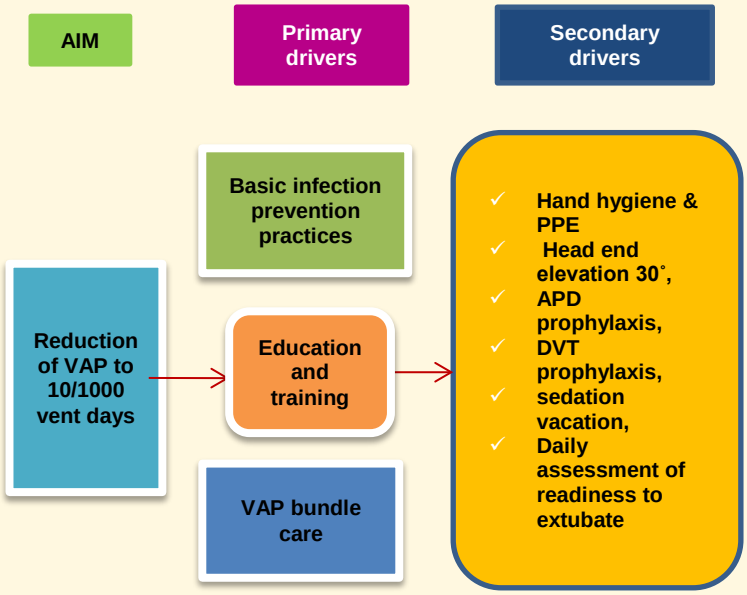

ii) Control chart for CAUTI from Jan to Dec 2020

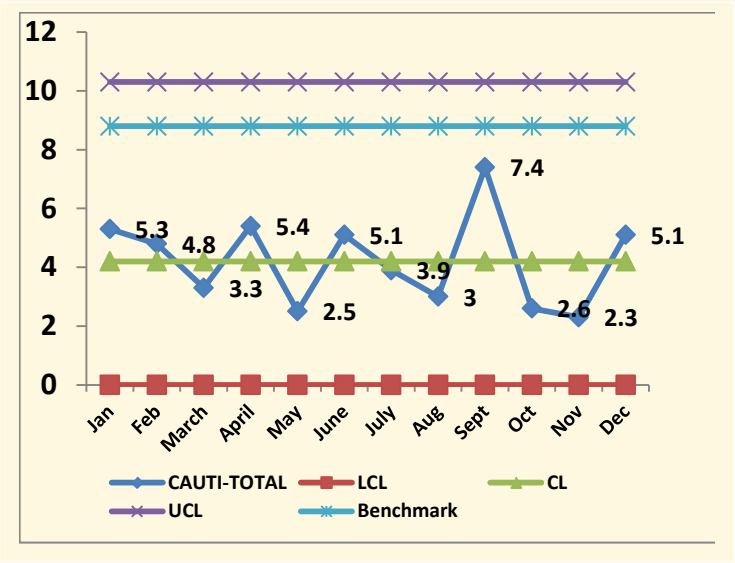

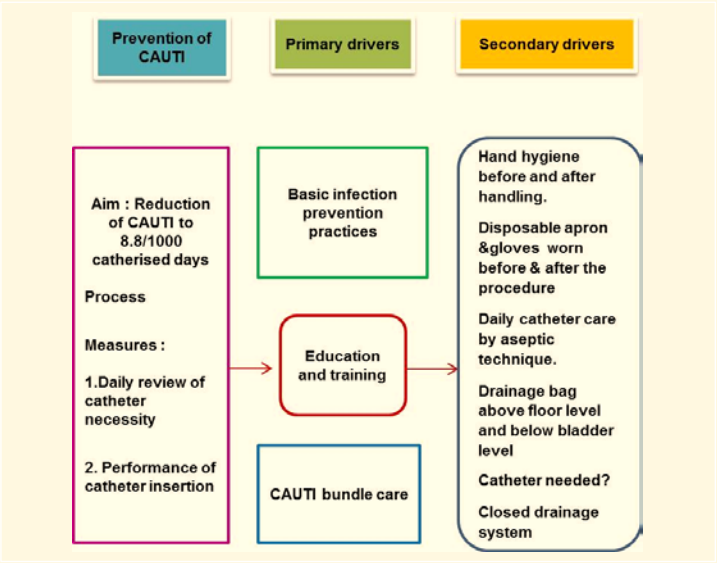

iii) Control chart for CLABSI from Jan to Dec 2020

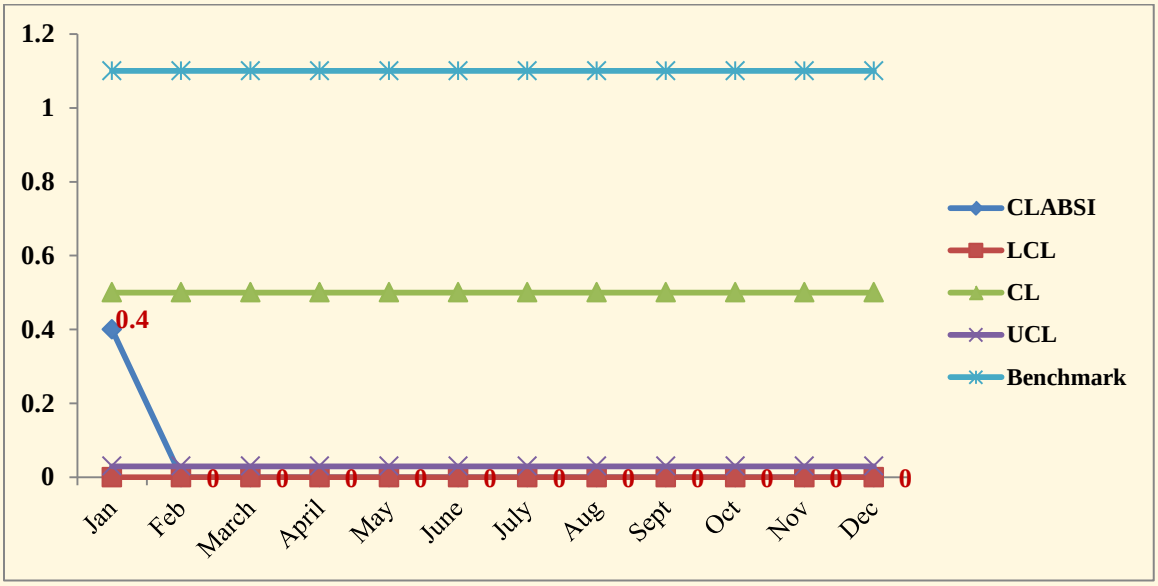

Driver diagram for CLABSI

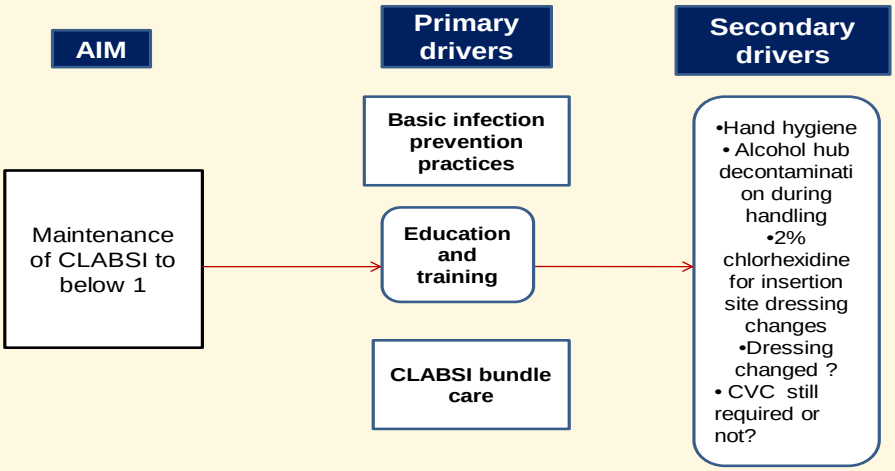

iv) Trends of SURGICAL SITE INFECTION (SSI) from Jan to Dec 2020

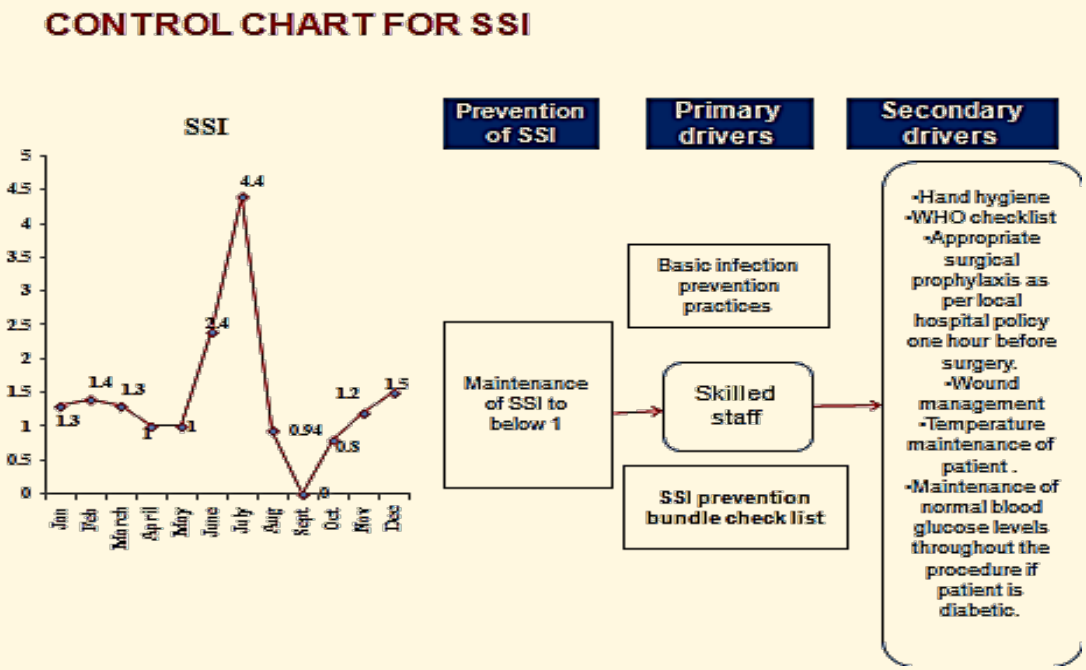

v) STANDARDIZED INFECTION RATIO (SIR) from Jan to Dec-2020

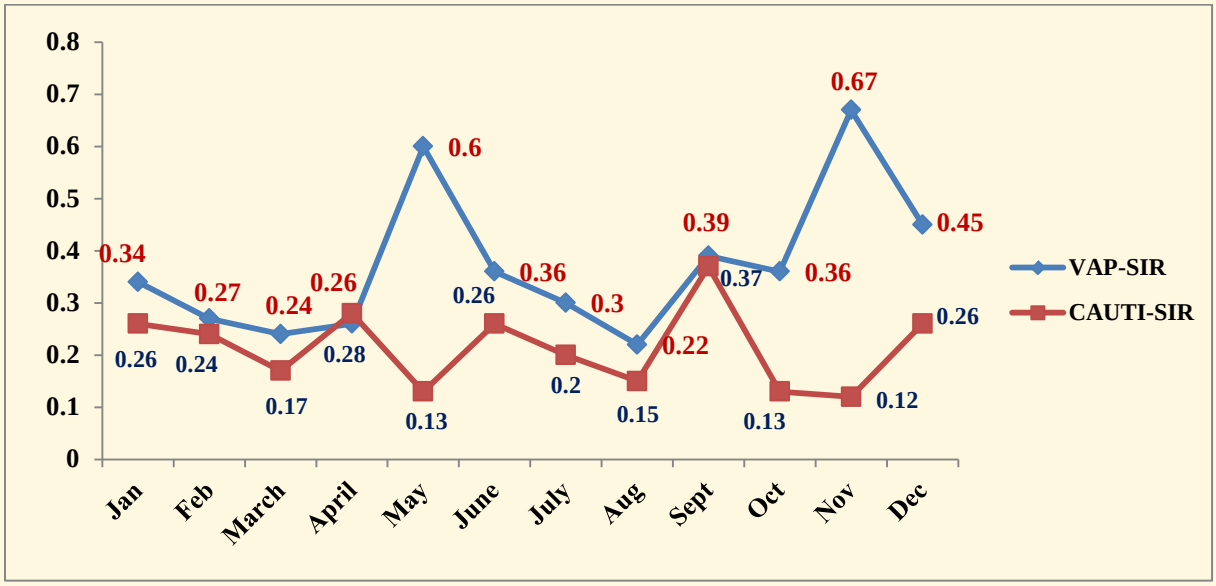

vi) Hand hygiene overall compliance rate from Jan to Dec 2020

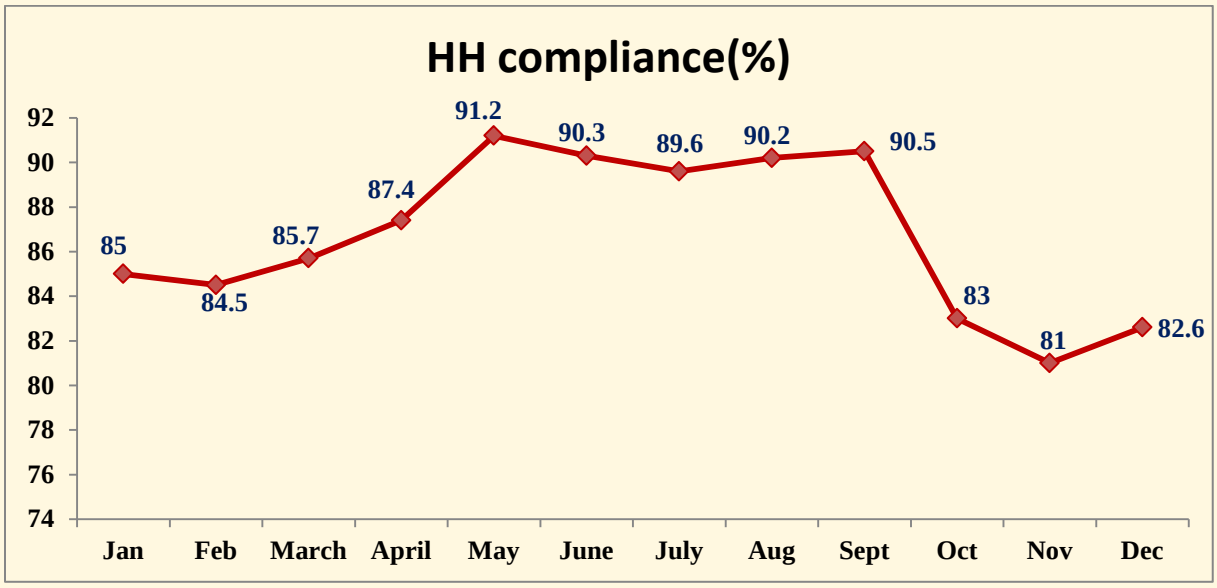

vii) **Needle stick injury incidences (NSI) from Jan to Dec 2020**

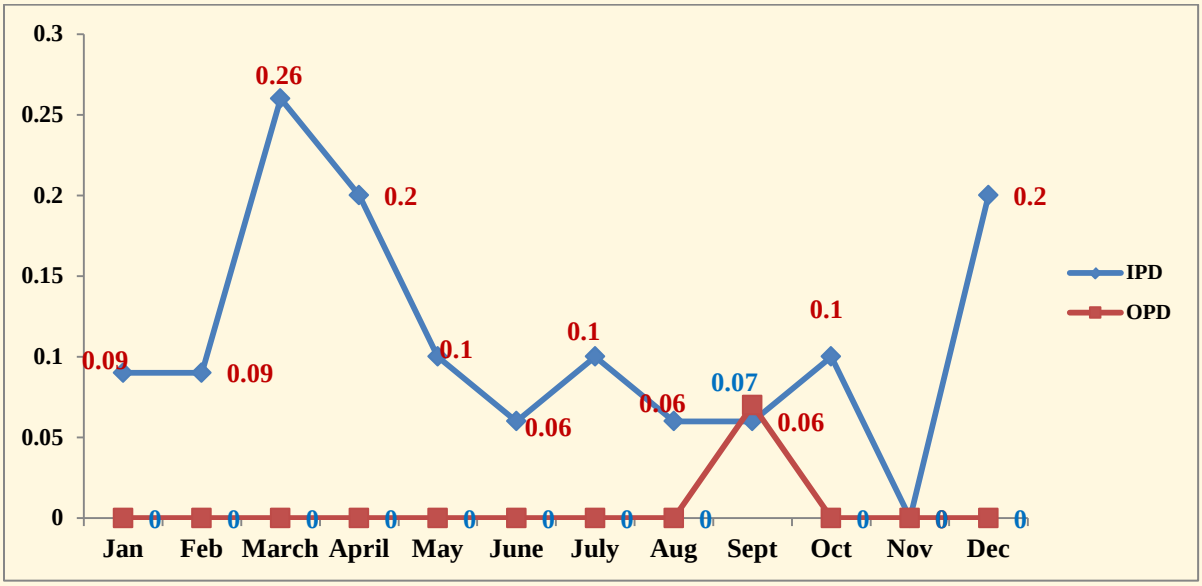

SRI VENKATESWARA INSTITUTE OF MEDICAL SCIENCES, TTD, TIRUPATI

ANTIMICROBIAL STEWARDSHIP POCKET GUIDE

JUL-DEC 2020 (10TH EDITION)

10th Edition

Editors

Dr B.Vengamma, Director-cum-VC

Dr. Ram, Medical Superintendent

Dr K.V.Sreedhar Babu (HOD I/C)

Dr R.Jayaprada, HICO, AMSP Lead

Dr N.Ramakrishna, HICO, AMSP Lead

Preface

Healthcare Associated Infections (HAI)

Dr. B.Vengamma, Director- cum-Vice Chancellor of SVIMS announced that SVIMS is taking a step forward to contribute in containing HAI in India. Adapting international guidelines (e.g. WHO, CDC), SVIMS is invoking a ten pronged strategy. One key component is 'Antimicrobial Stewardship', which aims to optimize antibiotic use among patients in order to reduce antibiotic resistance, improve patient outcomes and safety and ensure cost effective therapy. This will be revised 6 monthly and new editions will be released every January and July to inform all health care personnel (doctors, nurses, and allied health staff) of pathogen surveillance, antimicrobial use, infection control measures and outcomes. This programme is jointly monitored by Anti-Microbial Stewardship Committee Hospital Infection Control Committee and SVIMS Quality Council.

To learn how to use antibiotics, one must first learn how not to use antibiotics." -Unknown

Dr. B.Vengamma
Director cum Vice Chancellor

From the desk of editors……..

Greetings from Anti-Microbial Stewardship Programme & Infection Control team,

- Antimicrobial resistance (AMR) results in increased morbidity, mortality, and costs of healthcare
- Prevention of the emergence of resistance and the dissemination of resistant microorganisms will reduce these adverse effects and their attendant costs.
- Predominant isolates in ICUs were *Klebsiella* followed by *Acinetobacter, Escherichia coli and Pseudomonas spp.*
- In ICUs empirical choice of antibiotic in our institute is Cefoperazone + Sulbactam
- Based on Gram staining report prophylactic drug of choice for Gram negative bacilli is Cefoperazone + Sulbactam, and for Gram positive bacteria is Linezolid in all ICUs.

We therefore here by asseverate everyone to use antimicrobial agents judiciously

R.Jayaprada, N.Ramakrishna, S.Yamini
Infection Prevention & Control Officers,
AMSP Lead

Ram
Medical Superintendent

B.Vengamma
Director-cum-Vice

INDEX

1. Trends of Multidrug Resistance from July 2020 – December 2020
2. Antibiotic policy
3. Biomedical Waste Management
4. Post exposure prophylaxis (PEP)

1. Trends of Multidrug Resistance from July 2020 – December 2020

Key messages.....

- ✓ Prevalence of Multi drug resistance (MDR) from July to December 2020 was – **50.1%**
- ✓ Predominant isolates in intensive care units (ICU) were *Escherichia coli* followed by *Klebsiella spp*, *Acinetobacter spp* and *Pseudomonas spp*. As per our local antibiogram, empirical choice of antibiotic in **ICUs** in our institute is **Cefoperazone+sulbactam.** In case of suspicion of *Pseudomonas spp* infections, empirical choice of antibiotic is Piperacillin+ Tazobactam. Based on Gram staining report, prophylactic drug of choice for Gram negative bacilli is **Cefoperazone+ sulbactam,** and for Gram positive bacteria is **Vancomycin** in all ICUs depending on the department.
- ✓ Percentage of Vancomycin Resistance Enterococci (VRE): 9.5%
- ✓ Percentage of Methicillin resistance *Staphylococcus aureus* (MRSA): 74.7%,
- ✓ Percentage of Methicillin resistance *Coagulase negative Staphylococcus (*MRCoNS):75.7%
- ✓ Percentage of Vancomycin resistance *Staphylococcus aureus* (VRSA): 0.6%
- ✓ Percentage of Vancomycin resistance *Coagulase negative Staphylococcus* (VRCoNS): 1.4%
- ✓ Most common Gram negative isolates were *Escherichia coli, Klebsiella spp, Acinetobacter spp, Pseudomonas spp and Enterobacter spp.*
- ✓ *Escherichia coli* isolates were highly resistant to Cefazolin (90.9%%), Ciprofloxacin(88%), Cotrimoxazole (68.1%) and sensitive to Amikacin (73.7%), Cefoperazone+sulbactam (81.1%), Gentamicin (64.3%), Piperacillin+tazobactum (80.8%), Meropenem (94.9%), Colistin/Polymyxin B (99%) and Tigecycline (99.5%).
- ✓ *Klebsiellae spp.* isolates were highly resistant to Cefazolin (95.9%), Cotrimoxazole (91.9%), Ciprofloxacin (81%), Cefoperazone+sulbactam (54.5%), Amikacin (60.1%), Gentamicin (63.6%), Piperacillin +tazobactam (55%) and sensitive to Meropenem (53.1%), Colistin/Polymyxin B (98.%) and Tigecycline (97%).
- ✓ Acinetobacter spp. isolates were highly resistant to Cefazolin (96.6%), Ciprofloxacin (68.6%), Cotrimoxazole (81.3%), Amikacin (73.7%), Gentamicin (69.4%), Piperacillin +tazobactam (74.5%), Meropenem (73.7%), and sensitive to Cefoperazone+sulbactam (67.8%), Colistin/Polymyxin B (99.2%) and Tigecycline (71.2%).
- ✓ Pseudomonas spp. isolates were highly resistant to Ciprofloxacin (86.9%), Ceftazidime (72.4%), Amikacin (62.3%), Gentamicin (79.7%),and sensitive to Piperacillin + tazobactam (76.9%), Cefoperazone+sulbactam (60.9%), Imipenem (68.2%) and Colistin/Polymyxin B(100%).
- ✓ Most of the Gram negative isolates were shown highly resistant to cephalosporins (86.5%), cotrimoxazole (70.8%), and ciprofloxacin (71.4%).
- ✓ On the other hand, Gram negative isolates were shown sensitivity to cefoperazone+sulbactum (72%), aminoglycosides (58.3%), Meropenem (77.4%), and Polymyxin B (98.1%).
- ✓ Screening of health care workers (HCWs) for Methicillin resistance Staphylococcus aureus (MRSA) should be done as MRSA percentage was 74.7% & Methicillin resistance Coagulase negative Staphylococcus (MRCoNS) percentage was 75.7%, and these isolates were predominantly from Emergency, General Medicine and Nephrology departments. HCWs were treated for the same. As percentage of Methicillin resistance being high, mandate recommendation for HCWs is to follow standard precautions (Hand Hygiene, Contact precautions) strictly at all times of patient

care.

- ✓ Staphylococcus aureus has show high resistance against Ciprofloxacin (82.5%), Erythromycin (68.1%), Clindamycin (48.8%), and Cotrimoxazole (54.2%).
- ✓ VRE (Vancomycin Resistance Enterococci) percentage was 9.5% and most of the isolates were reported from EMD, Nephrology, General Medicine, Urology and Neurology departments.
- ✓ Imipenem resistance was noted high in Acinetobacter spp (73.7%) followed by Pseudomonas spp (68.2%), Klebsiellae spp (53.1%).
- ✓ Among isolated MDR Enterobacteriaceae, 15.1% were Carbapenem resistant Enterobacteriaceae (CRE)

So cautious and judicious prescription of carbapenems is required.

Note : Empirical therapy should be reviewed once the culture and susceptibility results are ready (usually within 72 hours) and targeted therapy should be done whenever possible to give the narrowest spectrum antibiotic based on culture and sensitivity report, the site of infection and the clinical status of the patient.

Fig 1: Resistance patterns to various antimicrobials among *Escherichia coli*

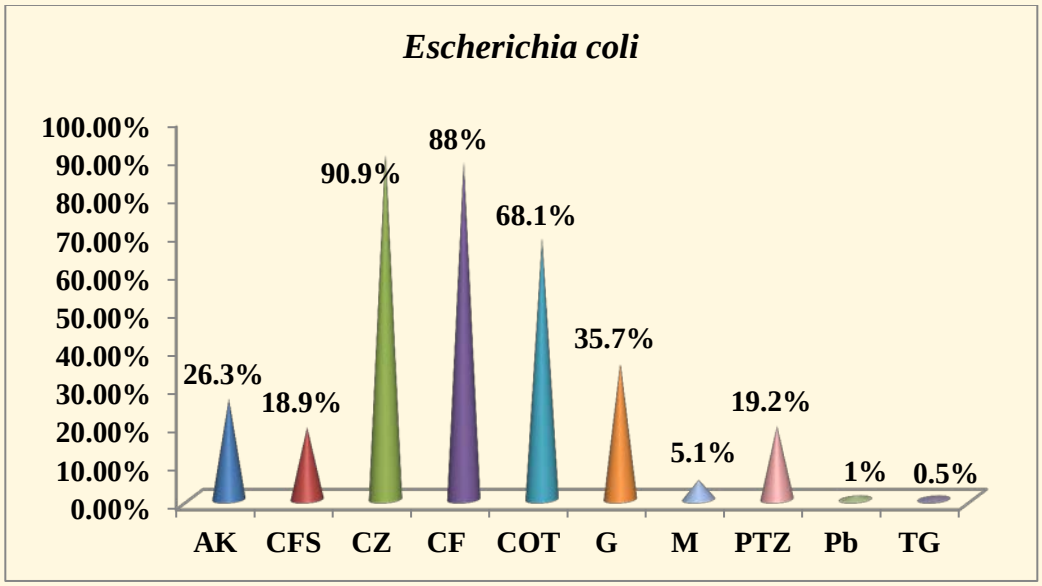

AK- AMIKACIN, CFS-CEFOPERAZONE+SULBACTAM, CZ-CEFAZOLIN, CF-CIPROFLOXACIN, COT-COTRIMOXAZOLE, G-GENTAMICIN, M-MEROPENEM, PTZ-PIPERACILLIN+TAZOBACTAM, Pb-POLYMYXIN-B, TG-TIGECYCLINE

Fig 2: Resistance patterns to various antimicrobials among *Klebsiella spp.*

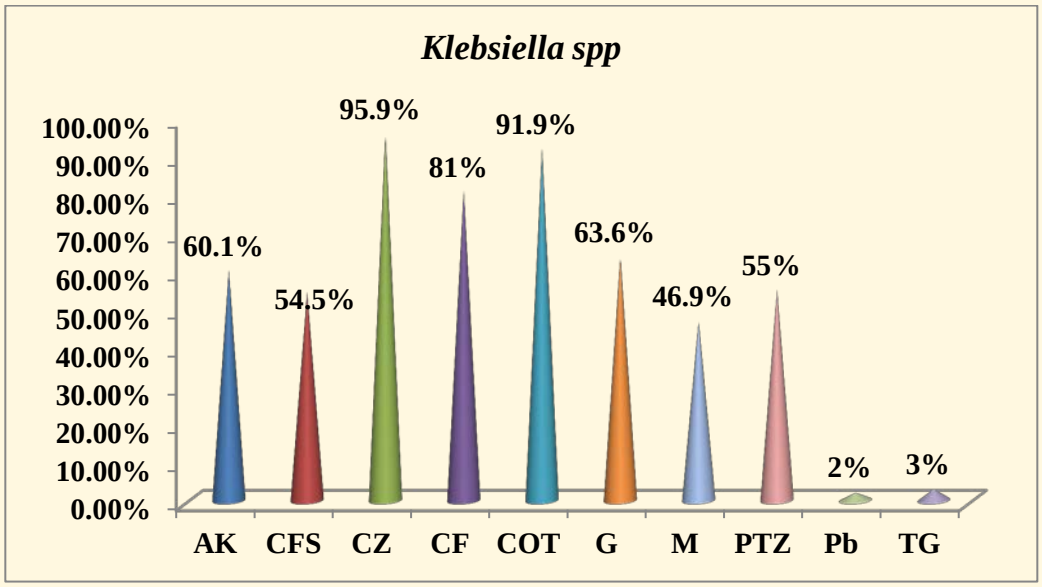

AK- AMIKACIN, CFS-CEFOPERAZONE+SULBACTAM, CZ-CEFAZOLIN, CF-CIPROFLOXACIN, COT-COTRIMOXAZOLE, G-GENTAMICIN, M-MEROPENEM, PTZ-PIPERACILLIN+TAZOBACTAM, Pb-POLYMYXIN-B, TG-TIGECYCLINE

Fig 3: Resistance patterns to various antimicrobials among *Acinetobacter spp*.

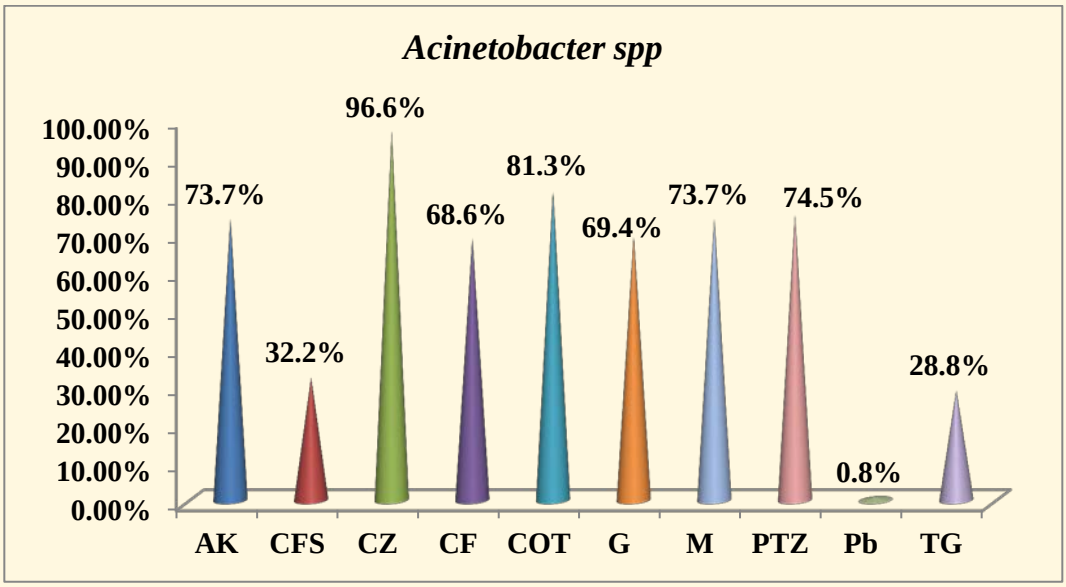

AK- AMIKACIN, CFS-CEFOPERAZONE+SULBACTAM, CZ-CEFAZOLIN, CF-CIPROFLOXACIN, COT-COTRIMOXAZOLE, G-GENTAMICIN, M-MEROPENEM, PTZ-PIPERACILLIN+TAZOBACTAM, Pb-POLYMYXIN-B, TG-TIGECYCLINE

Fig 4: Resistance patterns to various antimicrobials among *Pseudomonas spp.*

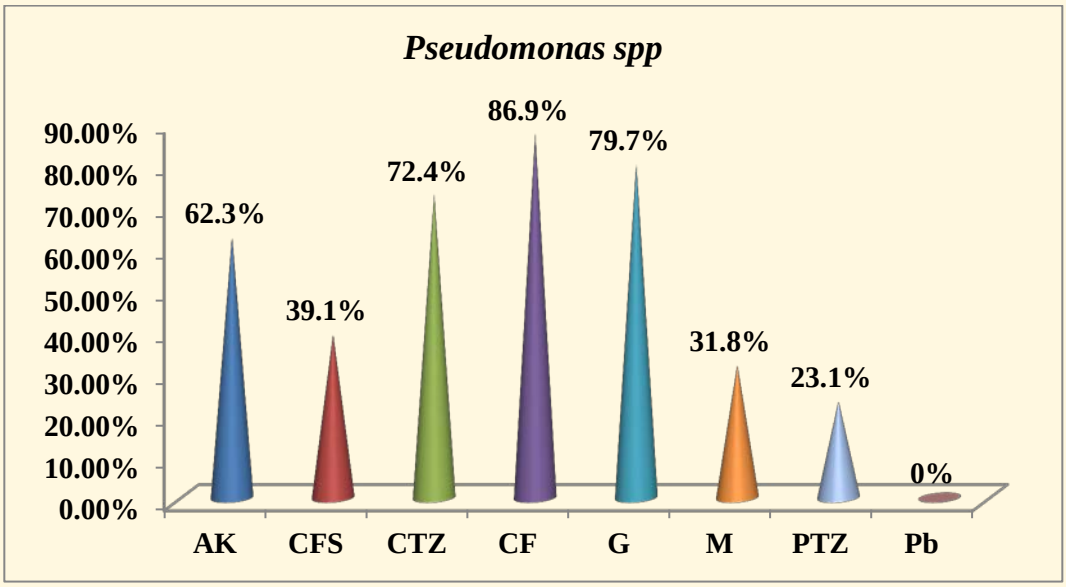

AK- AMIKACIN, CFS-CEFOPERAZONE+SULBACTAM, CZ-CEFAZOLIN, CF-CIPROFLOXACIN, G-GENTAMICIN, M-MEROPENEM, PTZ-PIPERACILLIN+TAZOBACTAM, Pb-POLYMYXIN-B.

Fig 5: Resistance patterns to various antimicrobials among *Enterobacter spp*.

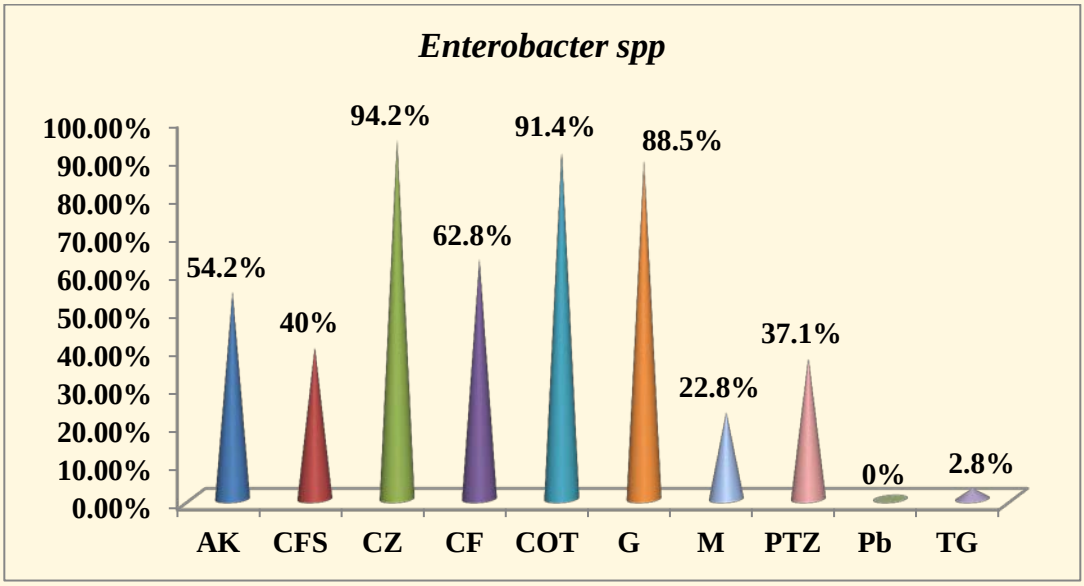

AK- AMIKACIN, CFS-CEFOPERAZONE+SULBACTAM, CZ-CEFAZOLIN, CF-CIPROFLOXACIN, COT-COTRIMOXAZOLE, G-GENTAMICIN, M-MEROPENEM, PTZ-PIPERACILLIN+TAZOBACTAM, Pb-POLYMYXIN-B, TG-TIGECYCLINE

Fig 6: Resistance pattern to various antimicrobials among *Staphylococcus aureus*

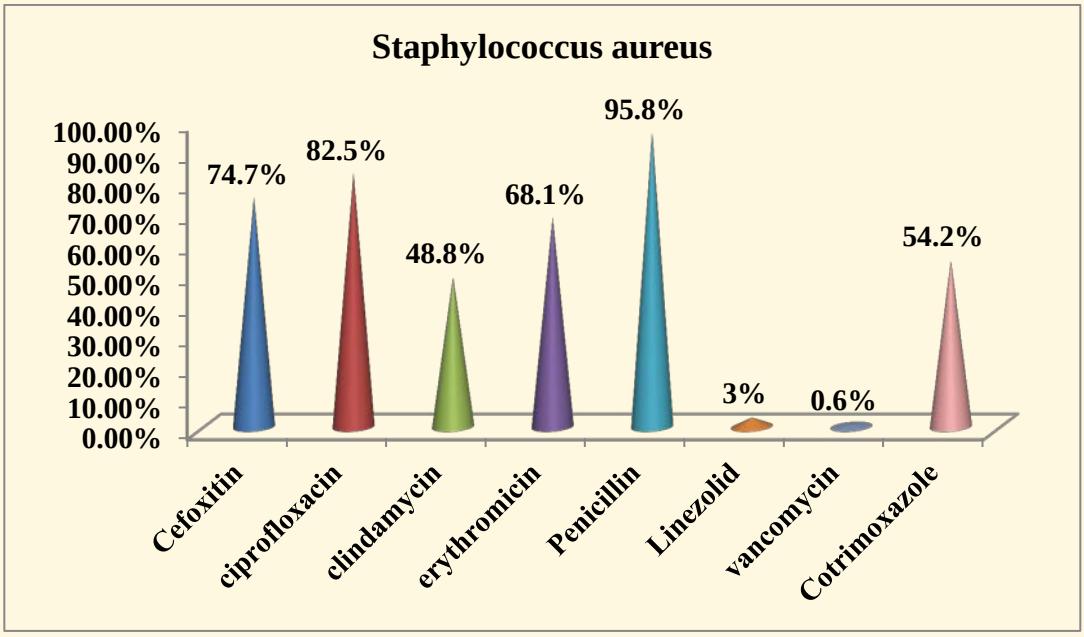

Fig 7: Resistance pattern to various antimicrobials among MRSA isolates

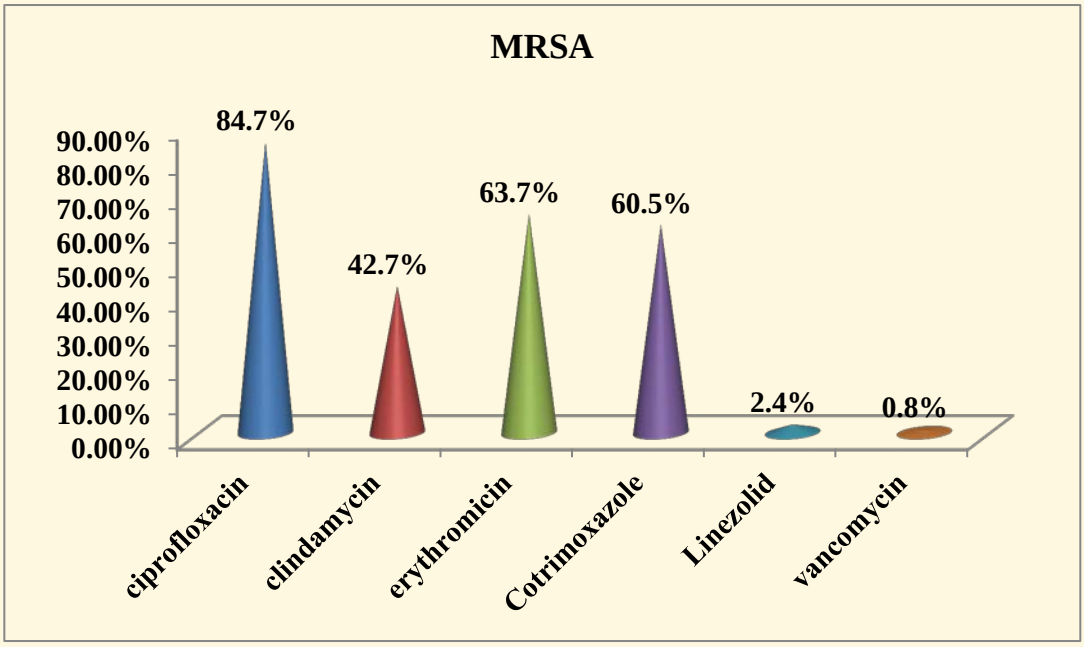

Fig 8: Resistance pattern to various antimicrobials among Coagulase negative *Staphylococcus aureus* (CoNS)

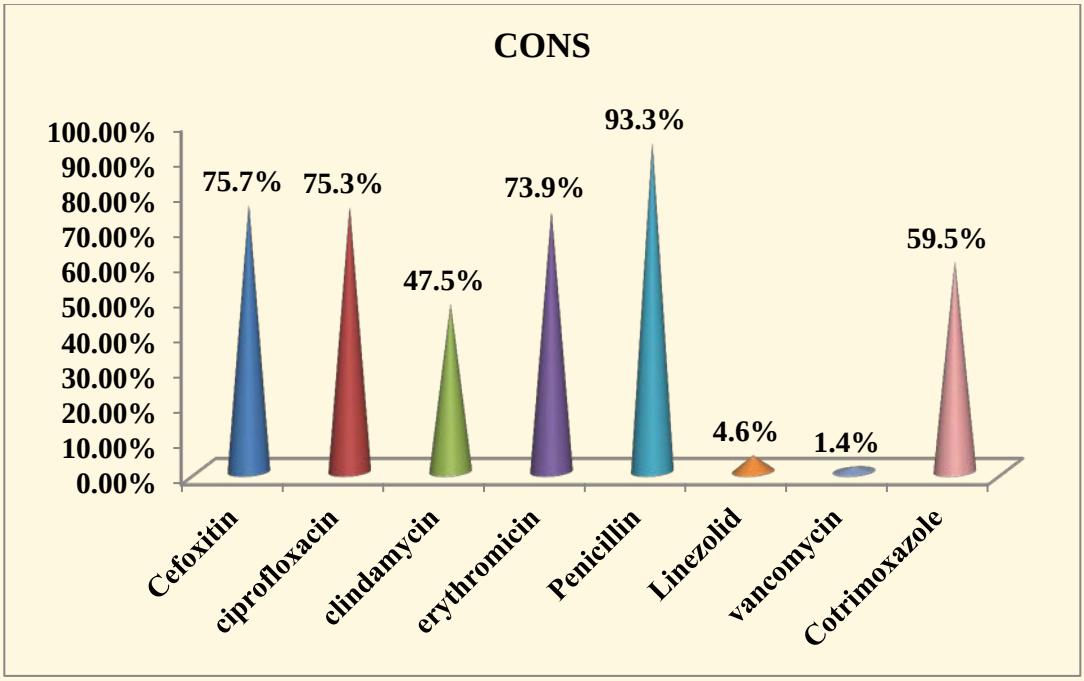

Fig 9: Resistance pattern to various antimicrobials among *Enterococcus spp*

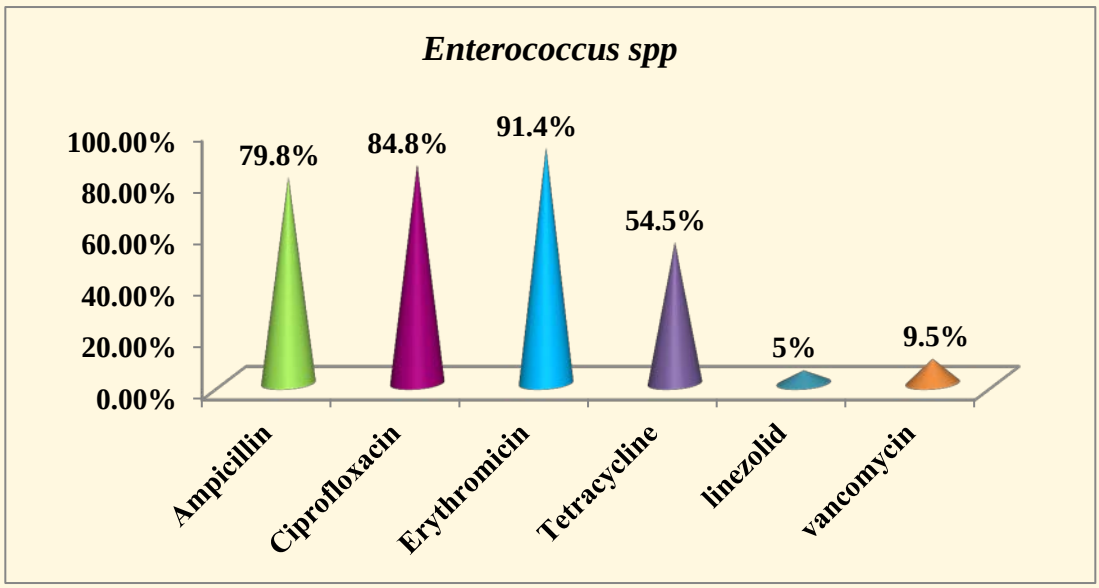

Fig 10: Resistance pattern among Gram positive isolates

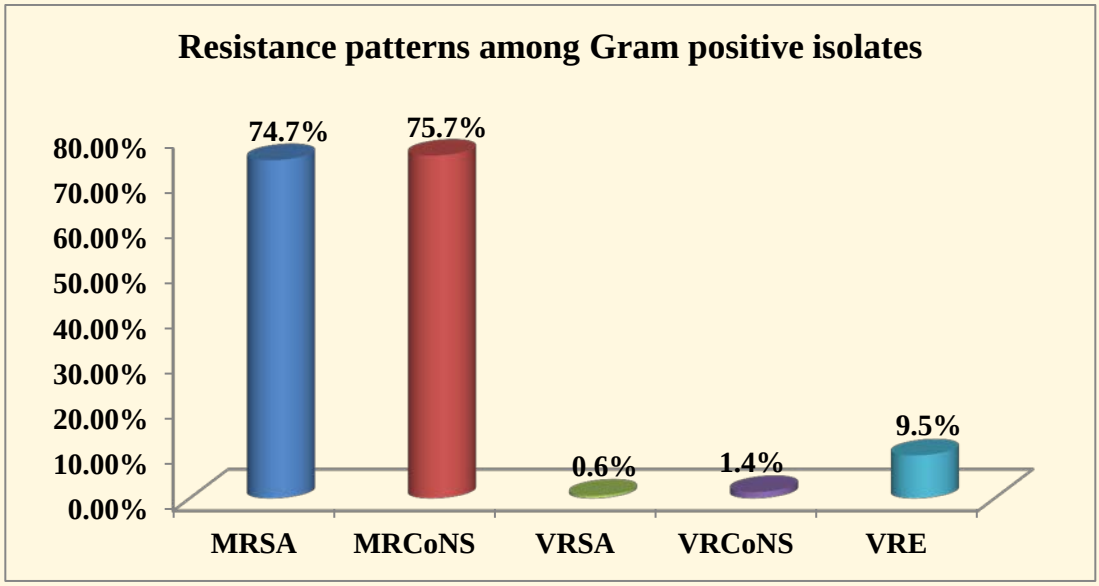

Table 1

Gram negative bacilli distribution and sensitivity pattern among (Multidrug resistance organisms) MDROs

Organism	AK	CFS	CZ	CF	COT	G	M/I	PTZ	Pb	TG
Escherichia coli (n=675)	73.7%	81.1%	9.1%	12%	31.9%	64.3%	94.9%	80.8%	99%	99.5%
Klebsiella spp. (n=198)	39.9%	45.5%	4.1%	19%	8.1%	36.4%	53.1%	45%	98%	97%
Acinetobacter spp. (n=118)	26.3%	67.8%	3.4%	31.4%	18.7%	30.6%	26.3%	25.5%	99.2%	71.2%
Pseudomonas spp. (n=69)	37.7%	60.9%	27.6%	13.1%		20.3%	68.2%	76.9%	100%	
Enterobacter spp. (n=35)	45.8%	60%	5.8%	37.2%	8.6%	11.5%	77.2%	62.9%	100%	97.2%

AK- AMIKACIN, CFS-CEFOPERAZONE+SULBACTAM, CZ-CEFAZOLIN, CF-CIPROFLOXACIN, COT-COTRIMOXAZOLE, G-GENTAMICIN, M-MEROPENEM, PTZ-PIPERACILLIN+TAZOBACTAM, Pb-POLYMYXIN-B, TG-TIGECYCLINE, n-number

MRSA percentage was 74.7% and VRE percentage was 9.6%.

<50% susceptible >80% susceptible

Table 2

Gram negative bacilli distribution and sensitivity pattern among Medical departments

Organism	AK	CFS	CZ	CF	COT	G	M/I	PTZ	Pb	TG
Escherichia coli (n=316)	70.3%	79.5%	8.6%	17.8%	27.5%	59.5%	94%	79.5%	99.7%	100%
Klebsiella spp. (n=70)	37.2%	42.9%	4.3%	41.5%	7.2%	45.8%	52.9%	42.9%	98.6%	95.8%
Acinetobacter spp. (n=34)	29.5%	76.5%	5.9%	41.2%	17.7%	35.3%	41.2%	38.3%	100%	70.6%
Pseudomonas spp. (n=27)	37.1%	63%	33.4%	7.5%		29.7%	63%	81.5%	96.3%	
Enterobacter spp. (n=9)	33.3%	33.3%	0%	44.5%	11.1%	11.1%	77.8%	44.5%	100%	100%

AK- AMIKACIN, CFS-CEFOPERAZONE+SULBACTAM, CZ-CEFAZOLIN, CF-CIPROFLOXACIN, COT-COTRIMOXAZOLE, G-GENTAMICIN, M-MEROPENEM, PTZ-PIPERACILLIN+TAZOBACTAM, Pb-POLYMYXIN-B, TG-TIGECYCLINE, n-number

MRSA percentage was 72.1% and VRE percentage was 13.3%. Percentage of Carbapenem resistance among Gram negative bacterial isolates was 18.9%.

<50% susceptible

>80% susceptible

50-80% susceptible

Table 3

Gram negative bacilli distribution and sensitivity pattern among Surgical departments

Organism	AK	CFS	CZ	CF	COT	G	M/I	PTZ	Pb	TG
Escherichia coli (n=229)	81.7%	86.5%	9.2%	19.3%	36.3%	70.8%	97%	86.1%	98.3%	98.7%
Klebsiella spp. (n=72)	44.5%	51.4%	5.6%	37.5%	9.8%	44.5%	59.8%	52.8%	95.9%	98.7%
Acinetobacter spp. (n=21)	23.9%	52.4%	0%	24%	24%	19.1%	14.3%	0%	100%	71.5%
Pseudomonas spp. (n=17)	53%	58.9%	23.6%	5.9%		23.6%	64.8%	88.3%	100%	
Enterobacter spp. (n=4)	50%	75%	0%	25%	25%	25%	100%	75%	100%	100%

AK- AMIKACIN, CFS-CEFOPERAZONE+SULBACTAM, CZ-CEFAZOLIN, CF-CIPROFLOXACIN, COT-COTRIMOXAZOLE, G-GENTAMICIN, M-MEROPENEM, PTZ-PIPERACILLIN+TAZOBACTAM, Pb-POLYMYXIN-B, TG-TIGECYCLINE, n-number

MRSA percentage was 88.9% and VRE percentage was 3.4%. Percentage of Carbapenem resistance among Gram negative bacterial isolates was 16.7%.

<50% susceptible

>80% susceptible

50-80% susceptible

Table 4

Gram negative bacilli distribution and sensitivity pattern among intensive care units (ICUs)

Organism	AK	CFS	CZ	CF	COT	G	M/I	PTZ	Pb	TG
Escherichia coli (n=26)	57.7%	61.6%	3.9%	38.5%	19.3%	23.9%	84.7%	50%	96.2%	100%
Klebsiella spp. (n=22)	13.7%	13.8%	0%	36.4%	4.6%	13.7%	27.3%	13.7%	100%	91%
Acinetobacter spp. (n=15)	20%	53.4%	0%	40%	26.7%	26.7%	20%	20%	100%	46.7%
Pseudomonas spp. (n=3)	0%	33.3%	33.3%	0%		0%	33.3%	33.3%	100%	
Enterobacter spp. (n=1)	0%	0%	0%	0%	0%	0%	0%	0%	100%	100%

AK- AMIKACIN, CFS-CEFOPERAZONE+SULBACTAM, CZ-CEFAZOLIN, CF-CIPROFLOXACIN, COT-COTRIMOXAZOLE, G-GENTAMICIN, M-MEROPENEM, PTZ-PIPERACILLIN+TAZOBACTAM, Pb-POLYMYXIN-B, TG-TIGECYCLINE, n-number

MRSA percentage was 100% and VRE percentage was 14.3%. Percentage of Carbapenem resistance among Gram negative bacterial isolates was 38.6%

<50% susceptible

>80% susceptible

50-80% susceptible

Table 5

Gram negative bacilli distribution and sensitivity pattern among OPD/OI samples

Organism	AK	CFS	CZ	CF	COT	G	M/I	PTZ	Pb	TG
Escherichia coli (n=72)	70.8%	83.4%	9.8%	25%	38.4%	72.3%	98.7%	84.3%	100%	100%
Klebsiella spp. (n=18)	61.2%	72.3%	0%	50%	5.6%	33.3%	72.3%	72.3%	100%	100%
Acinetobacter spp. (n=30)	36.7%	66.7%	3.3%	40%	10%	43.4%	16.7%	23.3%	96.7%	20%
Pseudomonas spp. (n=8)	50%	50%	25%	62.5%		25%	75.6%	75%	100%	
Enterobacter spp. (n=13)	77%	92.4%	0%	69.3%	0%	7.7%	92.4%	92.4%	100%	100%

AK- AMIKACIN, CFS-CEFOPERAZONE+SULBACTAM, CZ-CEFAZOLIN, CF-CIPROFLOXACIN, COT-COTRIMOXAZOLE, G-GENTAMICIN, M-MEROPENEM, PTZ-PIPERACILLIN+TAZOBACTAM, Pb-POLYMYXIN-B, TG-TIGECYCLINE, n-number

MRSA percentage was 73.8% and VRE percentage was 7.7%. %. Percentage of Carbapenem resistance among Gram negative bacterial isolates was 23.3%

<50% susceptible

>80% susceptible

50-80% susceptible

Table 6

Resistance pattern among various categories of Gram negative bacteria

S.No	Organisms	AK	CFS	CF	PTZ	Pb	TG	COT	M
1	**Enterobacteriaceae (*n*=1012)**	36.3%	26.9%	84%	27.6%	1.8%	1.7%	74.5%	15.1%
2	**CRE (*n*=153)**	83%	81.6%	90.8%	92%	2.6%	6.5%	89.5%	-
4	**Non-fermenters (*n*=210)**	67.1%	33.3%	71.9%	52.3%	1.9%	16.2%	52.8%	56.6%

AK- AMIKACIN, CFS-CEFOPERAZONE+SULBACTAM, CZ-CEFAZOLIN, CF-CIPROFLOXACIN, COT-COTRIMOXAZOLE, G-GENTAMICIN, M-MEROPENEM, PTZ-PIPERACILLIN+TAZOBACTAM, Pb-POLYMYXIN-B, TG-TIGECYCLINE, n-number

Table 7

CRE distribution among wards (*n*=153)

Area of the Hospital	Percentage of CRE
ICUs	16.3%
Surgical	24.8%
Medical	40.5%
OPD/OI	5.9%

Fig 11: Distribution of CRE among various departments

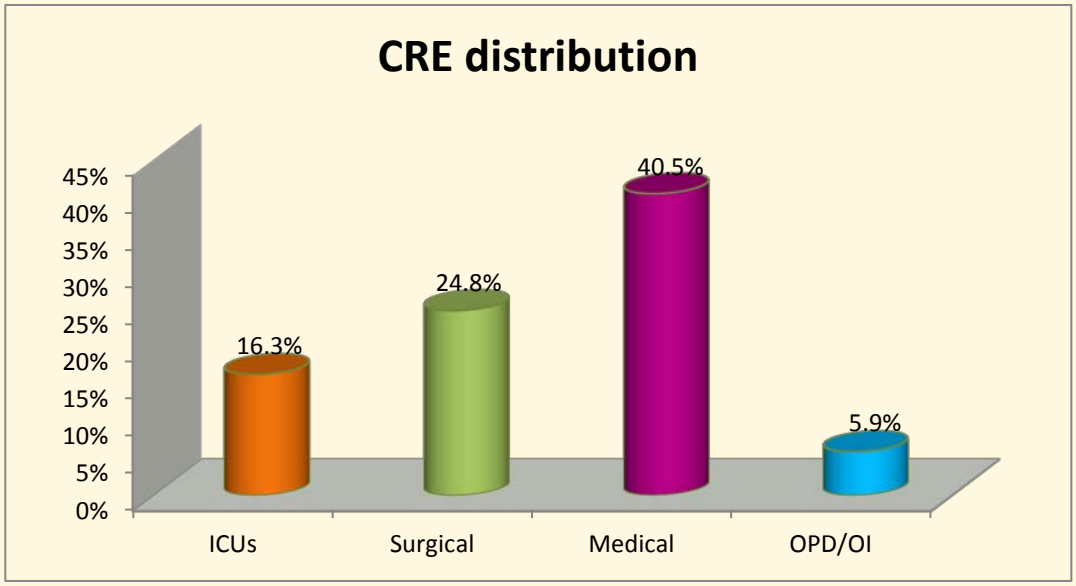

Fig 12: Distribution of various Gram negative bacteria

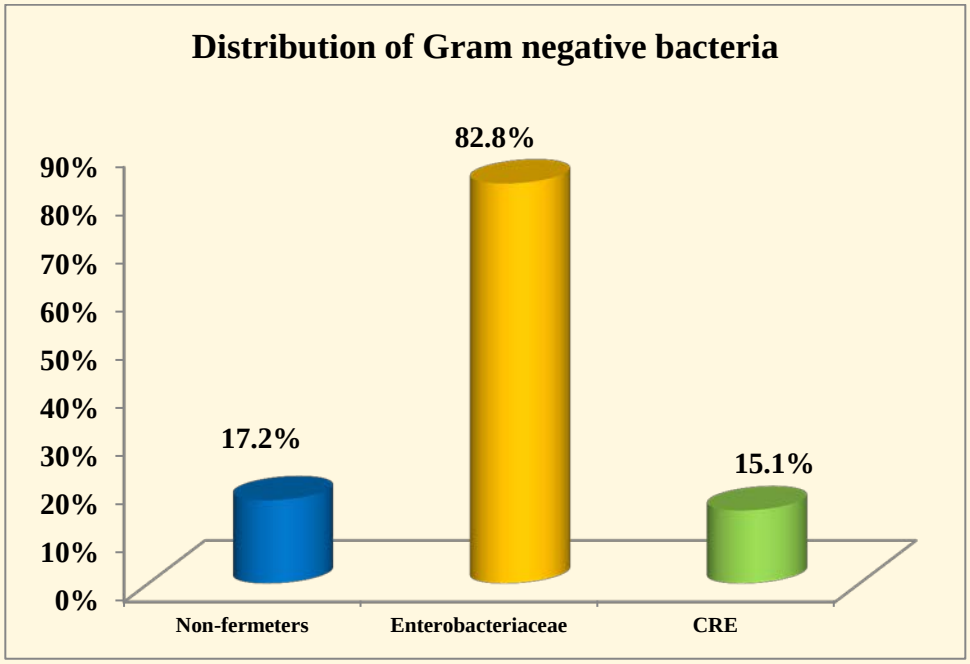

Overall MDR gram negative bacilli isolated were 1222, which includes 17.2% (210) of non-fermenters and 82.8% (1012) enterobacteriaceae. Out of 1012 enterobacteriaceae 15.1% (153) were CRE.

Fig 13: Organism wise distribution of isolates in Intensive care units (ICU)

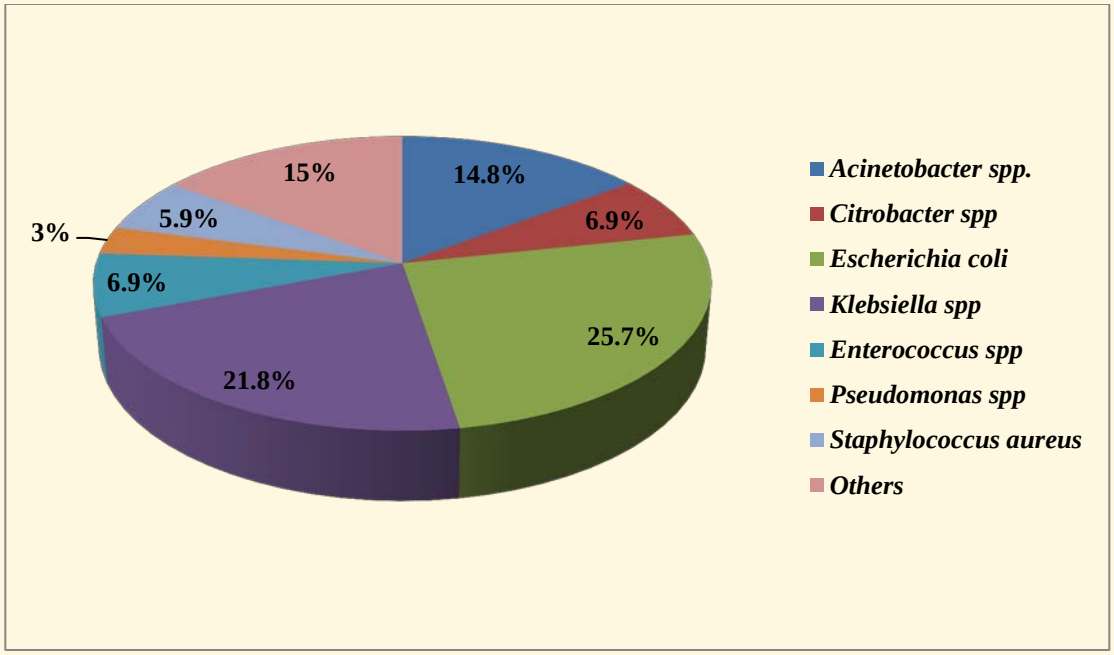

Fig 14: Sample wise distribution of Multi Drug Resistant Organisms (MDROs)

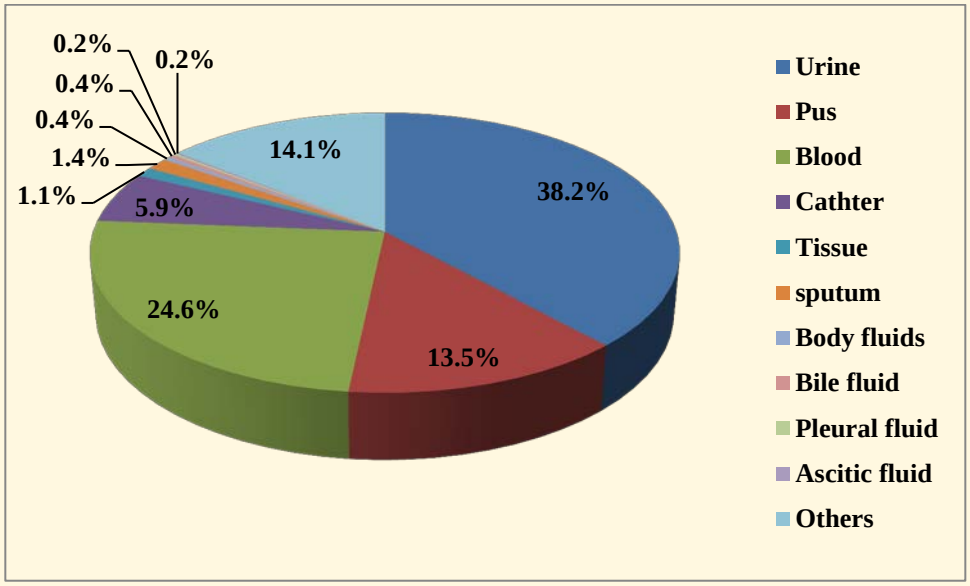

Fig 15: Organism wise distribution of Multi Drug Resistant Gram negative isolates

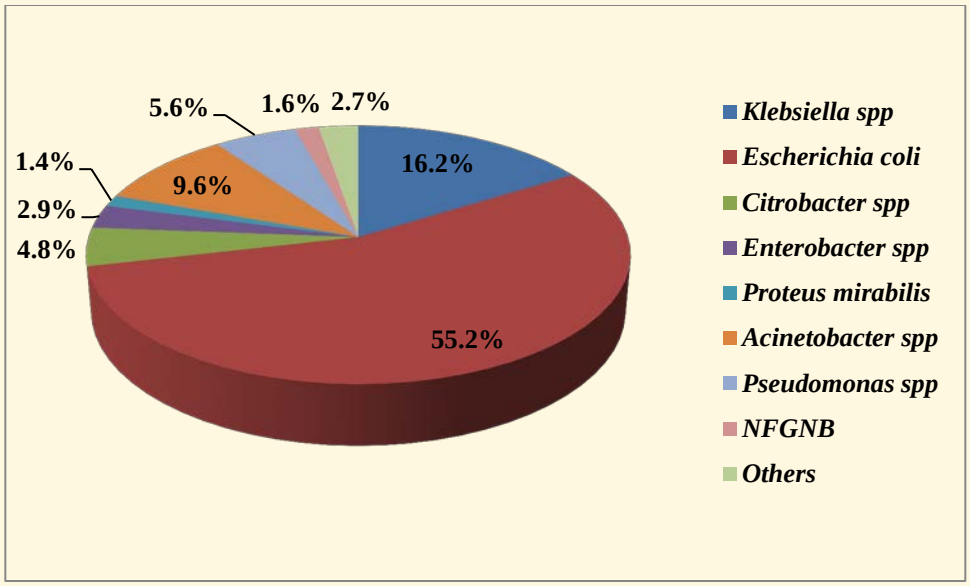

Fig 16: Organism wise distribution of Carbapenem Resistant Enterobacteriaceae (CRE) isolates

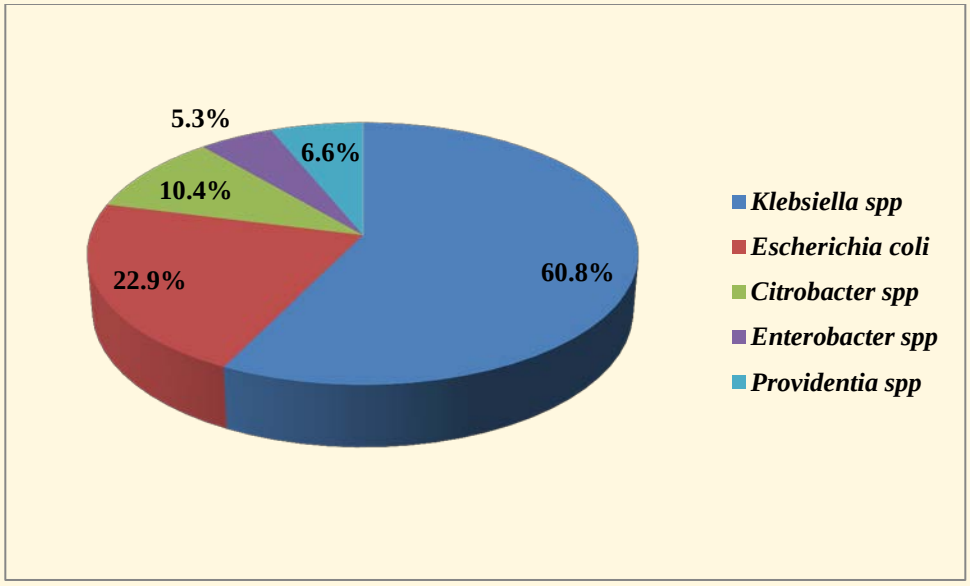

Fig 17: Department wise distribution of Carbapenem Resistant Enterobacteriaceae (CRE) isolates

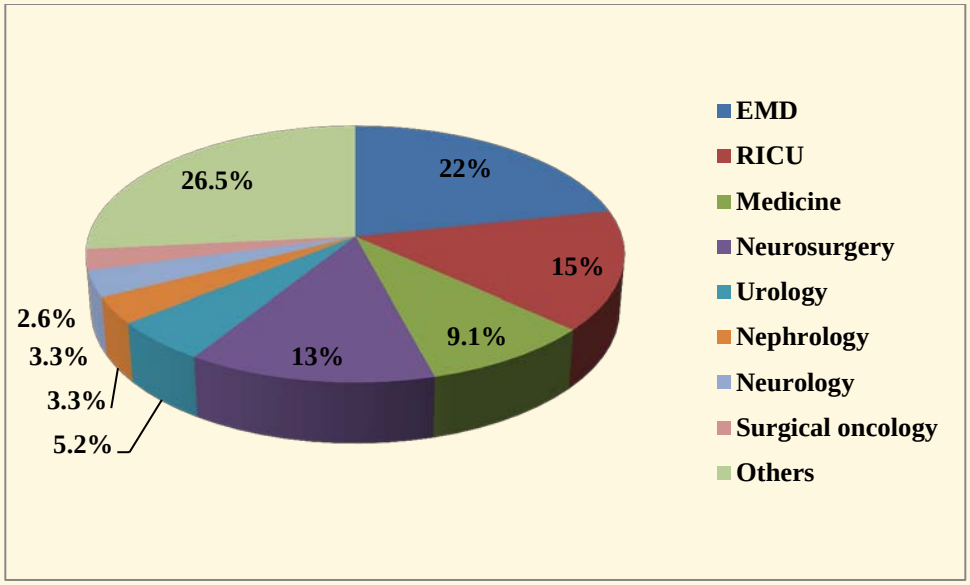

EMD-Emergency department, OPD-Outpatient department, GS-General surgery, RICU-Respiratory intensive care unit.

Fig 18: Department wise distribution of Multi Drug Resistant Organisms (MDROs)

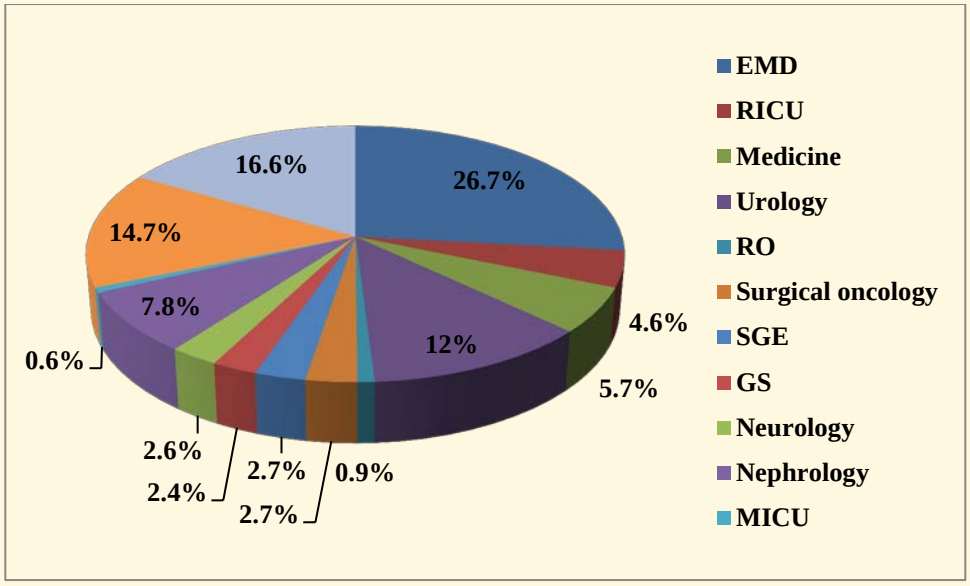

EMD-Emergency department, OPD-Outpatient department, GS-General surgery, RICU-Respiratory intensive care unit, RO-Radiation oncology, SGE-Surgical gastroenterology, MICU-Medical intensive care unit.

Fig 19: Organism wise distribution of Multi Drug Resistant Gram positive isolates

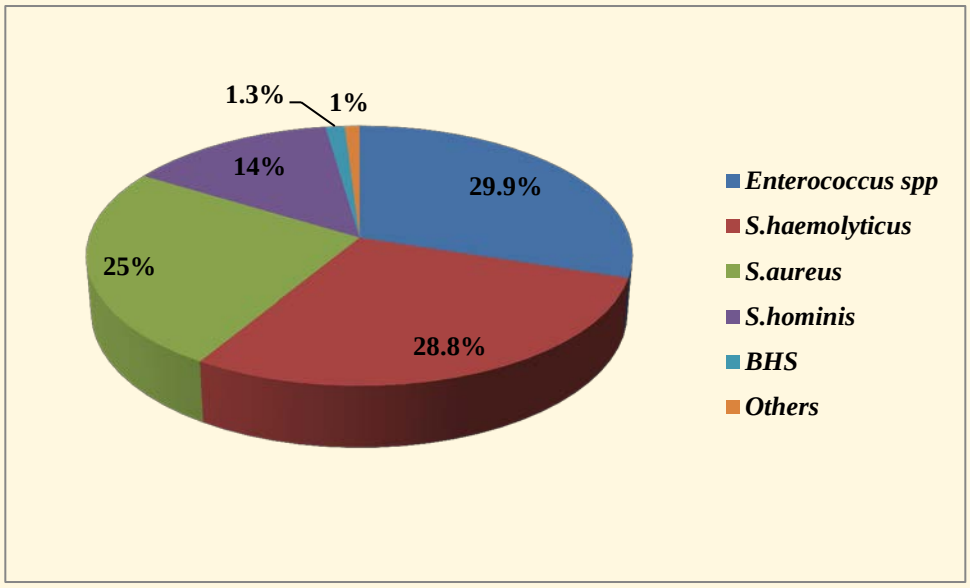

Fig 20: Department wise distribution of

Methicillin Resistant *Staphylococcus aureus* (*MRSA)* in clinical samples

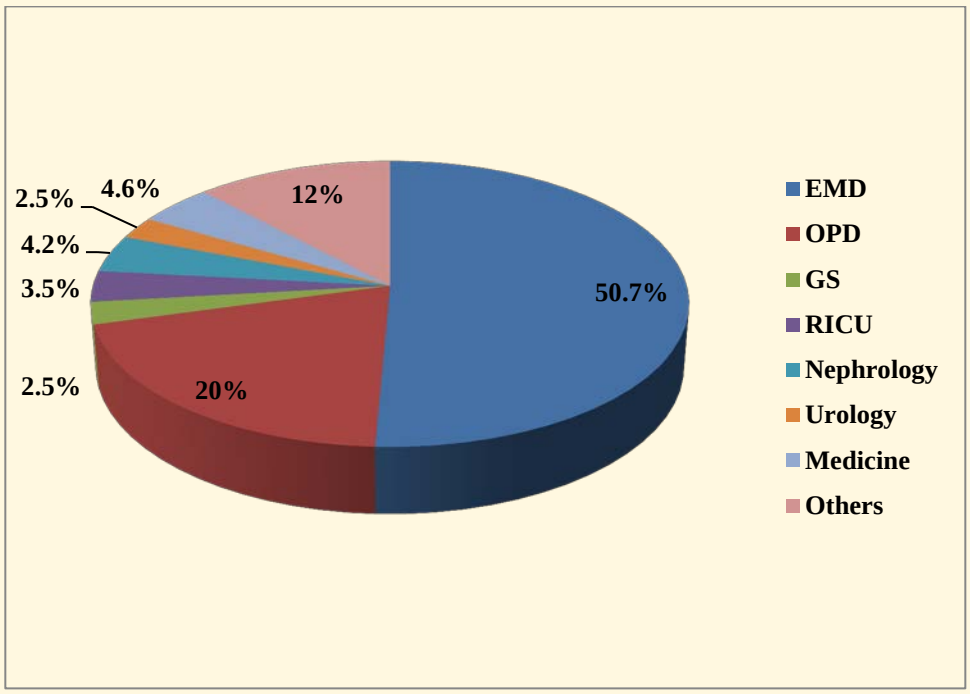

EMD-Emergency department, OPD-Outpatient department, GS-General surgery, RICU-Respiratory intensive care unit

2. Antibiotic policy

Antimicrobial policy should be implemented through the Antimicrobial stewardship committee or Hospital infection control committee.

- Antibiotic use must be justifiable on the basis of the clinical diagnosis and known or expecting micro-organisms.
- Appropriate specimens for bacteriological examination must be obtained before initiating antibiotic treatment, in order to confirm the treatment is appropriate.
- The selection of antibiotic must be based not only on the nature of the disease and that of the pathogenic agents, but on the sensitivity patterns, patient tolerance, and cost.

Selection based on

- Based on the spectrum of the antibiotic taking into account possible resistant patterns.
- Use the correct dose, route and duration.
- Ensure chosen antibiotic has adequate tissue penetration at the site of infection.
- Optimize PK-PD parameters according to co-morbidities

De-escalation/modification

a. Modify empiric broad spectrum antibiotics depending on culture and antimicrobial susceptibility reports and patient status
b. Stop polymyxins and glycopeptides if no carbapenem resistant organisms (CRO) or methicillin resistant *Staphylococcus aureus*(MRSA) identified on cultures
c. Avoid double or redundant gram negative or anaerobic coverage
d. Discontinue antibiotics if a non-infectious mimic identified
e. De-escalate combination therapy to a single agent
f. Change a broad spectrum antibiotic to a narrow spectrum one
g. Change IV to oral antibiotics
h. De-escalation is safe in all patients including febrile neutropenia and septic shock and reduces mortality and length of hospital stay.

- The physician should receive timely, relevant information of the prevalence of resistance in the facility.
- An agent with as narrow a spectrum as possible should be used.
- Antibiotic combinations should be avoided, if possible,
- Selected antibiotics may be restricted in use (like vancomycin, linezolid, Carbapenems etc..)
- The correct dose must be used (low doses may be ineffective for treating infections, and encourage the development of resistance, while excessive doses may have adverse effects, and may not prevent resistance)

Flow diagram for known MRSA positive patients

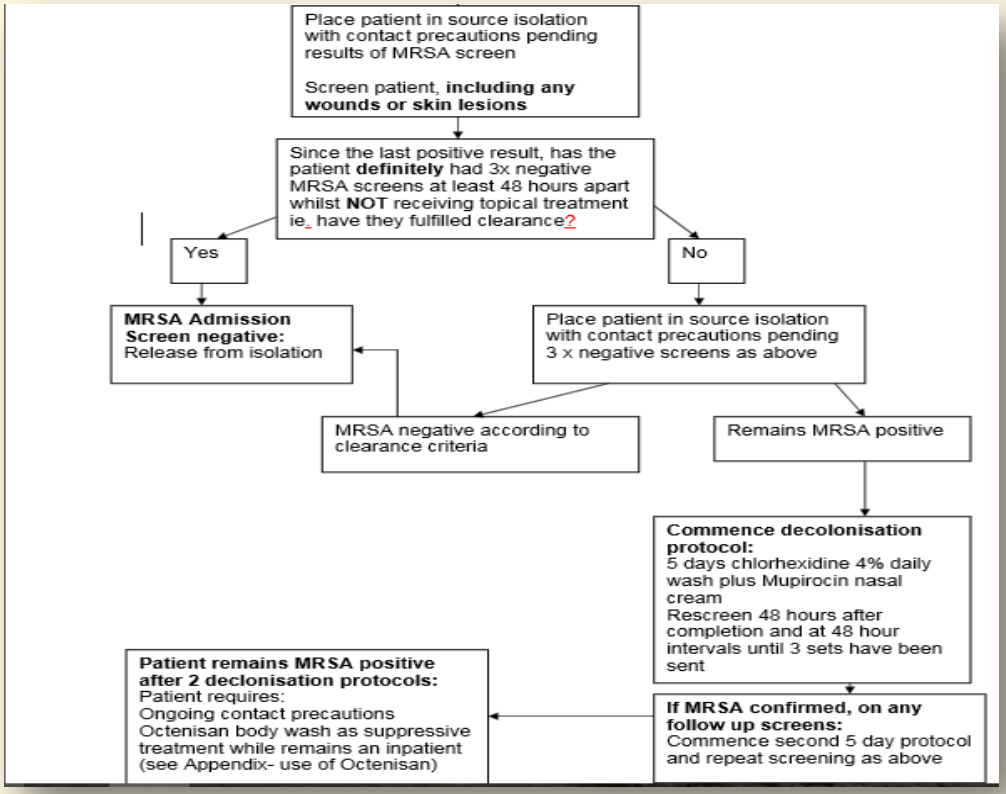

Routinely assess all patients on admission for CPE status
Guideline for Infection Prevention and Control (IPC) of Carbapenemase-Producing Enterobacteriaceae (CPE)

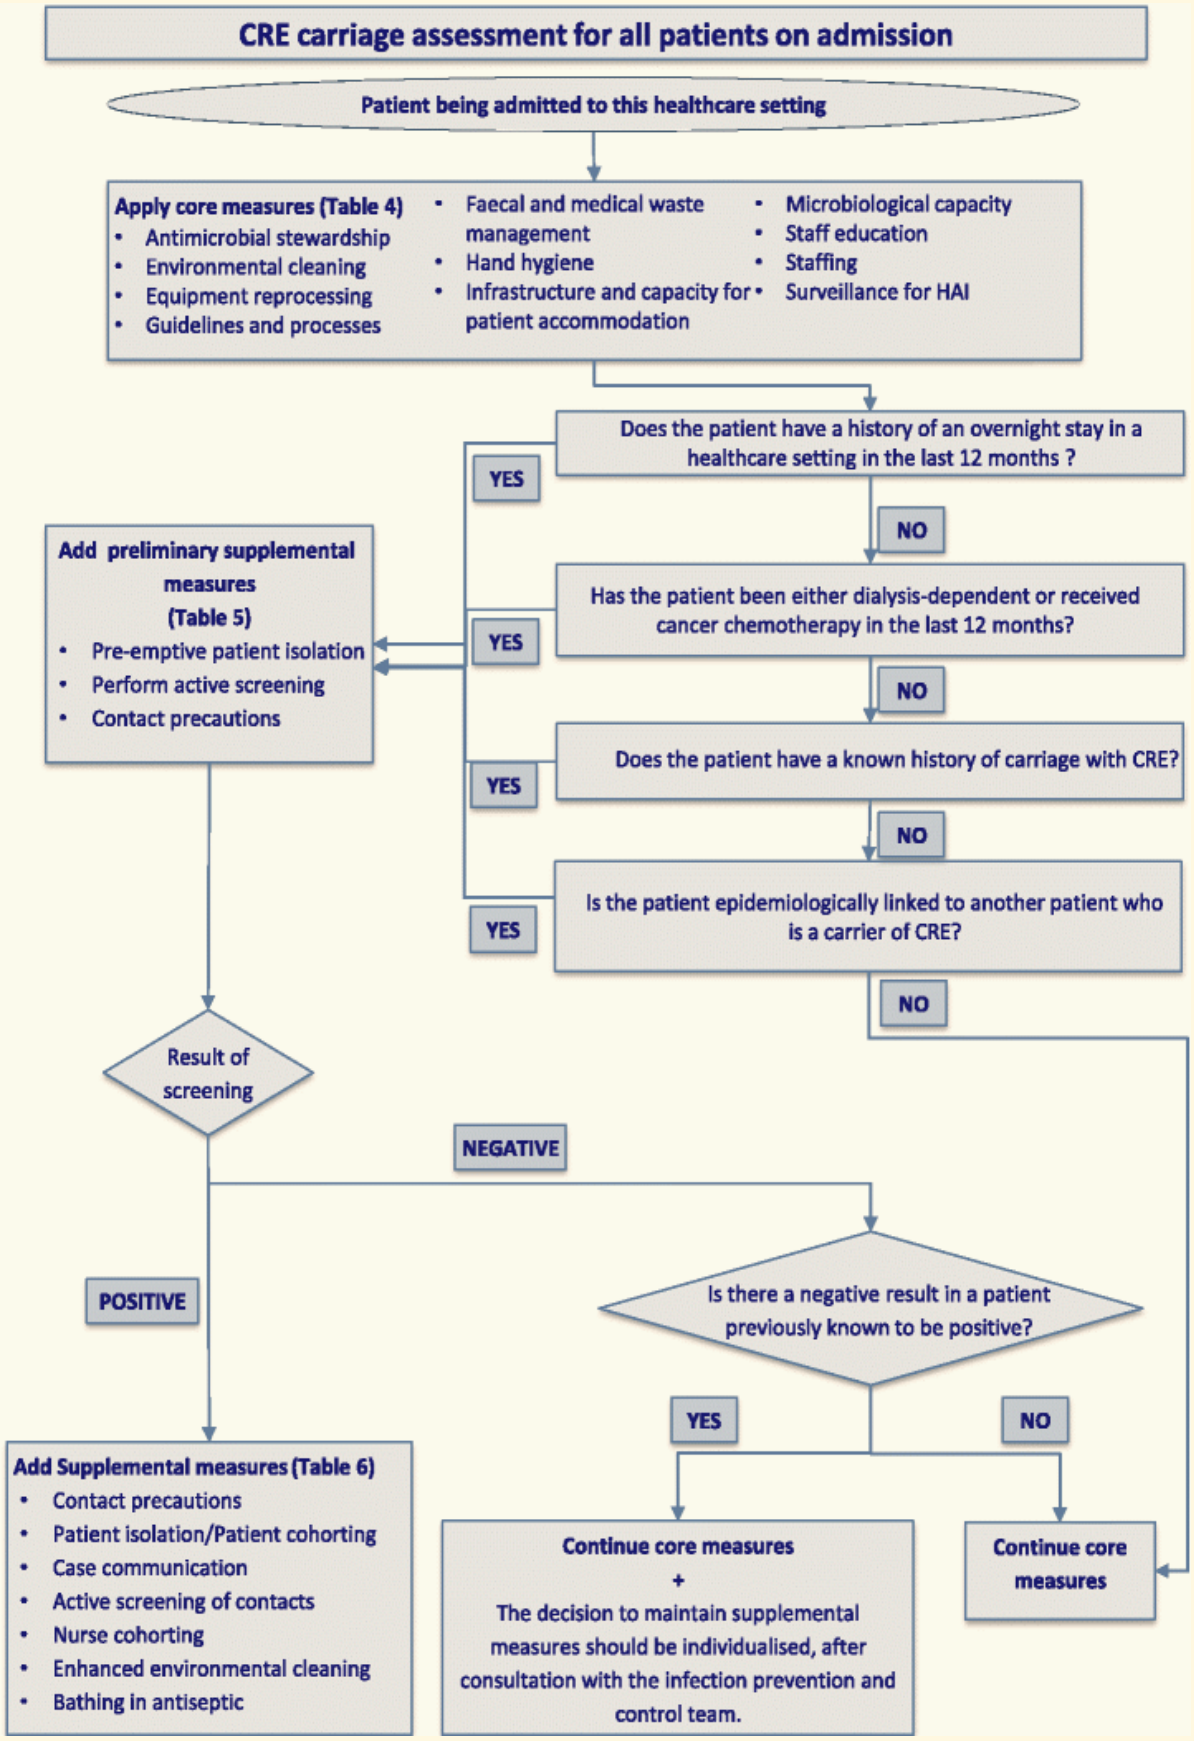

Revision of Antibiotic AWaRe Classification as per WHO 2019 guidelines

As part of the review of antibacterial agents, a new categorization of antibacterial agents into three groups was proposed:

- **ACCESS** – first and second choice antibiotics for the empiric treatment of most common infectious syndromes;
- **WATCH** – antibiotics with higher resistance potential whose use as first and second choice treatment should be limited to a small number of syndromes or patient groups; and
- **RESERVE** – antibiotics to be used mainly as 'last resort' treatment options

ACCESS Group

Beta-lactam medicines		Other antibacterials	
Amoxicillin	Cefotaxime*	Amikacin	Gentamicin
Amoxicillin + clavulanic acid	Ceftriaxone*	Azithromycin*	Metronidazole
Ampicillin	Cloxacillin	Chloramphenicol	Nitrofurantoin
Benzathinebenzylpenicillin	Phenoxymethylpenicillin	Ciprofloxacin*	Spectinomycin (EML only)
Benzylpenicillin	Piperacillin + tazobactam*	Clarithromycin*	Sulfamethoxazole + Trimethoprim
Cefalexin	Procaine benzyl Penicillin	Clindamycin	Vancomycin (oral)*
Cefazolin	*Meropenem**	Doxycycline	Vancomycin (parenteral)*
Cefixime*			

Watch group antibiotics

Quinolones and fluoroquinolones e.g. Ciprofloxacin, Levofloxacin, Moxifloxacin, Norfloxacin
3rd-generation cephalosporins (with or without beta-lactamase inhibitor) e.g. Cefixime, eftriaxone, Cefotaxime, Ceftazidime
Macrolides e.g. Azithromycin, Clarithromycin, Erythromycin
Glycopeptides e.g. Teicoplanin, Vancomycin
Anti-Pseudomonalpenicillins with beta-lactamase inhibitor e.g. piperacillin +tazobactam
Carbapenems e.g. Meropenem, Imipenem + Cilastatin, Penems e.g. Faropenem

Reserve group ('last-resort') antibiotics

Aztreonam	Fosfomycin (IV)
4th generation cephalosporins e.g. Cefepime	Oxazolidinones e.g. Linezolid
5th generation cephalosporins e.g.Ceftaroline	Tigecycline
Polymyxins e.g. Polymyxin B, Colistin	Daptomycin

3. Biomedical Waste Management

Segregation of Biomedical Waste			
Yellow (Non-Chlorinated Plastic Bags)	**Red (Non-Chlorinated Plastic Bags)**	**Blue Card Board Boxes**	**White (Translucent Puncture Proof Container)**
Human Anatomical, Infectious Waste & Cytotoxic Waste ➢ Human tissues, organs, body parts and foetus ➢ Items contaminated with blood, body fluids like dressings, plaster casts, cotton swabs ➢ Bags containing residual or discarded blood and blood components ➢ Antibiotics, cytotoxic drugs along with glass or plastic ampoules, vials (with cytotoxic labelled bag) ➢ Discarded disinfectants ➢ Discarded linen, mattresses, beddings contaminated with blood or body fluid ➢ Blood bags ➢ Laboratory culture, stocks or specimens of microorganisms ➢ Live or attenuated vaccines	**Contaminated Waste (Recyclable)** ➢ Disposable items ➢ Tubing ➢ Bottles ➢ Intravenous tubes & sets ➢ Catheters ➢ Urine bags ➢ Gloves ➢ Syringes (without needles and fixed needle syringes) ➢ Vaccutainers with their needles cut	**Glassware** ➢ Broken or discarded and contaminate glass including medicine vials and ampoules except those contaminate with cytotoxic wastes **metallic body implants**	**Waste Sharps Including Metals** ➢ Needles ➢ Syringes with fixed needles ➢ Needles from needle tip cutter or burner ➢ Scalpels ➢ Blades ➢ Any other contaminated sharp object that may cause puncture and cuts ➢ Contaminated sharps
Black/ Green – General Garbage (domestic waste, papers, packaging material, left over food)			

Biomedical Waste Management (BMW) RULES 2016

Category	Type ofwaste	Type of Bag/ container	Treatment/ Disposal options
Yellow	Human anatomical waste	Yellow coloured	Incineration/ Plasma pyrolysis/ deep burial
	Animal anatomical waste		
	Soiled waste	non chlorinated plastic bags	Incineration/ Plasma Pyrolysis/ deep burial/ autoclaving or hydroclaving + shredding/mutilation
	Expired/ discarded medicines- pharmaceutical waste, cytotoxic drugs	Yellow coloured containers/ non chlorinated plastic bags	Incineration (cytotoxic drugs at temperature > 1200□C)
	Chemical waste	Yellow coloured containers/ non chlorinated plastic bags	Incineration or Plasma pyrolysis or Encapsulation
	Discarded linen contaminated with blood/ body fluids	Non- chlorinated yellow plastic bags / suitable packing material	Non- chlorinated chemical disinfection followed by incineration/ plasmapyrolysis
	Microbiology, other clinical lab waste, blood bags, live/attenuated vaccines	Autoclave safe plastic bag/container	Pre-treat to sterilize with non-chlorinated chemicals on-site as per NACO/ WHO guidelines + Incineration
Red	Contaminated Waste(Recyclable)	Red coloured non-chlorinated Plastic bags or containers	• Autoclaving/ micro- waving/ hydroclaving + shredding • Mutilation/ sterilization+ shredding. Treated waste sent to registered or authorized recyclers or for energy recovery or plastics to diesel or fuel oil or for road making,
White (Translucent)	Waste sharps including Metals	Puncture proof, Leak proof, tamper proof containers	• Autoclaving/dry heat sterilization+ shredding/ mutilation • Encapsulation in metal container or cement concrete • Sanitary landfill/ designated concrete waste sharp pit
Blue	Glassware, Metallic body implants	• Glass test tubes • Empty glass Bottles • Contaminated glass bottles • Broken glass ampoules containing discarded/Expired medicines except chemotherapeutic medicines • Metallic body implants • Reusable glass slide	Disinfection (by soaking the washed glass waste after cleaning with detergent and Sodium Hypochlorite treatment)/ through autoclaving/ microwaving/ hydroclaving + recycling

BMW 2018 Amendment

- Establish a Bar- code system for bags
- Phase out use of chlorinated plastic bags (excluding blood bags) and gloves (By the 27th March, 2019)
- Health Care Facilities having less than ten beds shall have to install Sewage Treatment Plant by the 31st December, 2019.
- All the health care facilities (any number of beds) shall make available the annual report on its web-site within a period of two years from the date of publication of Bio-Medical Waste Management (Amendment) Rules,2018;"

h) Microbiology, Biotechnology and other clinical laboratory waste: Blood bags, Laboratory cultures, stocks or specimens of micro-organisms, live or attenuated vaccines, human and animal cell cultures used in research, industrial laboratories, production of biological, residual, toxins, dishes and devices used for cultures.	Autoclave safe plastic bags or containers	Pre-treat to sterilize with non-chlorinated chemicals on-site as per National AIDS Control Organization or World Health Organization guidelines thereafter for Incineration.

- Autoclave, Microwave and Hydroclave
- As per World Health Organisation guidelines on Safe management of wastes from healthcare activities and WHO Blue Book, 2014 and thereafter sent for incineration
- Routine mask and gown –yellow
- Cardboard boxes with blue colored marking - Puncture proof and leak proof boxes or containers with blue colored marking
- Chemical treatment using at least 10% Sodium Hypochlorite – corrected1-2%

Autoclave

Condition:

- 121°C, 15 pounds pressure for 60minutes
- 135°C, 31 pounds pressure for 45minutes
- 149°C, 52 pounds pressure for 30minutes

- Validation:
  - *Geobacillusstearothermophilus* with at least $1X10^6$ spores
  - Three monthly interval
- Daily - Chemical indicator strip

BMW 2019 Amendment

1. Update on day to day basis the bio-medical waste management register and display the monthly record on its website according to the bio-medical waste generated in terms of category and colour coding as specified in Scheduled.
2. Annual report on its web-site within a period of two years from the date of publication of the Bio- Medical Waste Management (Amendment) Rules, 2018 is made available.
3. Health Care Facilities having less than ten beds shall have to comply with the output discharge standard for liquid waste by 31st December,2019.

4. Post exposure prophylaxis (PEP)

"Post exposure prophylaxis" (PEP) refers to the comprehensive management given to minimize the risk of infection following potential exposure to blood-borne pathogens (HIV, HBV, HCV).

Steps for Managing Occupational Exposure

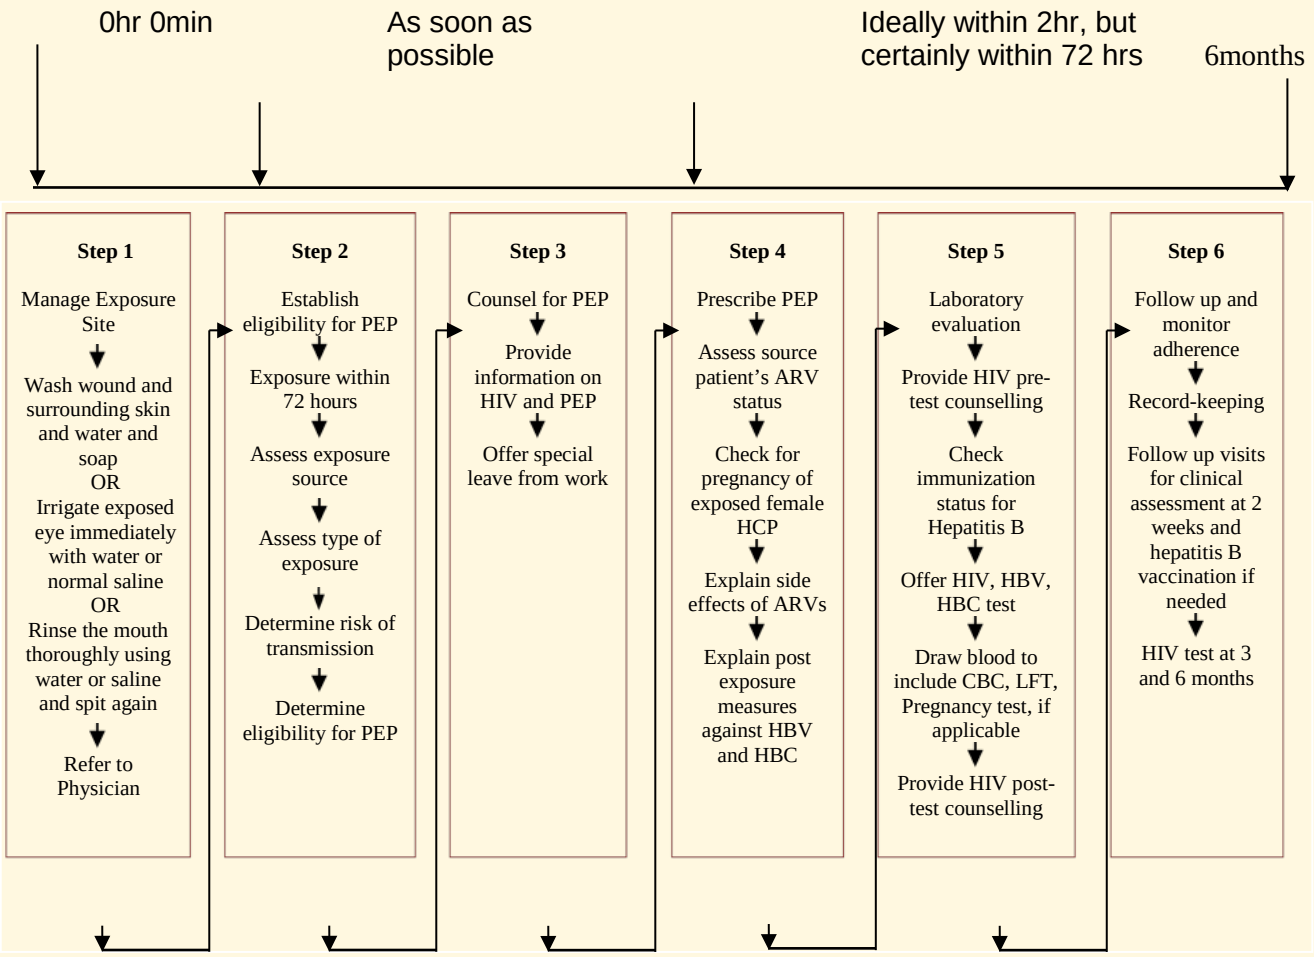

PEP : Post Exposure Prophylaxis ARV : Anti Retroviral
HCP : Health Care Professional CBC: Complete Blood Count
LFT : Liver Function Test.

References:

1. https://www.who.int/gpsc/5may/Hand_Hygiene_Why_How_and_When_Brochure.pdf
2. https://www.ijmm.org/documents/Treatment_Guidelines_2019_Final.pdf
3. https://www.who.int/medicines/news/2019/WHO_releases2019AWaRe_classification_antibiotics/en/
4. https://dhr.gov.in/sites/default/files/Bio-medical_Waste_Management_Rules_2016.pdf
5. https://www.cdc.gov/hai/organisms/cre/cre-facilities 2018.pdf

REAL-TIME ACTIONABLE PATIENT EXPERIENCE OF CARE (R-TAPE)

SRI VENKATESWARA INSTITUTE OF MEDICAL SCIENCES

వైద్య సేవల పట్ల మీ అనుభవాలని మాకు తెలియజేయండి

Tirumala Tirupati Devasthanams, Tirupati.

OPTION - 1 : Q.R CODE

HELP US TO SERVE YOU BETTER మీ కొరకు మా సేవలు మరింత మెరుగు పరుచుకోవడానికి మాతో సహకరించండి

HAVE WE TAKEN GOOD CARE OF YOU?

మా వైద్య సంరక్షణ సేవల పట్ల మీరు సంతృప్తి చెందారా?

SHARE YOUR FEED BACK

మీ అనుభవాన్ని తెలియచేయండి

SVIMS CELEBRATING 25 Years SILVER JUBILEE YEAR 1983 - 2018

OPTION - 2 : WEB LINK

https://internationalqualitymeasurers.org/svims

OPTION - 3 : KIOSK

STEP - 1

MOBILE NUMBER*
Enter Mobile Number*

మీ పది అంకెల సెల్ నెంబర్‌ను నమోదు చేయండి

2

OTP*
883482

మీ ఫోన్‌కు వచ్చిన ఓ.టి.పి తిరిగి నమోదు చేయండి

3

VERIFY OTP

'వెలిపై ఓ.టి.పి' ని వేలితో తాకండి

4

స్క్రీన్ పై వున్న ప్రశ్నలను చదివి మీకు నచ్చిన నక్షత్రాలను (రేటింగ్) ఇవ్వండి

WE VALUE YOUR FEEDBACK

YOUR VOICE MATTERS!

QualityTech

Technology Partners

SVIMS - Patient Experience of Care

Physical and Virtual options for sharing feedback

URL: https://internationalqualitymeasurers.org/svims

SVIMS Sri Venkateswara Institute of Medical Sciences

AN AUTONOMOUS UNIVERSITY ESTABLISHED BY ACT OF ANDHRA PRADESH STATE LEGISLATURE IN 1996 RECOGNIZED UNDER SECTION 12(B) OF UGC

ENGLISH | తెలుగు | தமிழ் | हिंदी

PATIENT EXPERIENCE OF CARE - GINEE (VIRTUAL ASSISTANT)

Though we work hard to provide our seamless services, we need your inputs to serve you better. Please rate us to help improve our services.

1. Communication Experience with Doctors
2. Communication Experience with Nurses
3. Communication Experience with Staff.
4. Communication about Medicines.
5. Discharge Process.
6. Cleanliness of Hospital & Toilets.
7. Responsiveness of Staff/Doctors/Nurses.
8. Overall Rating of Hospital.
9. Will you recommend this Hospital to someone for Care?

○ Yes ○ No ○ May Be

SVIMS Sri Venkateswara Institute of Medical Sciences

AN AUTONOMOUS UNIVERSITY ESTABLISHED BY ACT OF ANDHRA PRADESH STATE LEGISLATURE IN 1996 RECOGNIZED UNDER SECTION 12(B) OF UGC

ENGLISH | తెలుగు | தமிழ் | हिंदी

PATIENT EXPERIENCE OF CARE - GINEE (VIRTUAL ASSISTANT)

Though we work hard to provide our seamless services, we need your inputs to serve you better. Please rate us to help improve our services.

1. డాక్టర్లు మీతో మాట్లాడు విధానం
2. నర్సులు మీతో మాట్లాడు విధానం
3. ఆసుపత్రి సిబ్బంది మీతో మాట్లాడు విధానం
4. మందుల గురించి మీకు చెప్పిన విధానం
5. డిశ్చార్జ్ విధానం
6. ఆసుపత్రి మరియు మరుగు దొడ్లు యొక్క పరిశుభ్రత
7. సిబ్బంది / డాక్టర్లు / నర్సులు మీకు సహకరించు విధానం
8. మన ఆసుపత్రి గురించి మీ ఓవరాల్ రేటింగ్
9. మన ఆసుపత్రిని మీరు మిగిలిన వారికి సిఫార్స్ చేస్తారా

● Yes ○ No ○ May Be

The feedback form is available in 4 languages i.e., English, Telugu, Hindi and Tamil.

Patient Experience of Care
Consolidated Data as on 31-01-2021

OP Feedbacks – 1249
IP Feedbacks – 13201
Total Feedbacks - 14450

OP Feedbacks

Rating	Communication Experience with Doctors.
5	848
4	198
3	110
2	32
1	61

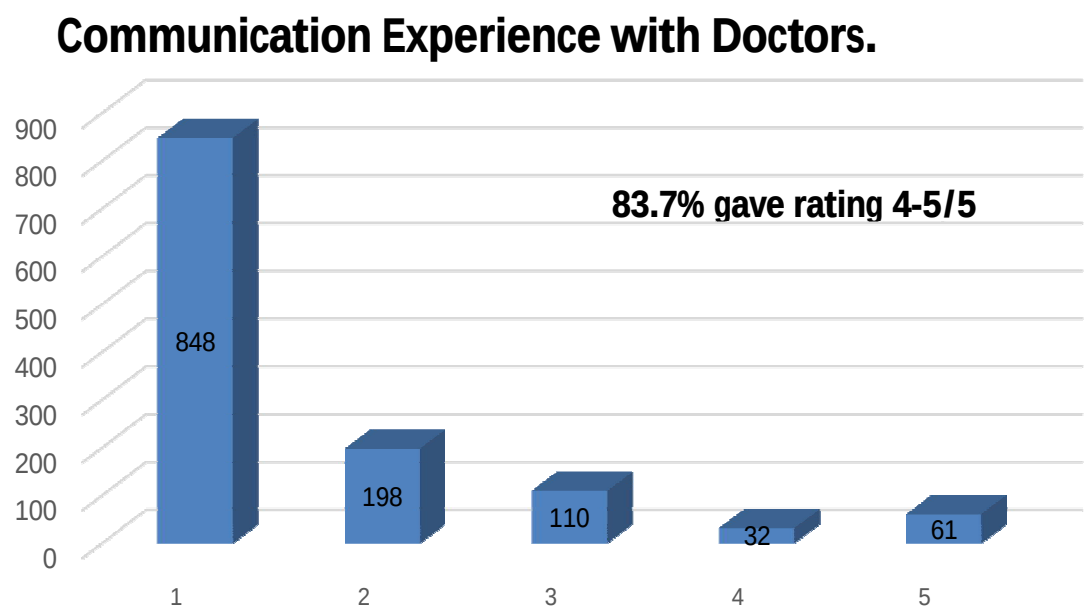

Rating	Communication Experience with Nurses.
5	817
4	177
3	133
2	55
1	67

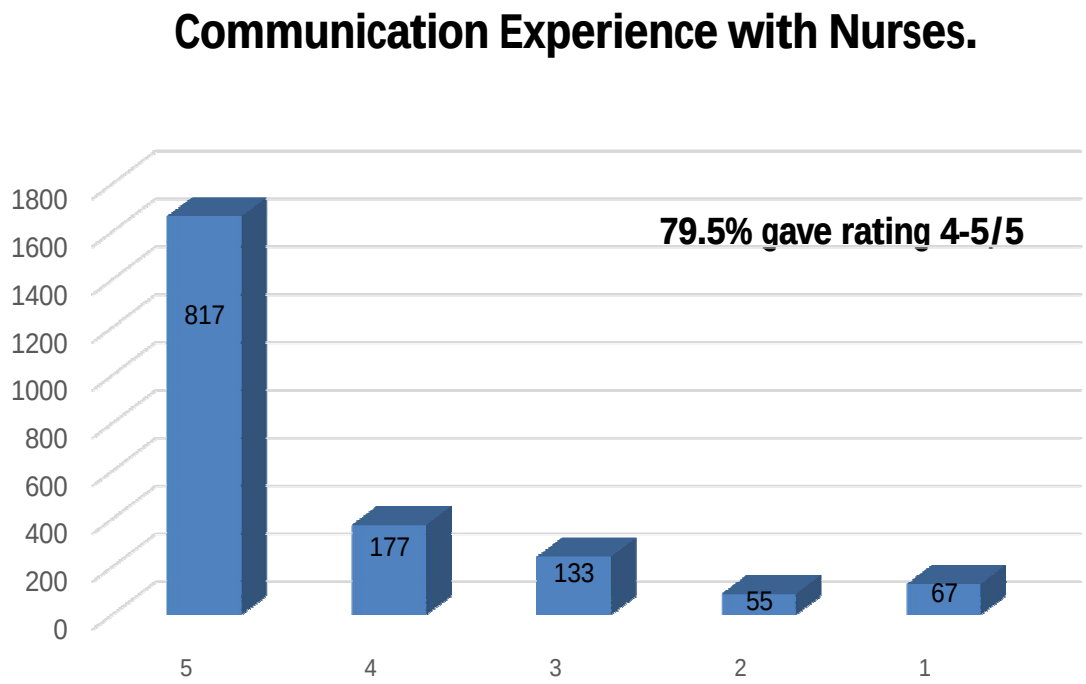

OP Feedbacks

Rating	Communication Experience with Staff.
5	1066
4	108
3	65
2	4
1	6

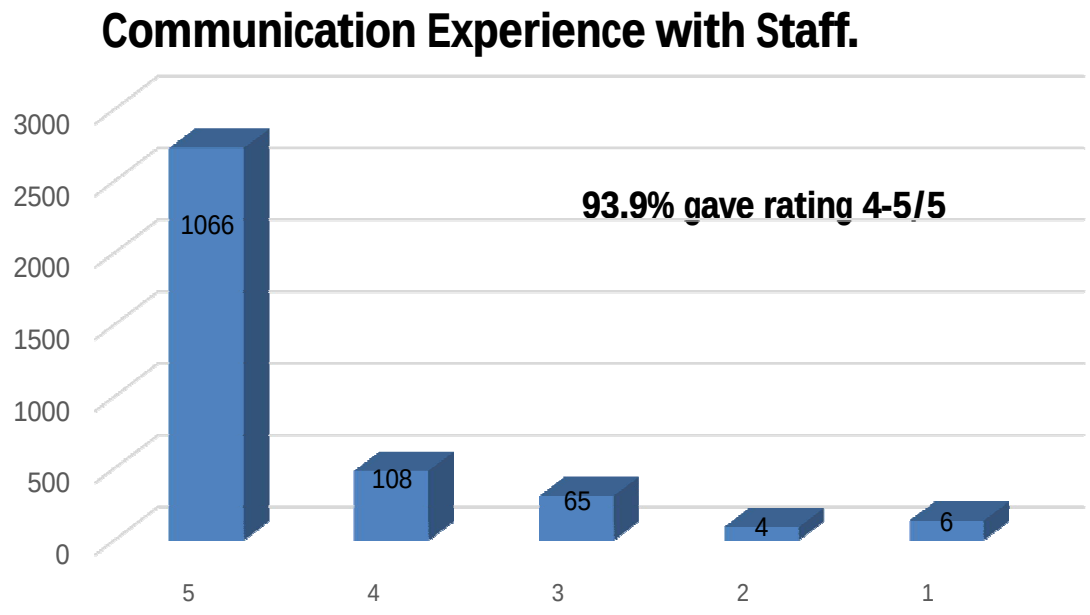

Rating	Communication about Medicines.
5	849
4	146
3	162
2	39
1	53

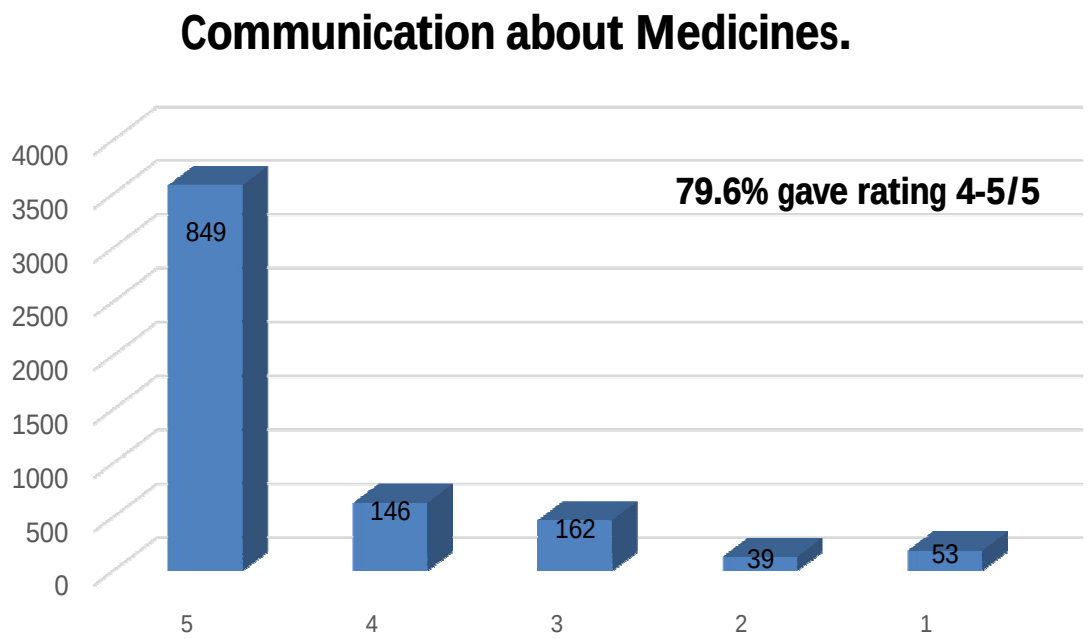

OP Feedbacks

Rating	Cleanliness of OPD and Toilets
5	1057
4	122
3	56
2	11
1	3

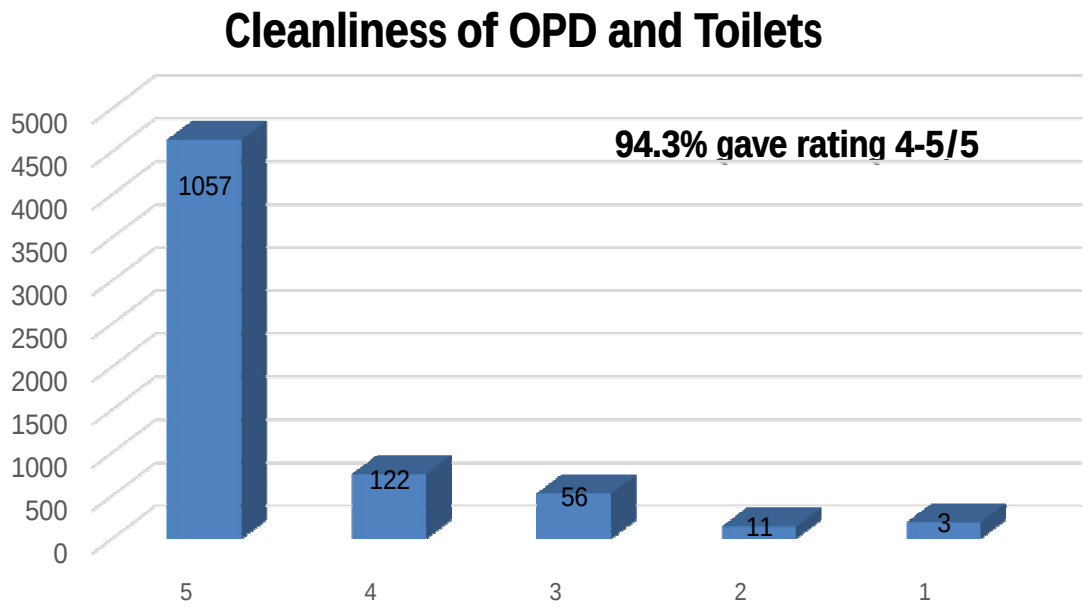

Rating	Availability & Responsiveness of Doctors/Nurses/Staff
5	821
4	146
3	166
2	46
1	70

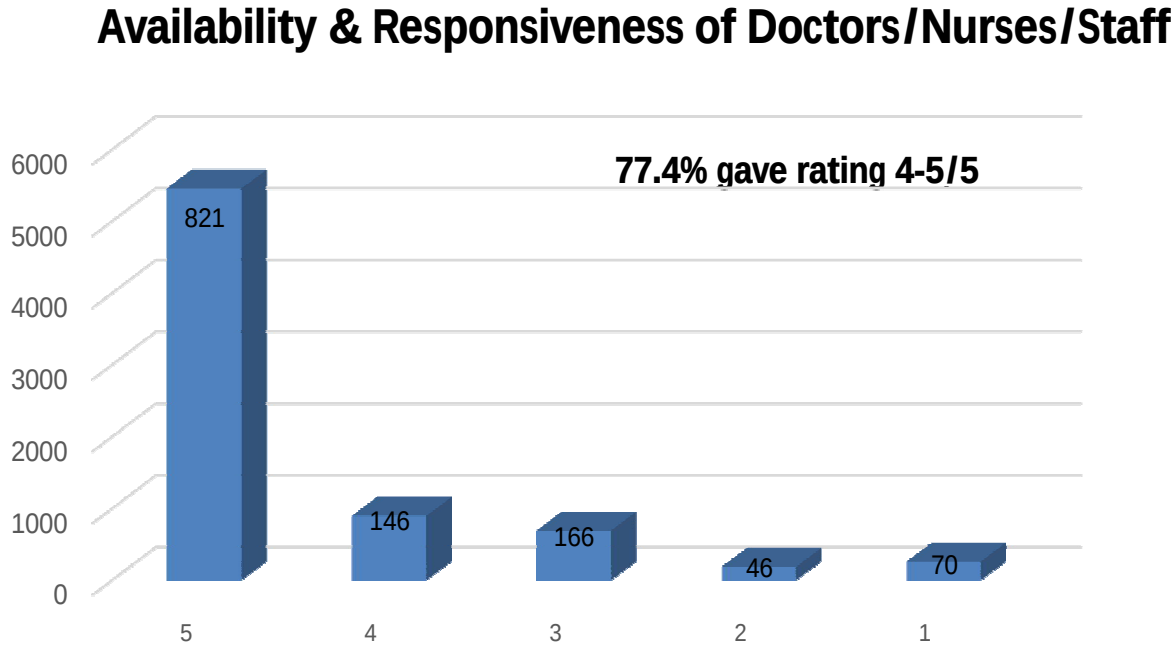

OP Feedbacks

Rating	Waiting time at Registration Counter including Reception
5	1043
4	140
3	52
2	5
1	9

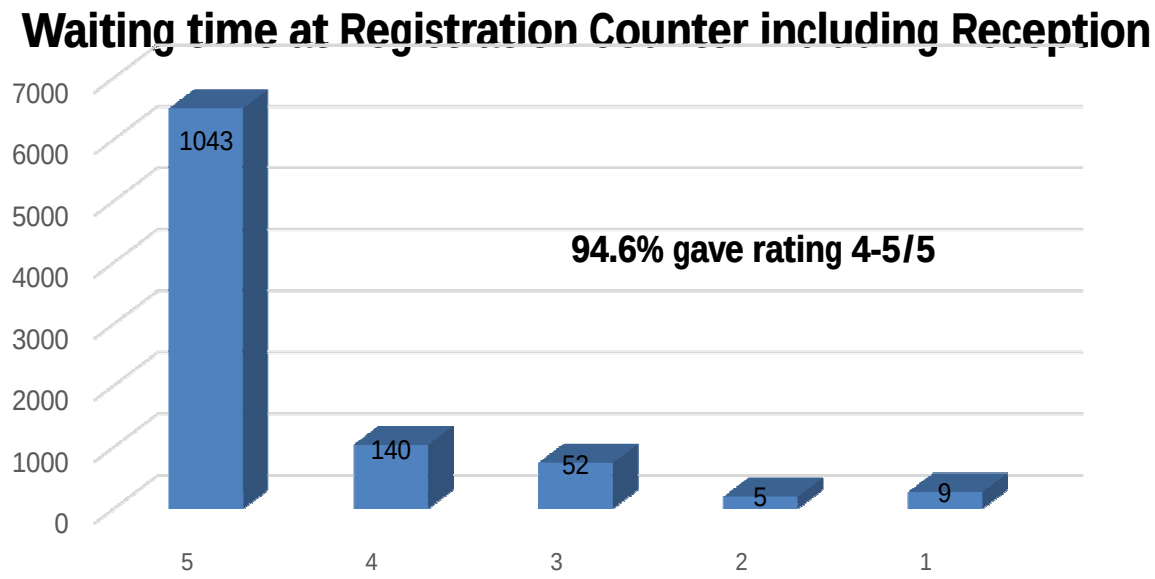

Rating	Time spent on Consultation, Examination and Counselling with Doctor
5	1045
4	79
3	111
2	10
1	4

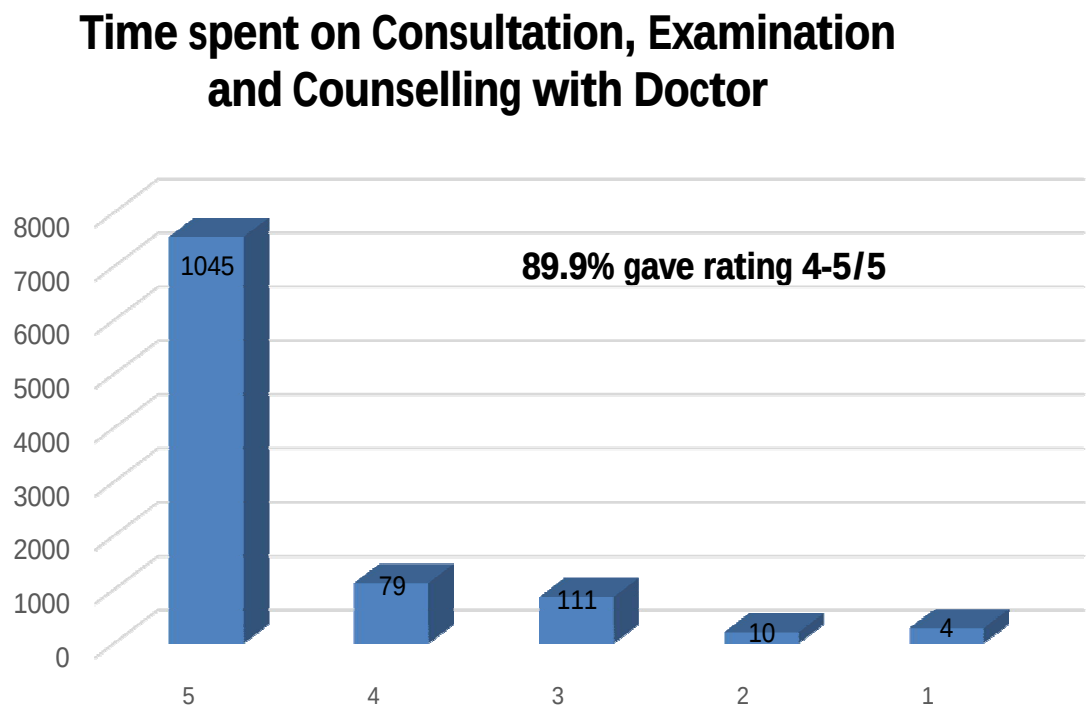

OP Feedbacks

Rating	Availability of Lab and Radiology investigation services within the Hospital
5	1041
4	120
3	79
2	5
1	4

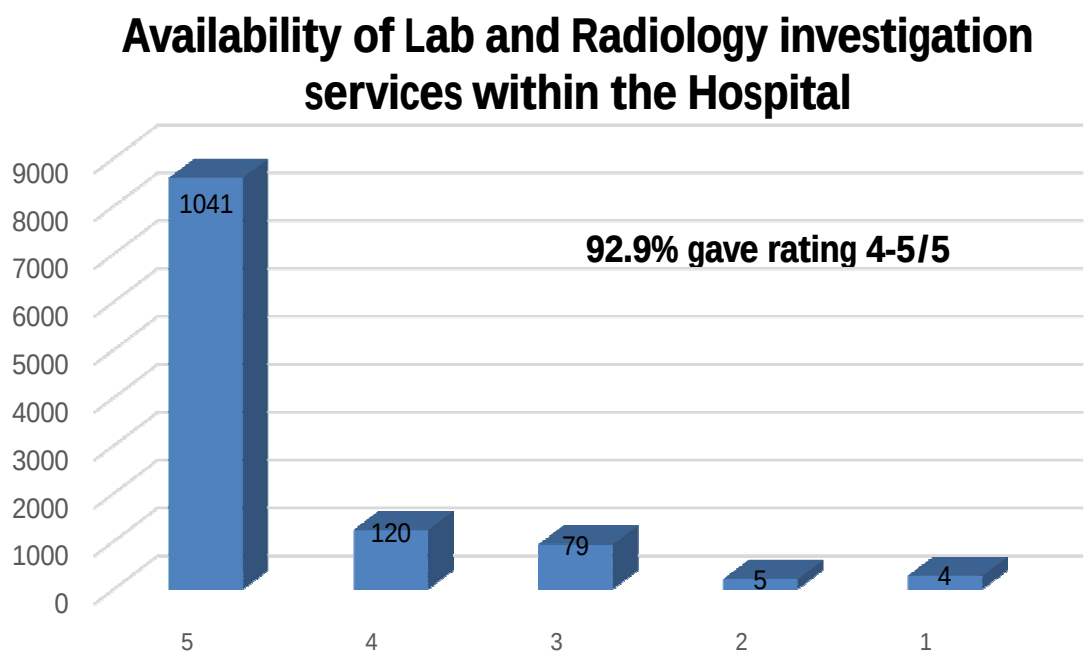

Rating	Overall Rating of Hospital
5	828
4	161
3	154
2	50
1	56

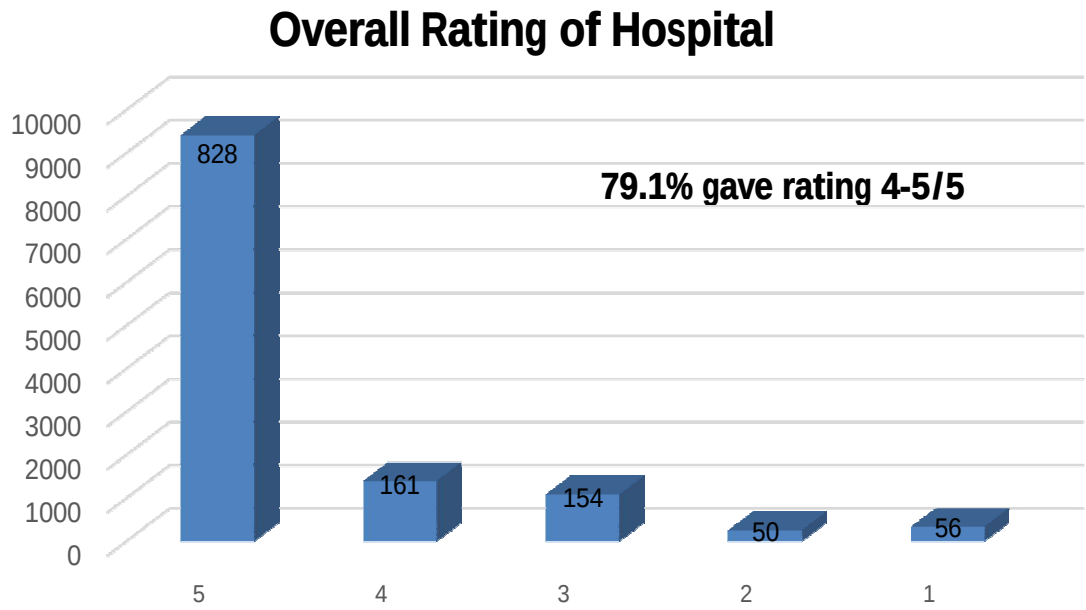

OP Feedbacks

Will you recommend this Hospital OP Services to someone for Care?

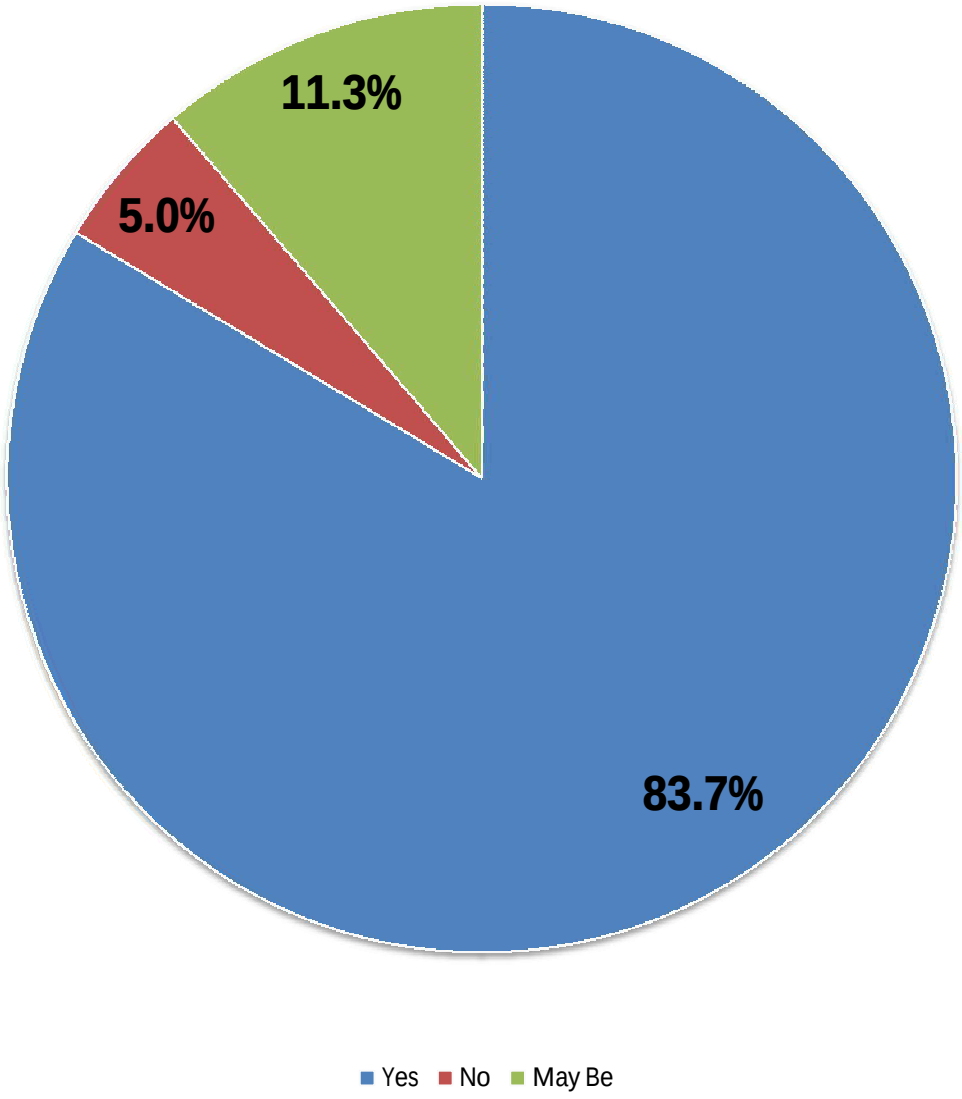

Opted For	Count	%
Yes	1045	83.7%
No	63	5.0%
May Be	141	11.3%
Total	**1249**	

IP Feedbacks

Rating	Communication Experience with Doctors.
5	9120
4	3335
3	419
2	173
1	154

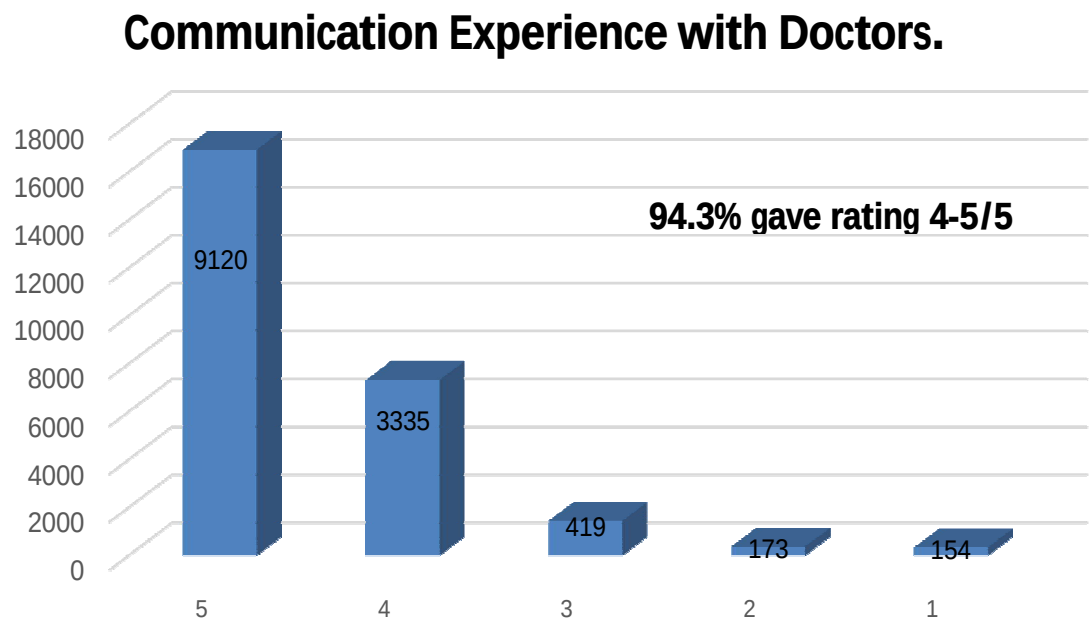

Rating	Communication Experience with Nurses.
5	7957
4	4026
3	748
2	239
1	231

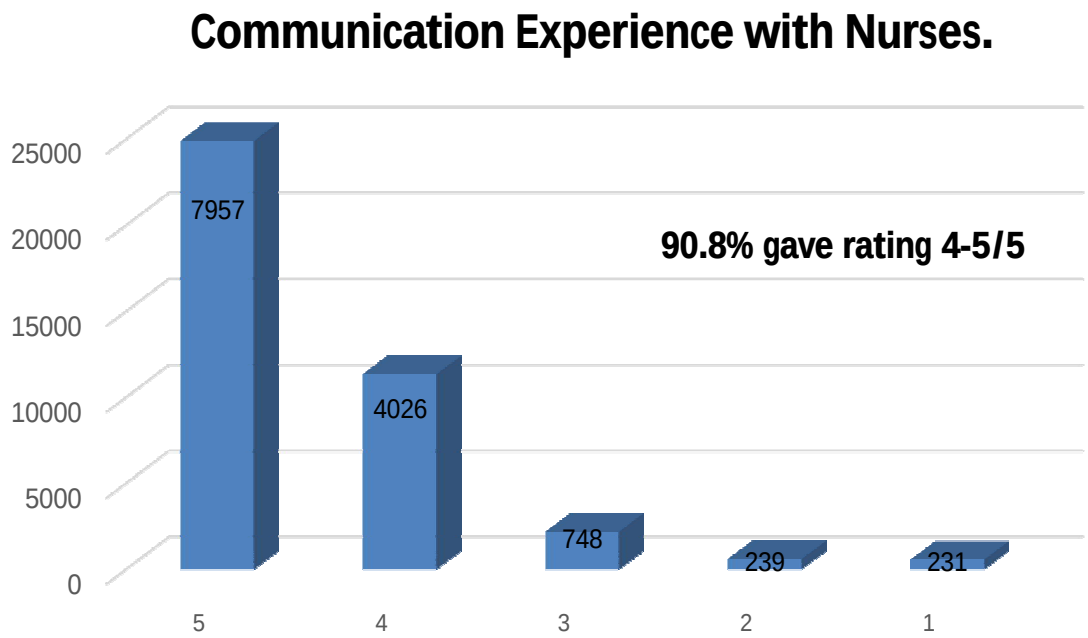

IP Feedbacks

Rating	Communication Experience with Staff and Ward boys.
5	8782
4	3456
3	523
2	211
1	229

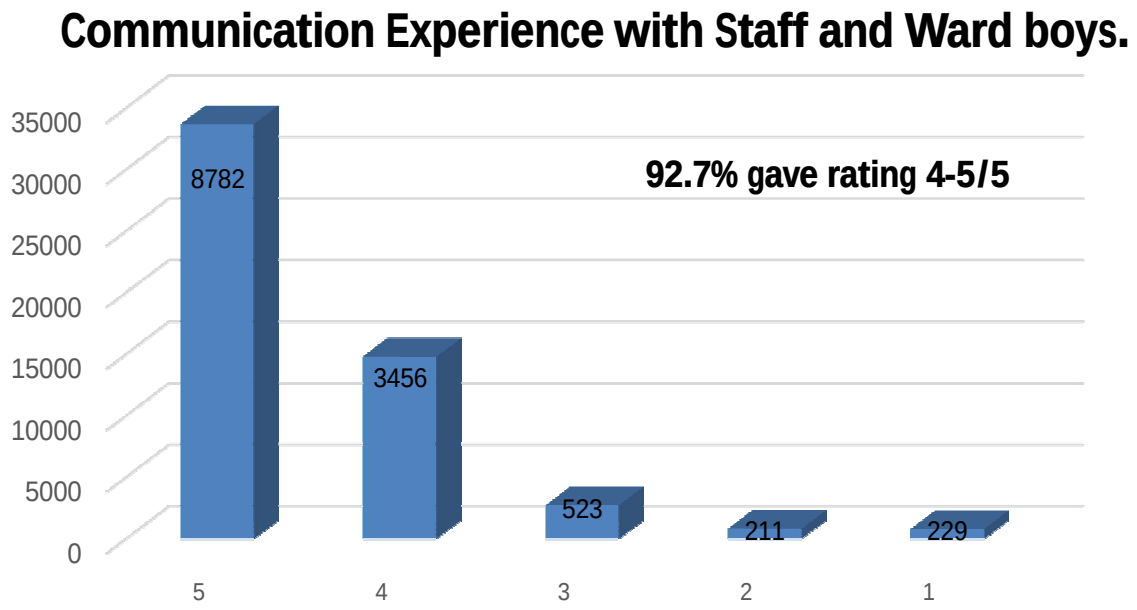

Rating	Communication about Medicines.
5	8021
4	4057
3	700
2	222
1	201

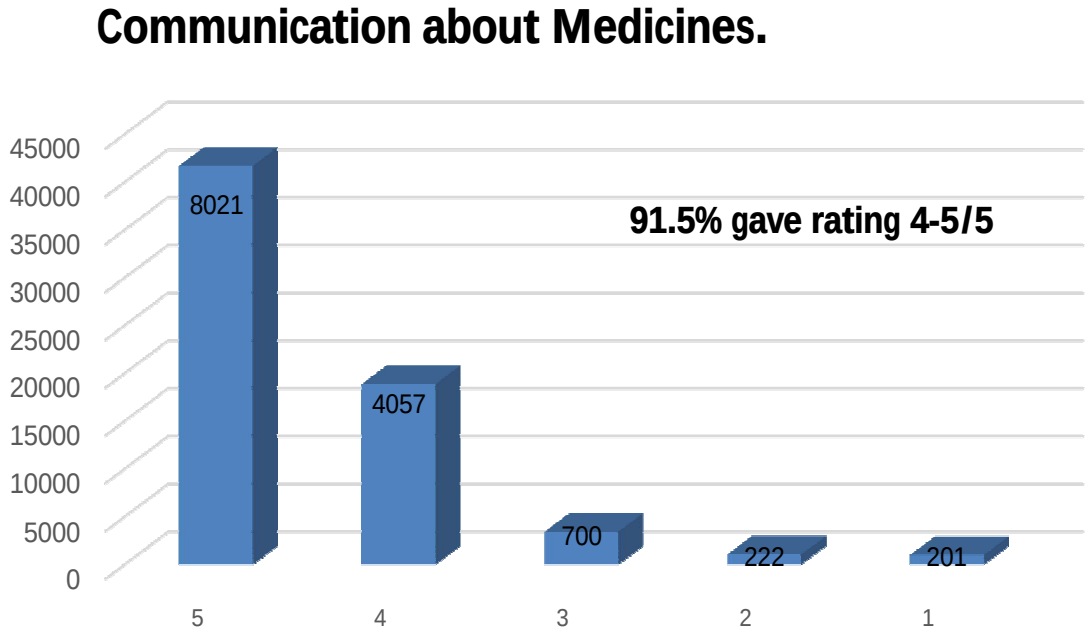

IP Feedbacks

Rating	Cleanliness of Wards & Toilets.
5	7754
4	4140
3	796
2	283
1	228

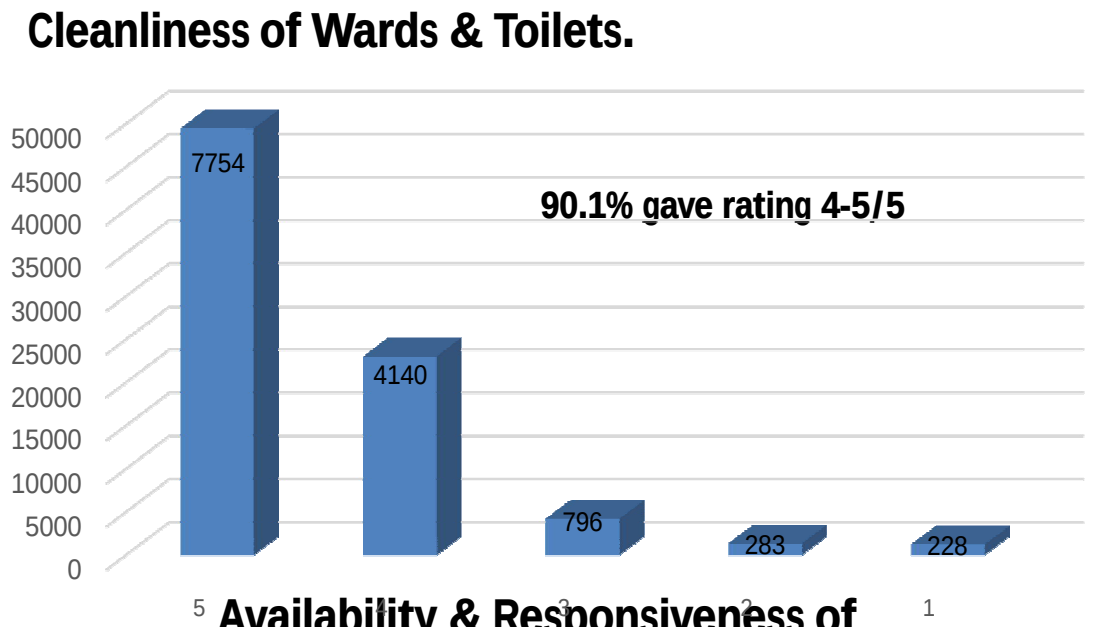

Rating	Availability & Responsiveness of Doctors/Nurses/Staff/Ward Boys.
5	11558
4	1222
3	372
2	26
1	23

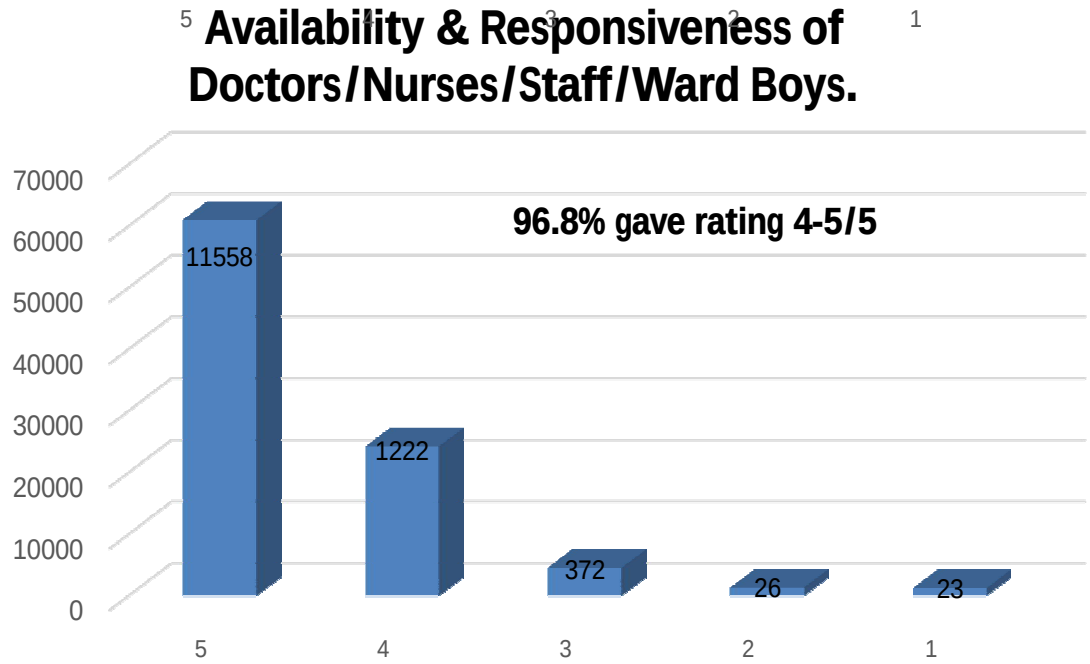

IP Feedbacks

Rating	Wait time at Admission Counter.
5	11725
4	1035
3	337
2	65
1	39

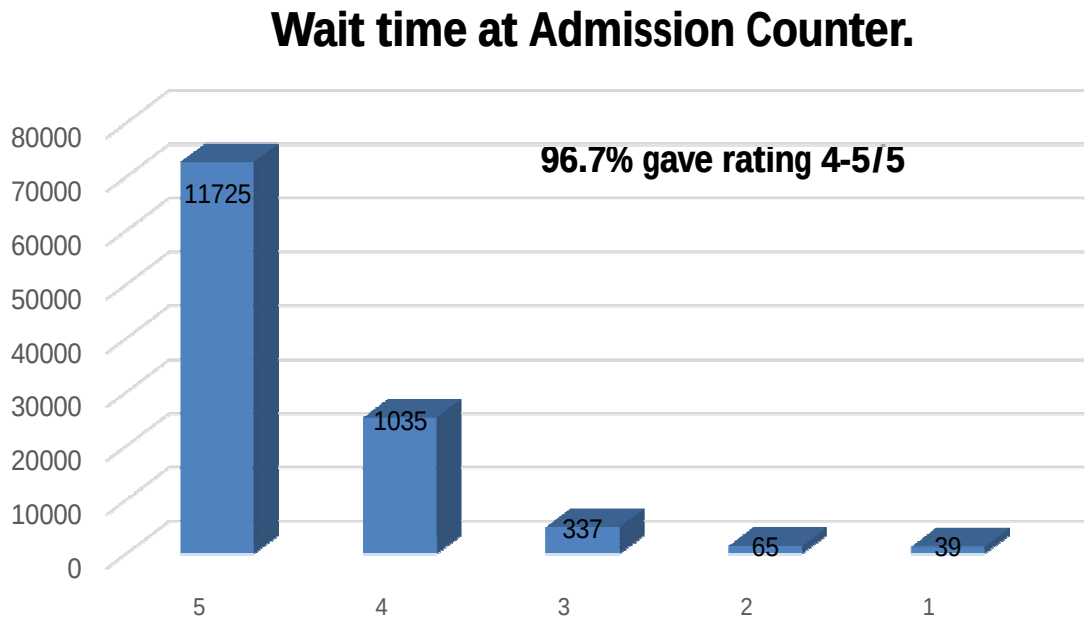

Rating	Supply of quality, prescribed diet in-time.
5	11604
4	1143
3	416
2	23
1	15

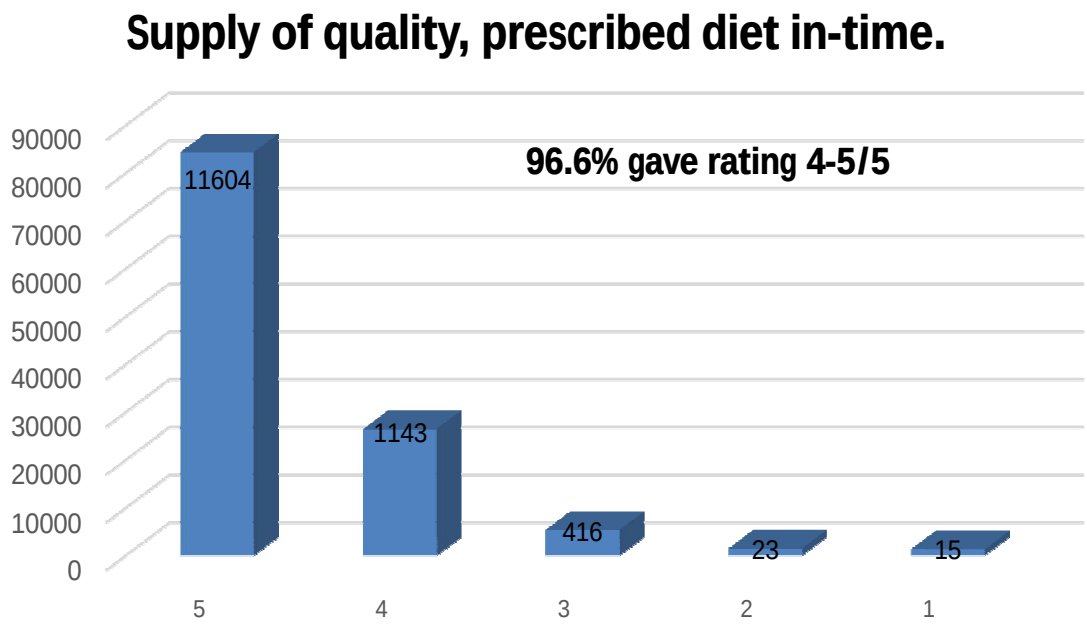

IP Feedbacks

Rating	Discharge Process.
5	8545
4	3334
3	790
2	257
1	275

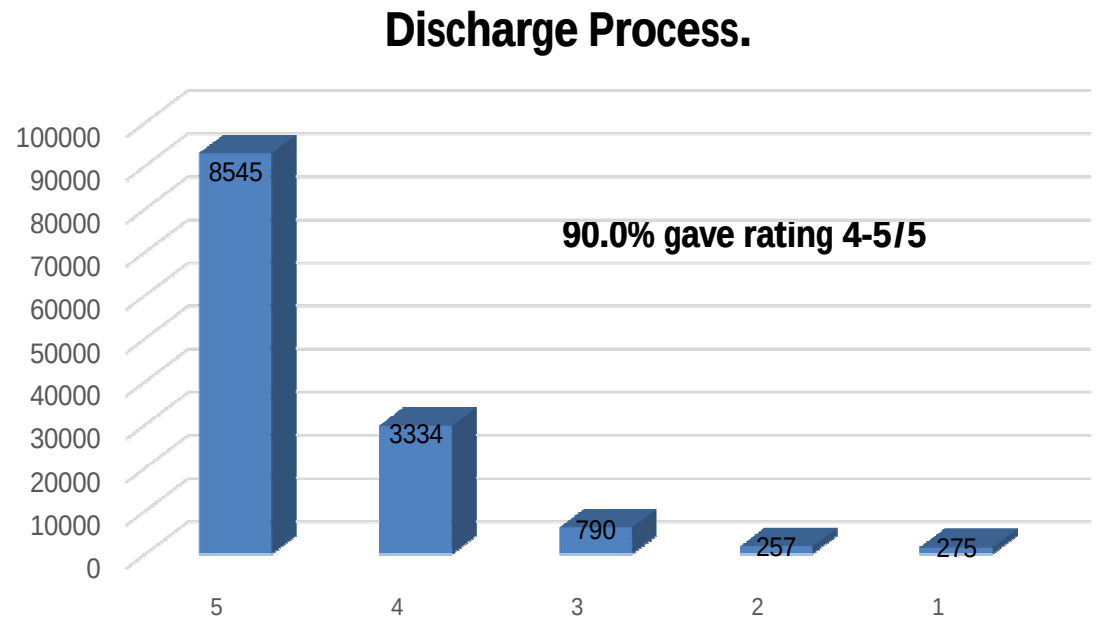

Rating	Overall Rating of Hospital
5	7808
4	3985
3	1023
2	203
1	182

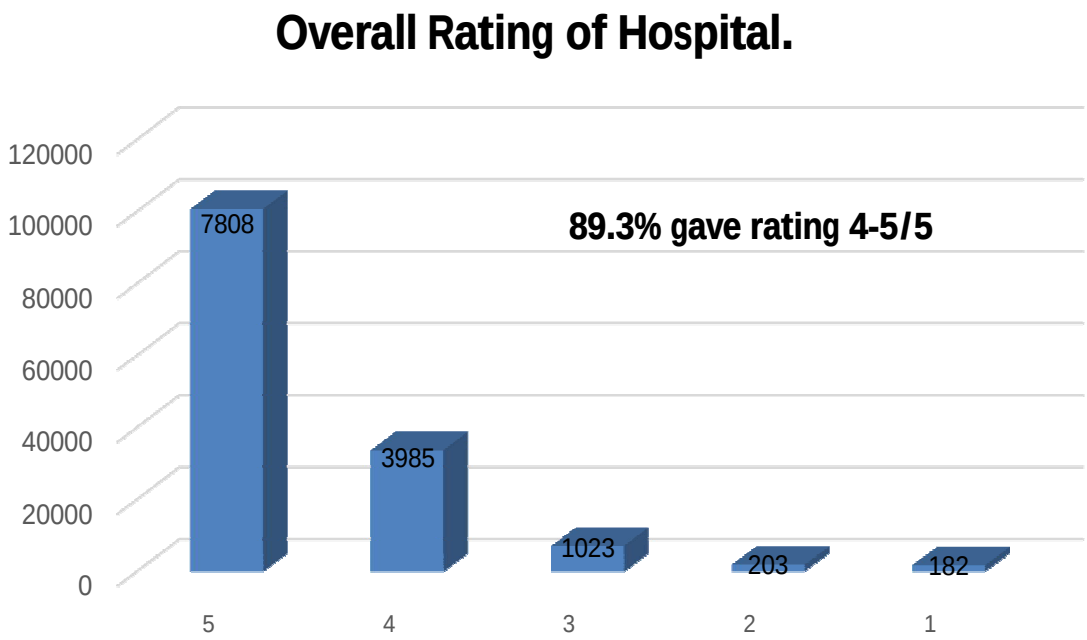

IP Feedbacks

Will you recommend this Hospital IP Services to someone for Care?

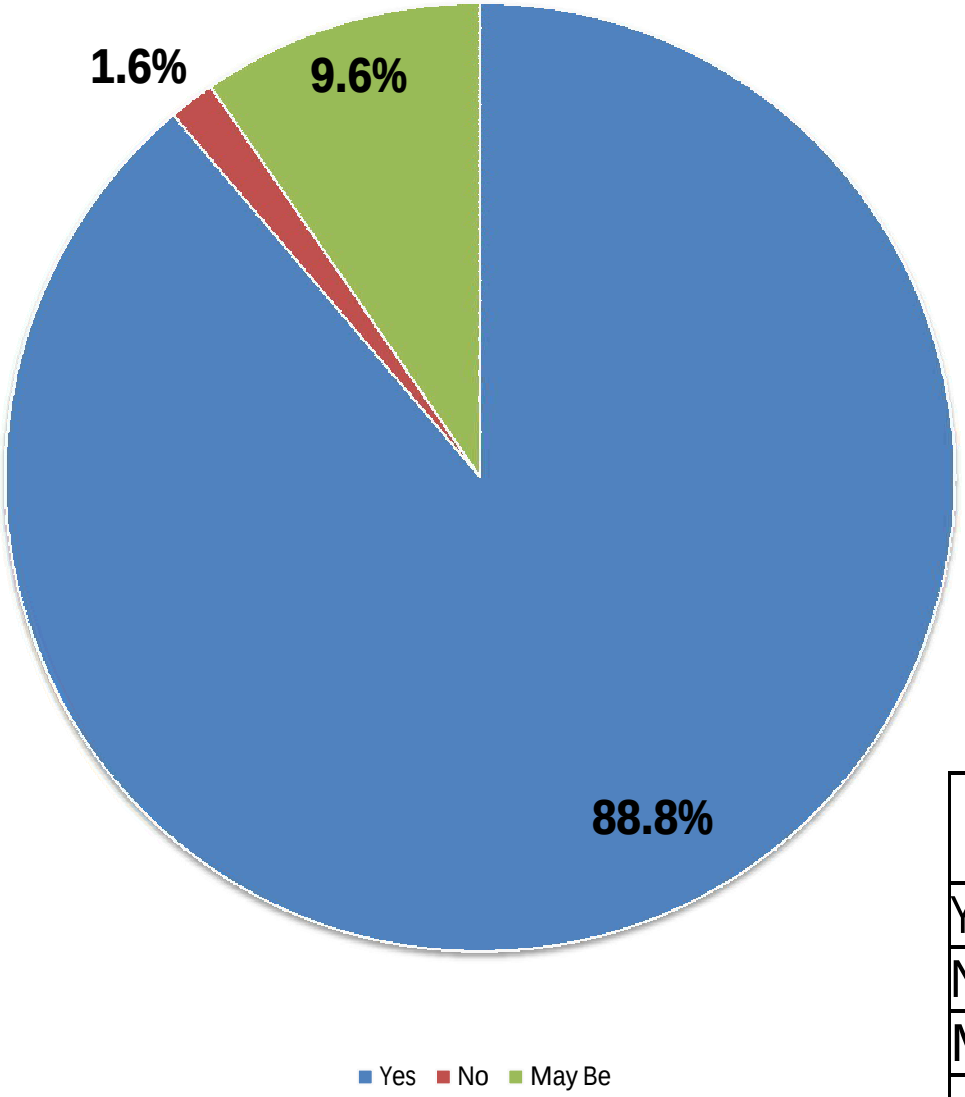

Opted For	Count	%
Yes	11726	88.8%
No	208	1.6%
May Be	1267	9.6%
Total	**13201**	

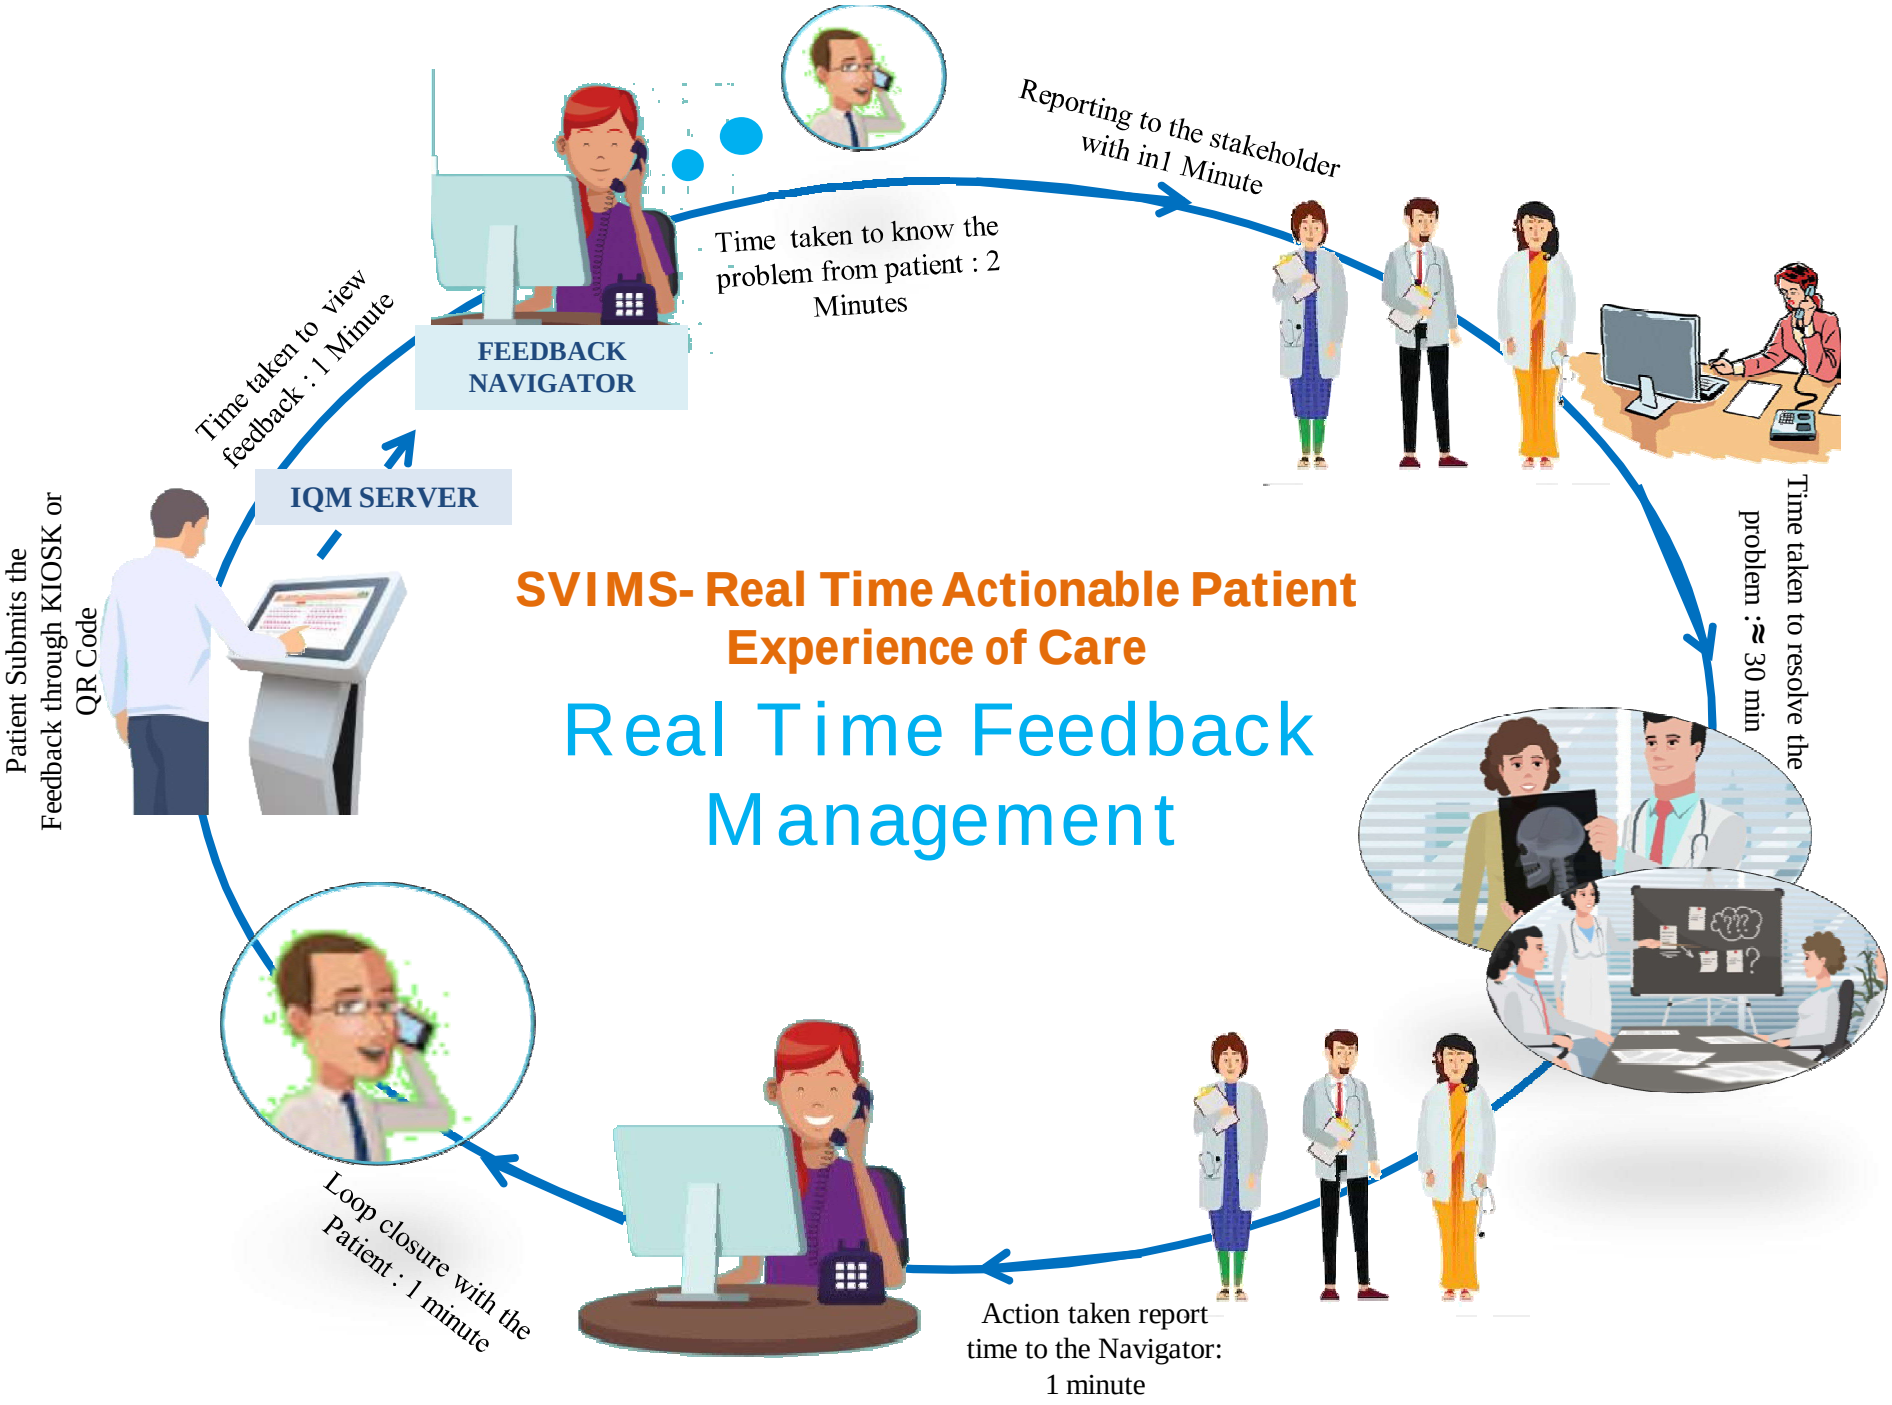
SVIMS- Real Time Actionable Patient Experience of Care
Real Time Feedback Management
Patient Submits the Feedback through KIOSK or QR Code
IQM SERVER
Time taken to view feedback : 1 Minute
FEEDBACK NAVIGATOR
Time taken to know the problem from patient : 2 Minutes
Reporting to the stakeholder with in1 Minute
Time taken to resolve the problem :≈ 30 min
Action taken report time to the Navigator: 1 minute
Loop closure with the Patient : 1 minute

Patient Experience of Care
Real-Time Action Taken Data as on 31-01-2021

Total Feedbacks - 12853

R-TAPE : Real-Time Action Started from 01-Aug-2018 – Consolidated Data as on 31-Jul-2020

Total Number of Responses

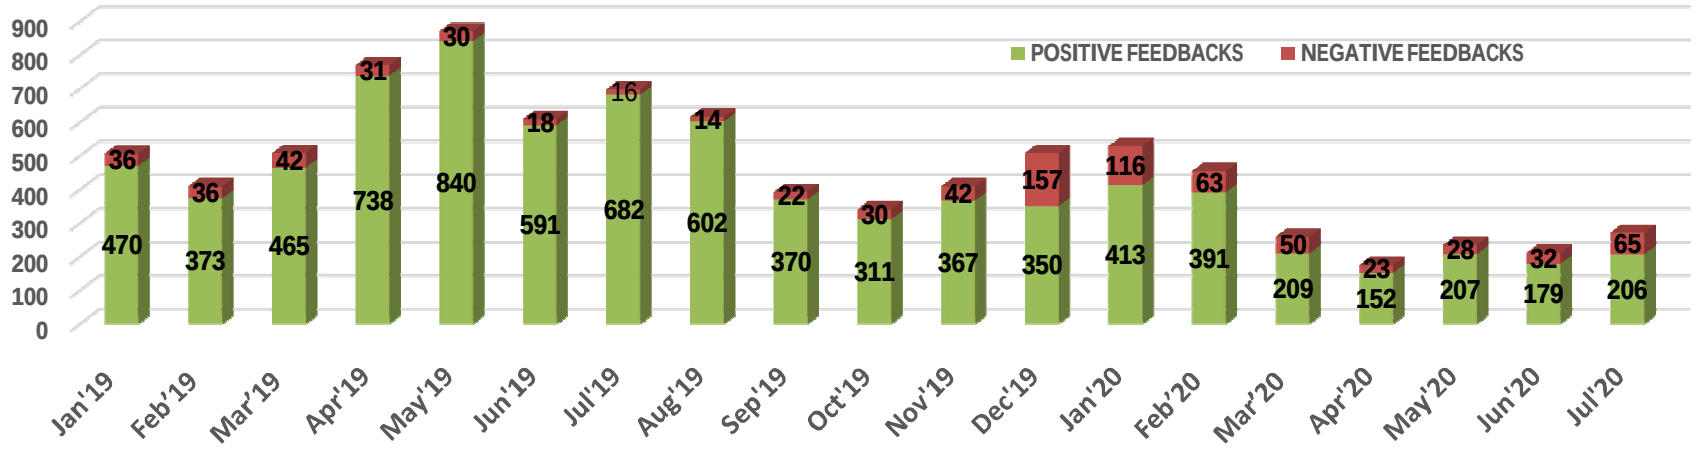

Month	Aug'18	Sep'18	Oct'18	Nov'18	Dec'18	Jan'19	Feb'19	Mar'19	Apr'19	May'19	Jun'19	Jul'19	Aug'19	Sep'19	Oct'19	Nov'19	Dec'19	Jan'20	Feb'20	Mar'20	Apr'20	May'20	Jun'20	Jul'20	Total
NEGATIVE FEEDBACKS	56	110	86	60	37	36	36	42	31	30	18	16	14	22	30	42	157	116	63	50	23	28	32	65	1200
POSITIVE FEEDBACKS	436	871	671	637	461	470	373	465	738	840	591	682	602	370	311	367	350	413	391	209	152	207	179	206	10992
TOTAL FEEDBACKS	492	981	757	697	498	506	409	507	769	870	609	698	616	392	341	409	507	529	454	259	175	235	211	271	12192

Trend in Positive & Negative Feedbacks Percentage

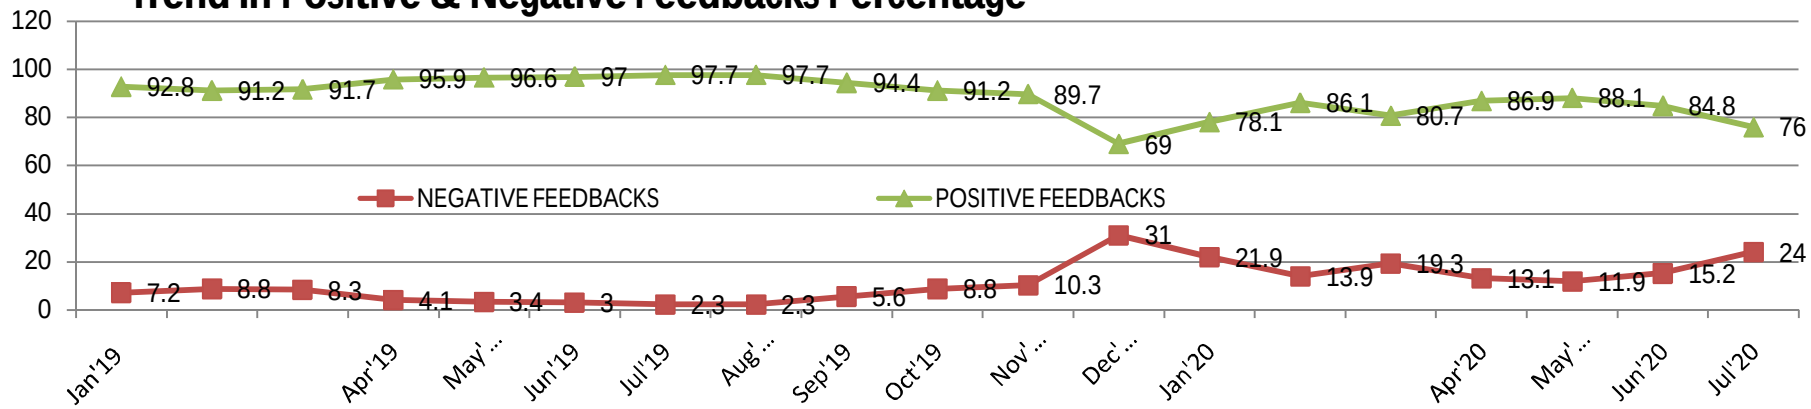

***Source**: V. Pranaya Theja, Network Engineer, SVIMS*

R-TAPE : Real-Time Action Started from 01-Aug-2020 – Consolidated Data as on 31-Jan-2021

Total Number of Responses

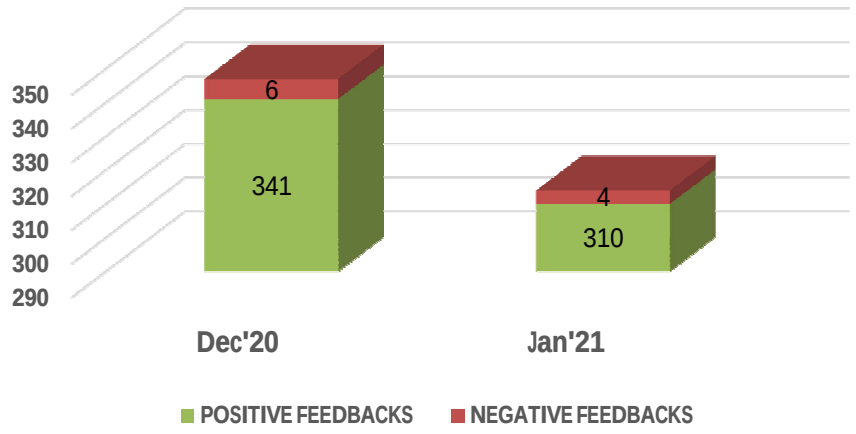

Month	Dec'20	Jan'21	Total
NEGATIVE FEEDBACKS	6	4	10
POSITIVE FEEDBACKS	341	310	651
TOTAL FEEDBACKS	347	314	661

Trend in Positive & Negative Feedbacks Percentage

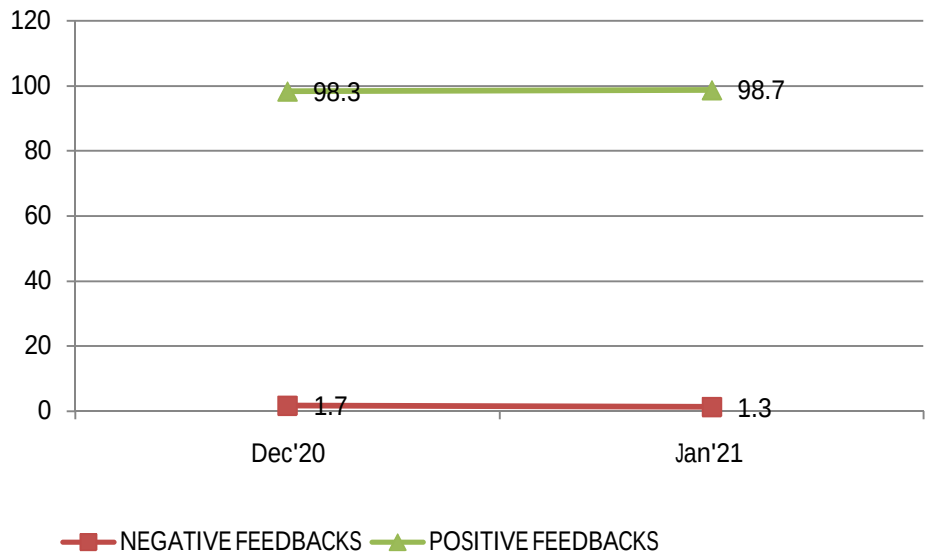

***Source**: V. Pranaya Theja, Network Engineer, SVIMS*

Old Standard Paper Based Feedback Collection: Year Wise Feedback Data : 2014-2020

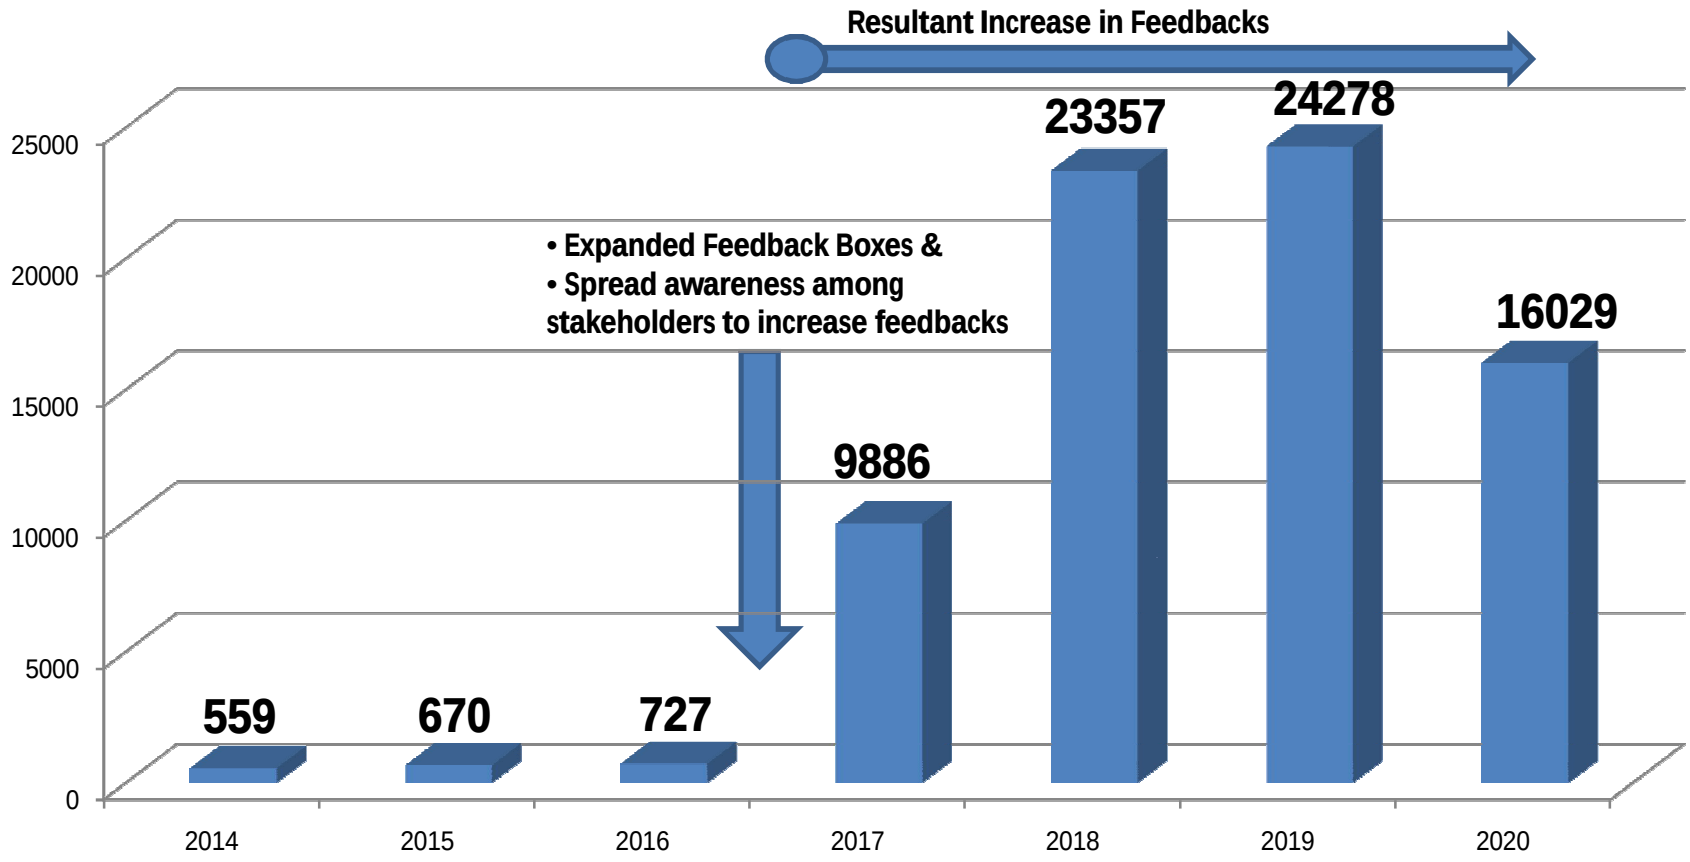

Year	2014	2015	2016	2017	2018	2019	2020
Feedbacks	559	670	727	9886	23357	24278	16029

***Source**: Dept. Of MSW, SVIMS*

Thank You.!!

MORTALITY

SVIMS instituted mortality reduction & quality improvement strategies along a novel strategy of "Multiple Sequential Wedges of improvement". Each set of quality improvements is introduced every 6 months & effects measured. These '6 month spells' of average mortality rate are represented in the Table.

Mortality rate - Jan'2020 to Dec''2020							
	Discharges						
		Expired					
Month & Year	Alive	Under 48 hrs	Over 48 hrs	Total	Total	NDR	GDR
Jan-20	3743	83	97	180	3923	2.53	4.59
Feb-20	3711	107	103	210	3921	2.70	5.36
Mar-20	3607	103	98	201	3808	2.65	5.28
Apr-20	1808	70	67	137	1945	3.57	7.04
May-20	1668	70	68	138	1806	3.92	7.64
Jun-20	2610	92	77	169	2779	2.87	6.08
Jul-20	2715	145	129	274	2989	4.54	9.17
Aug-20	2370	176	177	353	2723	6.95	12.96
Sep-20	2756	137	165	302	3058	5.65	9.88
Oct-20	3015	114	162	276	3291	5.10	8.39
Nov-20	2685	81	121	202	2887	4.31	7.00
Dec-20	2944	97	95	192	3136	3.13	6.12
Total	**33632**	**1275**	**1359**	**2634**	**36266**	**3.88**	**7.26**